

Data Path : Z:\voasrv\HPCHEM1\MSVOA\_X\Data\VX102022\  
Data File : VX032253.D  
Acq On : 20 Oct 2022 11:24  
Operator : JC/MD  
Sample : VX1020MBL01  
Misc : 5.00g/10mL/100uL/5.00mL/MSVOA\_X/MEOH  
ALS Vial : 3 Sample Multiplier: 1

Instrument :  
MSVOA\_X  
ClientSampleId :  
VX1020MBL01

Integration Parameters: RTEINT.P

Integrator: RTE

Smoothing : ON

Filtering: 5

Sampling : 1

Min Area: 3 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA\_X\Method\82X101922W.M

Title : SW846 8260

Signal : TIC: VX032253.D\data.ms

| peak<br># | R.T.<br>min | first<br>scan | max<br>scan | last<br>scan | PK<br>TY | peak<br>height | corr.<br>area | corr.<br>% max. | % of<br>total |
|-----------|-------------|---------------|-------------|--------------|----------|----------------|---------------|-----------------|---------------|
| 1         | 5.379       | 693           | 704         | 717          | rBV      | 108548         | 317970        | 33.71%          | 6.341%        |
| 2         | 5.544       | 721           | 731         | 750          | rVB      | 201614         | 569764        | 60.40%          | 11.363%       |
| 3         | 5.952       | 788           | 798         | 811          | rBV      | 121667         | 324516        | 34.40%          | 6.472%        |
| 4         | 6.757       | 919           | 930         | 947          | rBV      | 287122         | 688680        | 73.00%          | 13.734%       |
| 5         | 8.647       | 1233          | 1240        | 1251         | rBV      | 618937         | 943341        | 100.00%         | 18.813%       |
| 6         | 10.055      | 1465          | 1471        | 1483         | rBV      | 578542         | 782957        | 83.00%          | 15.614%       |
| 7         | 11.079      | 1634          | 1639        | 1648         | rBV      | 518795         | 638352        | 67.67%          | 12.730%       |
| 8         | 12.024      | 1788          | 1794        | 1804         | rBV      | 592310         | 748778        | 79.38%          | 14.933%       |




Sum of corrected areas: 5014358

Data Path : Z:\voasrv\HPCHEM1\MSVOA\_X\Data\VX102022\  
Data File : VX032253.D  
Acq On : 20 Oct 2022 11:24  
Operator : JC/MD  
Sample : VX1020MBL01  
Misc : 5.00g/10mL/100uL/5.00mL/MSVOA\_X/MEOH  
ALS Vial : 3 Sample Multiplier: 1

Instrument :  
MSVOA\_X  
ClientSampleId :  
VX1020MBL01

Quant Method : Z:\voasrv\HPCHEM1\MSVOA\_X\Method\82X101922W.M  
Quant Title : SW846 8260

TIC Library : C:\Database\NIST20.L  
TIC Integration Parameters: LSCINT.P

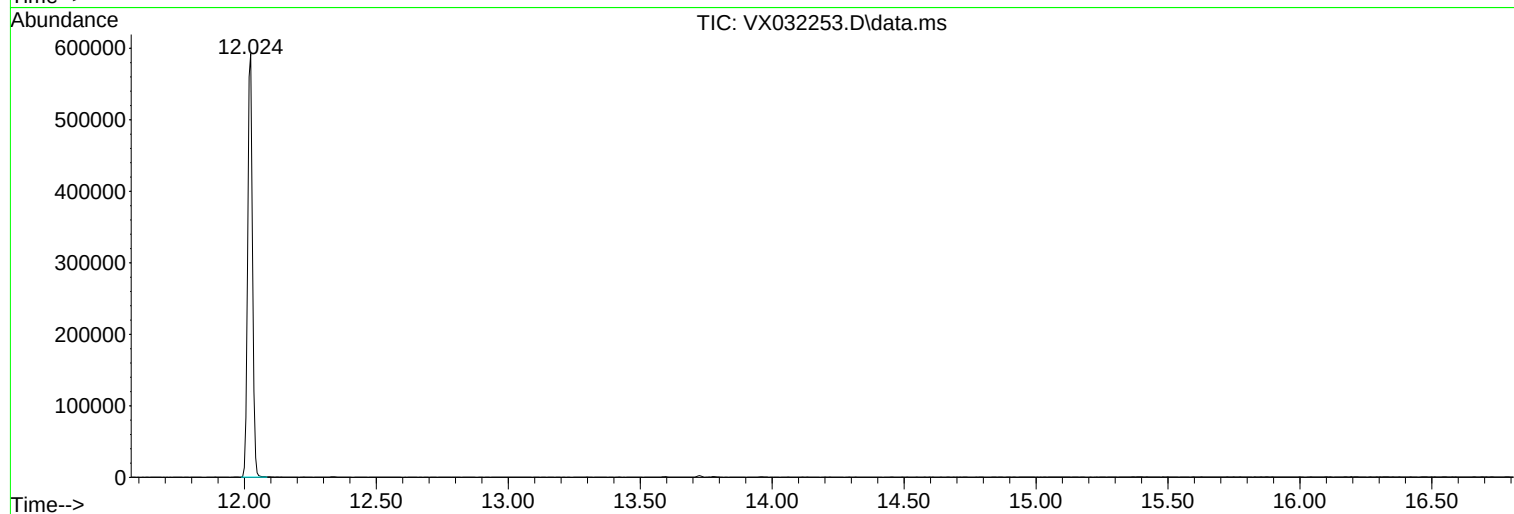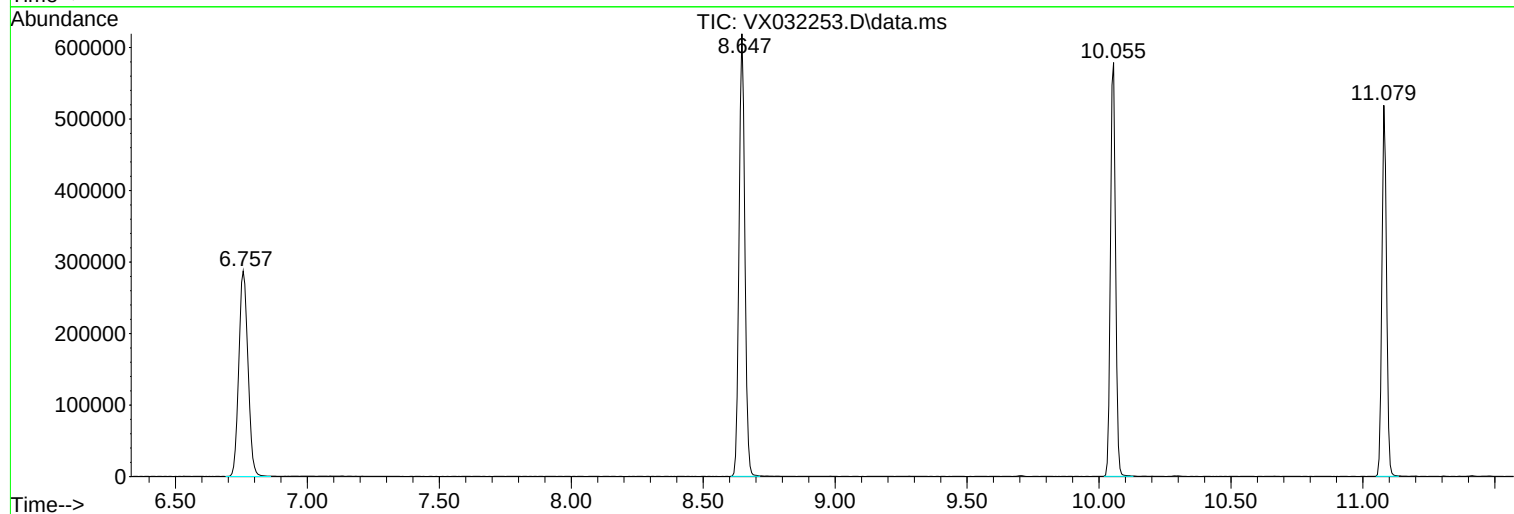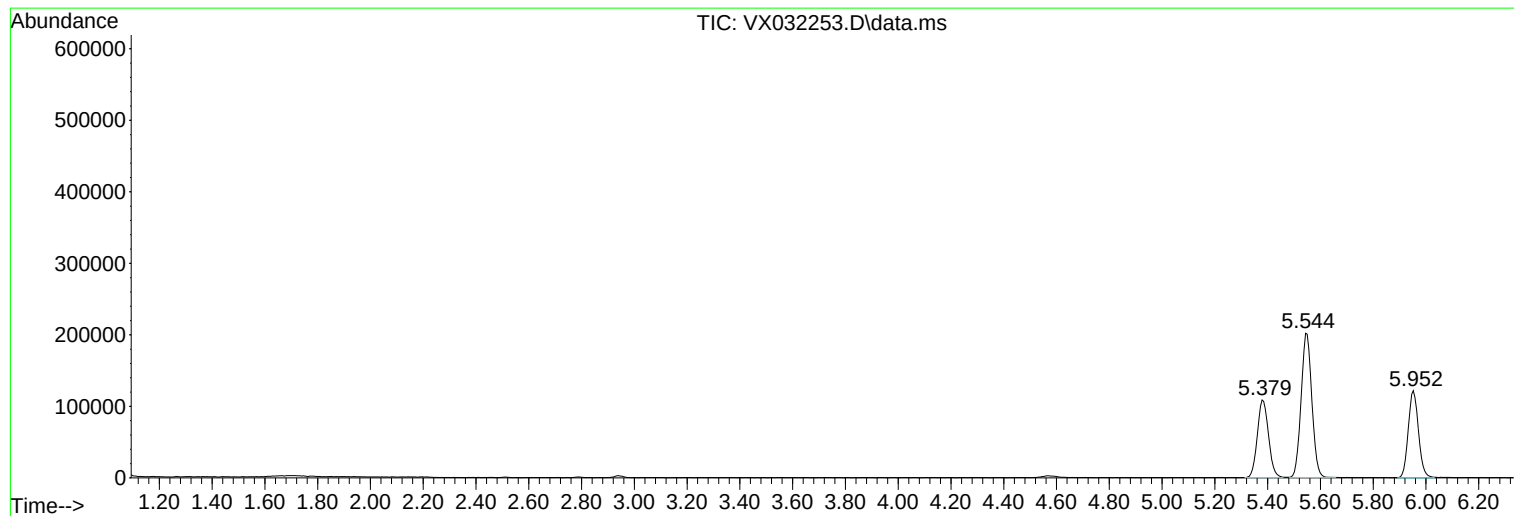

Data Path : Z:\voasrv\HPCHEM1\MSVOA\_X\Data\VX102022\  
Data File : VX032253.D  
Acq On : 20 Oct 2022 11:24  
Operator : JC/MD  
Sample : VX1020MBL01  
Misc : 5.00g/10mL/100uL/5.00mL/MSVOA\_X/MEOH  
ALS Vial : 3 Sample Multiplier: 1

Instrument :  
MSVOA\_X  
ClientSampleId :  
VX1020MBL01

Quant Method : Z:\voasrv\HPCHEM1\MSVOA\_X\Method\82X101922W.M  
Quant Title : SW846 8260

TIC Library : C:\Database\NIST20.L  
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

\*\*\*\*\*

Data Path : Z:\voasrv\HPCHEM1\MSVOA\_X\Data\VX102022\  
Data File : VX032253.D  
Acq On : 20 Oct 2022 11:24  
Operator : JC/MD  
Sample : VX1020MBL01  
Misc : 5.00g/10mL/100uL/5.00mL/MSVOA\_X/MEOH  
ALS Vial : 3 Sample Multiplier: 1

Instrument :  
MSVOA\_X  
ClientSampleId :  
VX1020MBL01

Quant Method : Z:\voasrv\HPCHEM1\MSVOA\_X\Method\82X101922W.M  
Quant Title : SW846 8260

TIC Library : C:\Database\NIST20.L  
TIC Integration Parameters: LSCINT.P

| TIC Top Hit name | RT | EstConc | Units | Response | --Internal Standard-- |    |      |      |
|------------------|----|---------|-------|----------|-----------------------|----|------|------|
|                  |    |         |       |          | #                     | RT | Resp | Conc |