
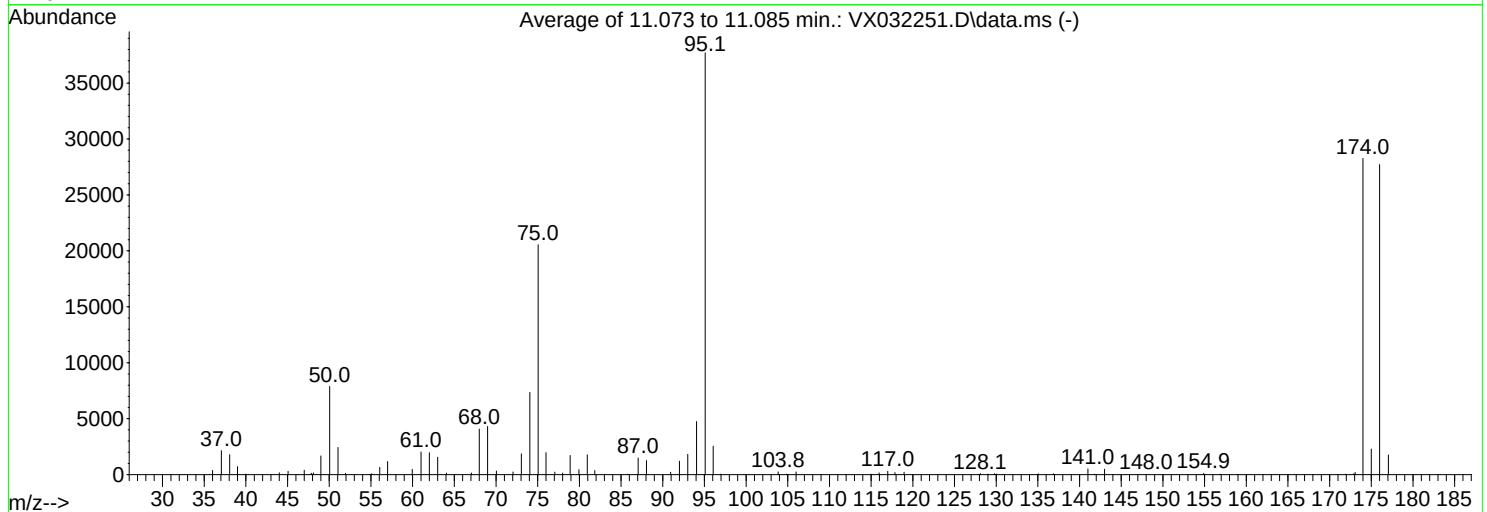


Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX102022\
 Data File : VX032251.D
 Acq On : 20 Oct 2022 09:41
 Operator : JC/MD
 Sample : BFB
 Misc : 5.0mL/MSVOA_X/WATER
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_X
 ClientSampleId :
 BFB

Integration File: RTEINT.P

Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\82X101922W.M
 Title : SW846 8260
 Last Update : Wed Oct 19 16:51:09 2022

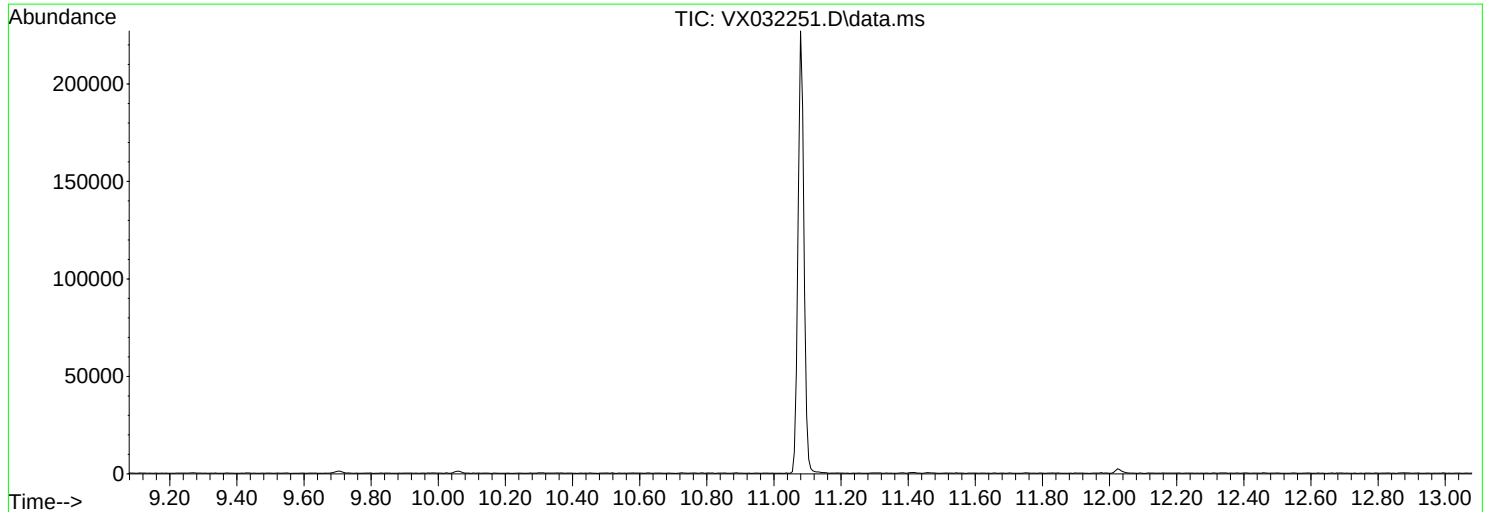

AutoFind: Scans 1638, 1639, 1640; Background Corrected with Scan 1632

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	15	40	20.9	7884	PASS
75	95	30	60	54.5	20544	PASS
95	95	100	100	100.0	37699	PASS
96	95	5	9	6.8	2547	PASS
173	174	0.00	2	0.7	196	PASS
174	95	50	100	75.0	28261	PASS
175	174	5	9	8.1	2291	PASS
176	174	95	101	98.1	27712	PASS
177	176	5	9	6.3	1755	PASS