

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX102023\
 Data File : VX038392.D
 Acq On : 20 Oct 2023 10:06
 Operator : JC/MD
 Sample : VX1020MBL01
 Misc : 5.00g/10mL/100uL/5.00mL/MSVOA_X/MEOH
 ALS Vial : 3 Sample Multiplier: 1

Instrument :
 MSVOA_X
 ClientSampleId :
 VX1020MBL01

Quant Time: Oct 21 01:25:35 2023
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\82X100523W.M
 Quant Title : SW846 8260
 QLast Update : Thu Oct 05 15:27:13 2023
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)

Internal Standards						
1) Pentafluorobenzene	5.550	168	124891	50.000	ug/l	0.00
34) 1,4-Difluorobenzene	6.763	114	220393	50.000	ug/l	0.00
63) Chlorobenzene-d5	10.055	117	222265	50.000	ug/l	0.00
72) 1,4-Dichlorobenzene-d4	12.024	152	112530	50.000	ug/l	0.00

System Monitoring Compounds						
33) 1,2-Dichloroethane-d4	5.958	65	88454	44.033	ug/l	0.00
Spiked Amount	50.000	Range	78 - 117	Recovery	=	88.060%
35) Dibromofluoromethane	5.379	113	71492	45.018	ug/l	0.00
Spiked Amount	50.000	Range	75 - 124	Recovery	=	90.040%
50) Toluene-d8	8.647	98	276826	45.618	ug/l	0.00
Spiked Amount	50.000	Range	92 - 112	Recovery	=	91.240%#
62) 4-Bromofluorobenzene	11.079	95	103323	44.911	ug/l	0.00
Spiked Amount	50.000	Range	83 - 123	Recovery	=	89.820%


Target Compounds	Qvalue

(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX102023\
Data File : VX038392.D
Acq On : 20 Oct 2023 10:06
Operator : JC/MD
Sample : VX1020MBL01
Misc : 5.00g/10mL/100uL/5.00mL/MSVOA_X/MEOH
ALS Vial : 3 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
VX1020MBL01

Quant Time: Oct 21 01:25:35 2023
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\82X100523W.M
Quant Title : SW846 8260
QLast Update : Thu Oct 05 15:27:13 2023
Response via : Initial Calibration




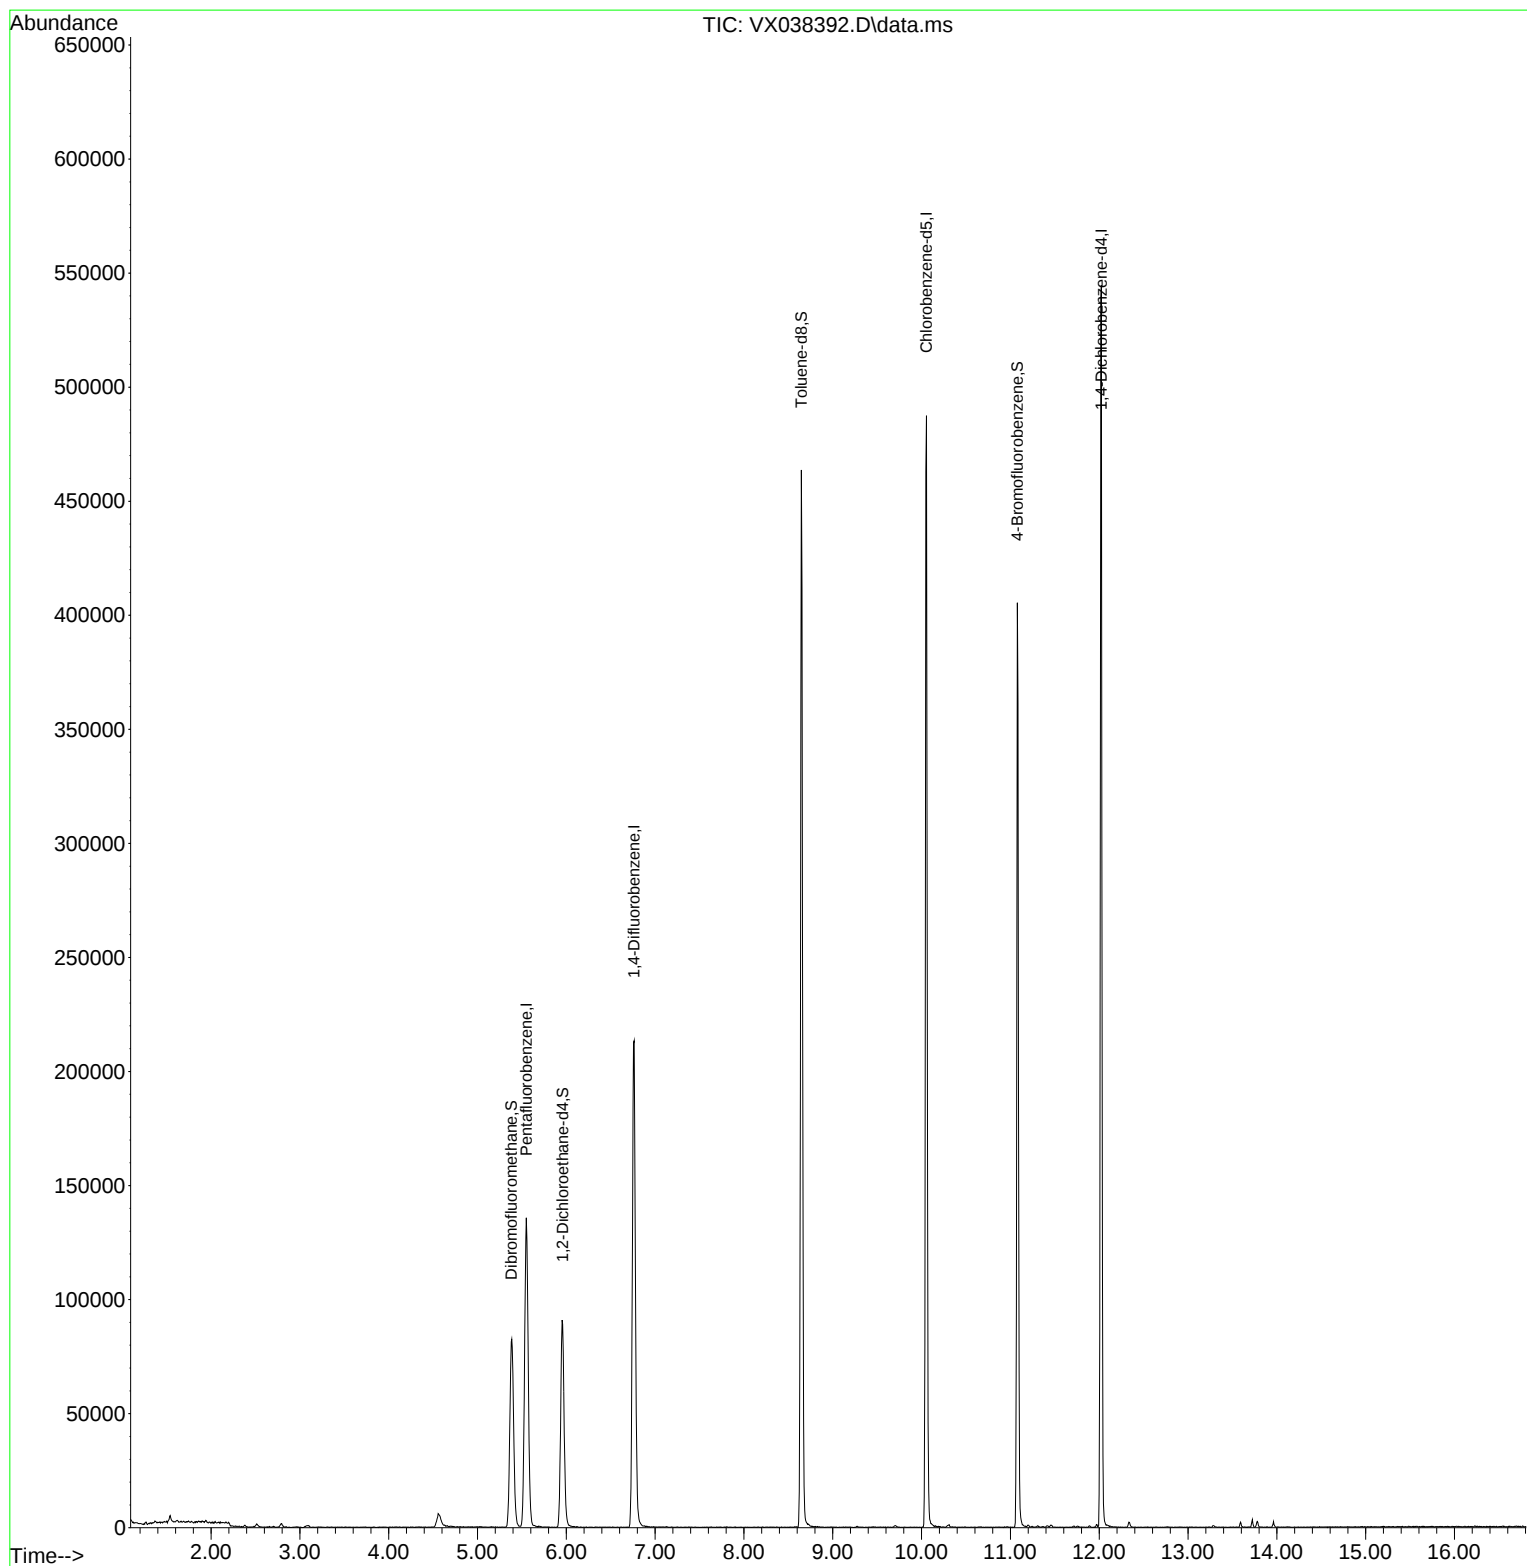




#1
Pentafluorobenzene
Concen: 50.000 ug/l
RT: 5.550 min Scan# 71
Delta R.T. -0.006 min
Lab File: VX038392.D
Acq: 20 Oct 2023 10:06




Instrument :
MSVOA_X
ClientSampleId :
VX1020MBL01


Tgt Ion:168 Resp: 124891
Ion Ratio Lower Upper
168 100
99 56.7 56.6 85.0

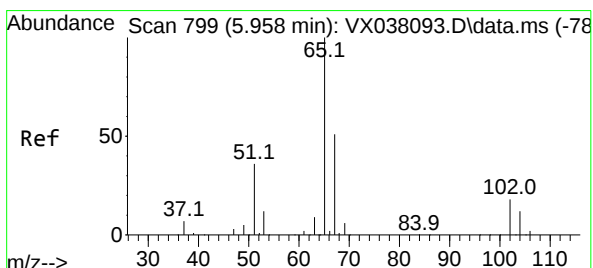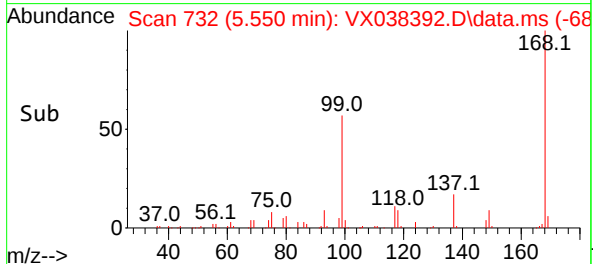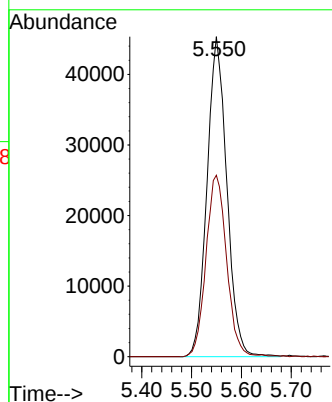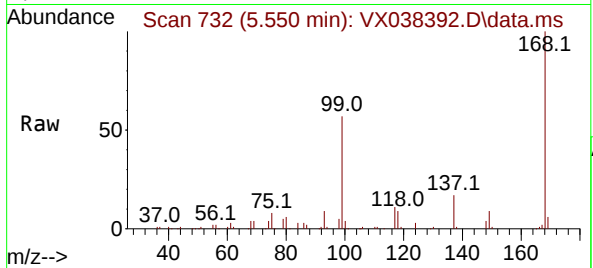

#33
1,2-Dichloroethane-d4
Concen: 44.033 ug/l
RT: 5.958 min Scan# 799
Delta R.T. 0.000 min
Lab File: VX038392.D
Acq: 20 Oct 2023 10:06

Tgt Ion: 65 Resp: 88454
Ion Ratio Lower Upper
65 100
67 52.4 0.0 100.2


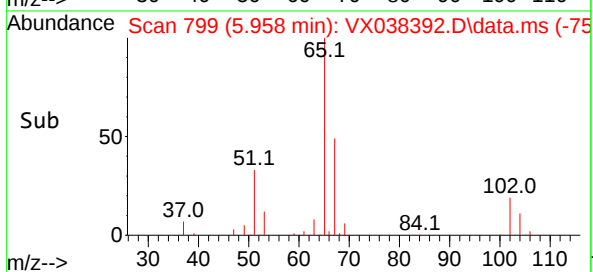
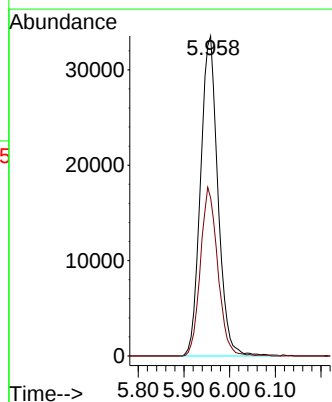
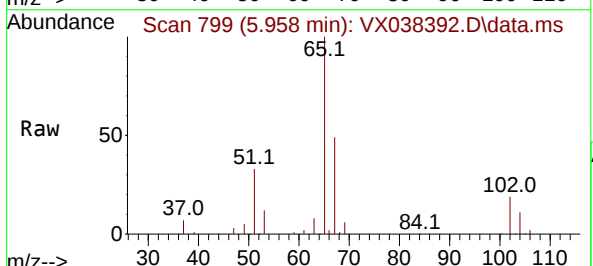


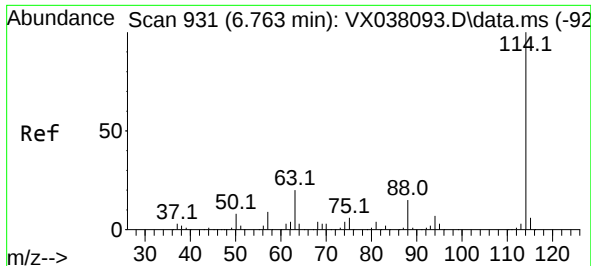

#34
1,4-Difluorobenzene
Concen: 50.000 ug/l
RT: 6.763 min Scan# 91
Delta R.T. -0.000 min
Lab File: VX038392.D
Acq: 20 Oct 2023 10:06




Instrument :
MSVOA_X
ClientSampleId :
VX1020MBL01


Tgt Ion:114 Resp: 220393
Ion Ratio Lower Upper
114 100
63 19.6 0.0 45.0
88 15.5 0.0 36.6

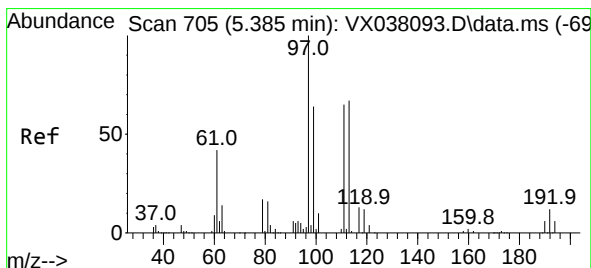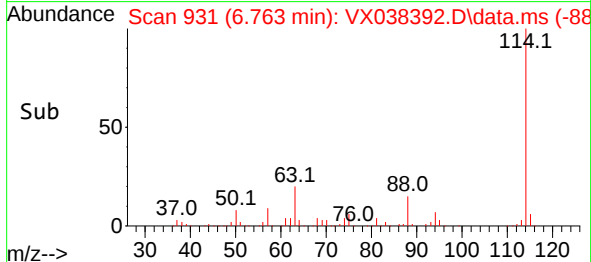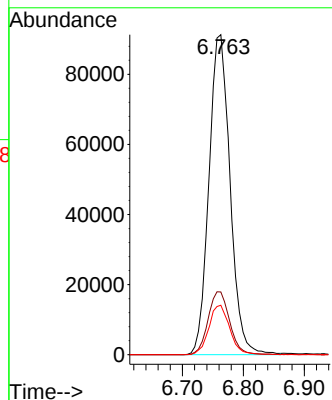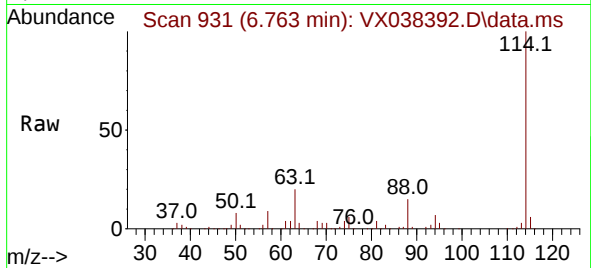

#35
Dibromofluoromethane
Concen: 45.018 ug/l
RT: 5.379 min Scan# 704
Delta R.T. -0.006 min
Lab File: VX038392.D
Acq: 20 Oct 2023 10:06

Tgt Ion:113 Resp: 71492
Ion Ratio Lower Upper
113 100
111 104.6 82.9 124.3
192 18.4 13.3 19.9


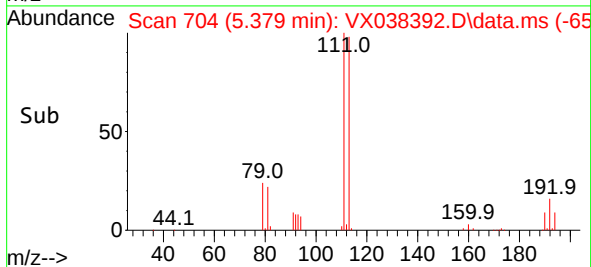
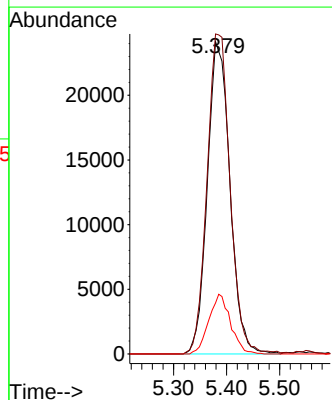
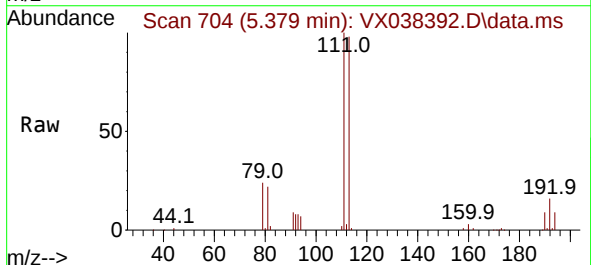


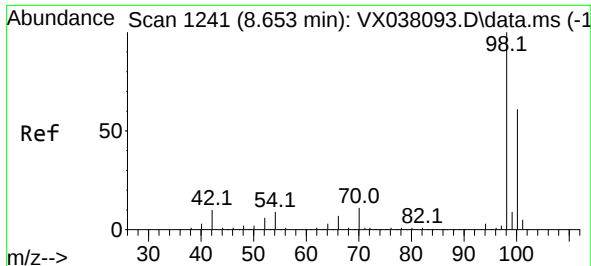

#50
Toluene-d8
Concen: 45.618 ug/l
RT: 8.647 min Scan# 11
Delta R.T. -0.006 min
Lab File: VX038392.D
Acq: 20 Oct 2023 10:06




Instrument :
MSVOA_X
ClientSampleId :
VX1020MBL01


Tgt Ion: 98 Resp: 276826
Ion Ratio Lower Upper
98 100
100 63.9 53.1 79.7

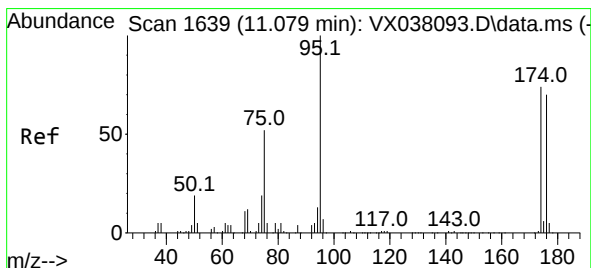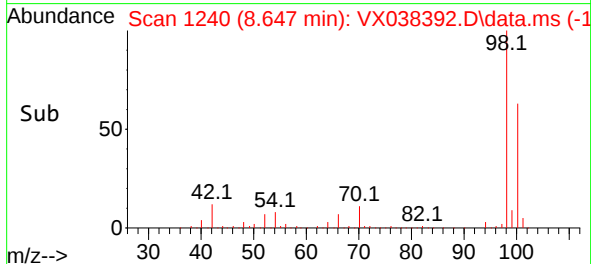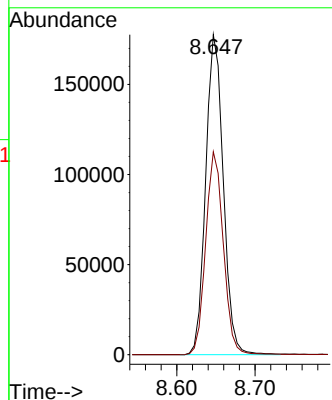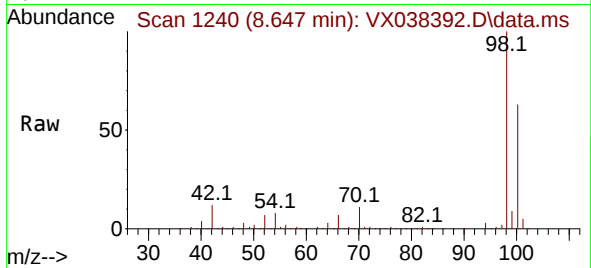

#62
4-Bromofluorobenzene
Concen: 44.911 ug/l
RT: 11.079 min Scan# 1639
Delta R.T. 0.000 min
Lab File: VX038392.D
Acq: 20 Oct 2023 10:06

Tgt Ion: 95 Resp: 103323
Ion Ratio Lower Upper
95 100
174 81.5 0.0 135.6
176 78.6 0.0 131.0


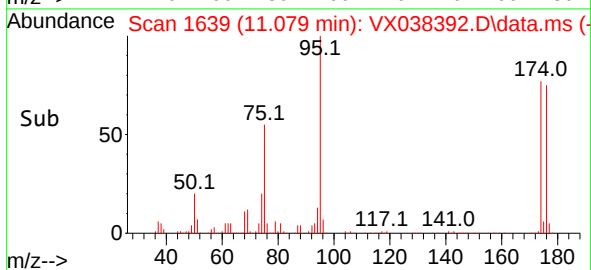
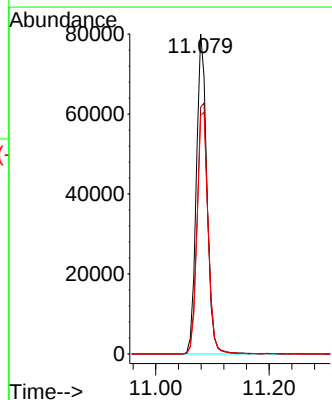
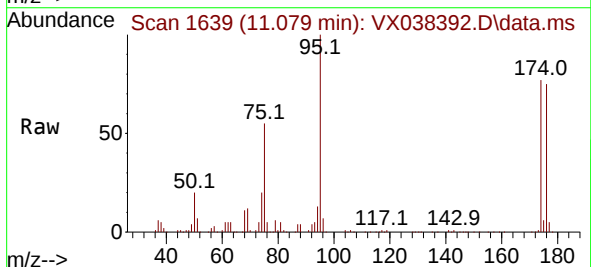


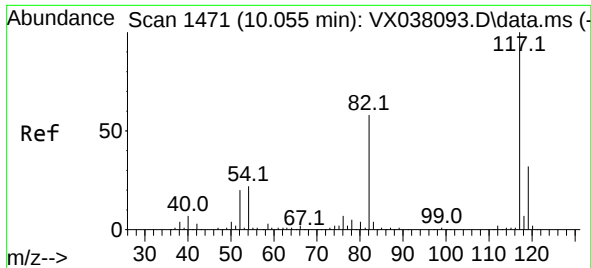

#63
Chlorobenzene-d5
Concen: 50.000 ug/l
RT: 10.055 min Scan# 1471
Delta R.T. -0.000 min
Lab File: VX038392.D
Acq: 20 Oct 2023 10:06

Instrument :
MSVOA_X
ClientSampleId :
VX1020MBL01

Tgt Ion:117 Resp: 222265
Ion Ratio Lower Upper
117 100
82 55.4 46.2 69.4
119 32.8 25.5 38.3

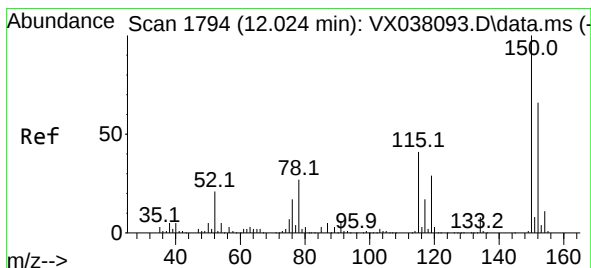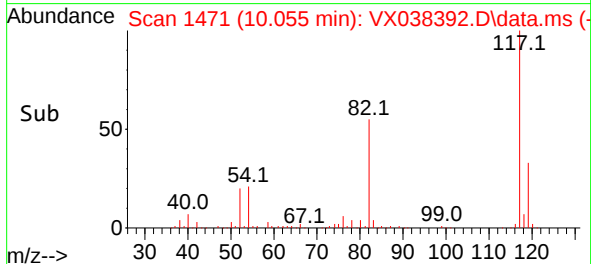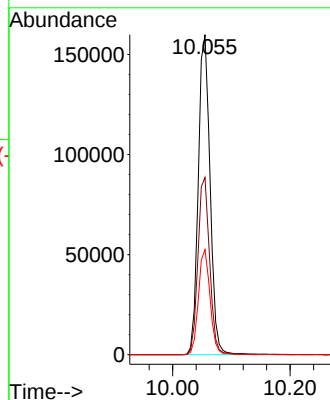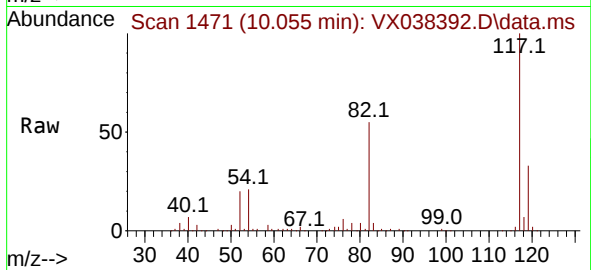

#72
1,4-Dichlorobenzene-d4
Concen: 50.000 ug/l
RT: 12.024 min Scan# 1794
Delta R.T. 0.000 min
Lab File: VX038392.D
Acq: 20 Oct 2023 10:06

Tgt Ion:152 Resp: 112530
Ion Ratio Lower Upper
152 100
115 61.2 43.3 129.9
150 156.5 0.0 345.0

