

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX102023\
 Data File : VX038412.D
 Acq On : 20 Oct 2023 18:58
 Operator : JC/MD
 Sample : 04987-04
 Misc : 5.0mL/MSVOA_X/WATER
 ALS Vial : 23 Sample Multiplier: 1

Instrument :
 MSVOA_X
 ClientSampleId :
 STORAGE-BLANK-SAMPLE-MANAG

Quant Time: Oct 21 01:49:44 2023
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\82X100523W.M
 Quant Title : SW846 8260
 QLast Update : Thu Oct 05 15:27:13 2023
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)

Internal Standards						
1) Pentafluorobenzene	5.550	168	122727	50.000	ug/l	# 0.00
34) 1,4-Difluorobenzene	6.763	114	219049	50.000	ug/l	0.00
63) Chlorobenzene-d5	10.055	117	219492	50.000	ug/l	0.00
72) 1,4-Dichlorobenzene-d4	12.024	152	113751	50.000	ug/l	0.00
System Monitoring Compounds						
33) 1,2-Dichloroethane-d4	5.952	65	87150	44.149	ug/l	0.00
Spiked Amount	50.000	Range	78 - 117	Recovery	=	88.300%
35) Dibromofluoromethane	5.385	113	71603	45.365	ug/l	0.00
Spiked Amount	50.000	Range	75 - 124	Recovery	=	90.720%
50) Toluene-d8	8.647	98	269842	44.739	ug/l	0.00
Spiked Amount	50.000	Range	92 - 112	Recovery	=	89.480%#
62) 4-Bromofluorobenzene	11.079	95	102547	44.848	ug/l	0.00
Spiked Amount	50.000	Range	83 - 123	Recovery	=	89.700%


Target Compounds Qvalue


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX102023\
Data File : VX038412.D
Acq On : 20 Oct 2023 18:58
Operator : JC/MD
Sample : 04987-04
Misc : 5.0mL/MSVOA_X/WATER
ALS Vial : 23 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
STORAGE-BLANK-SAMPLE-MANAG

Quant Time: Oct 21 01:49:44 2023
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\82X100523W.M
Quant Title : SW846 8260
QLast Update : Thu Oct 05 15:27:13 2023
Response via : Initial Calibration




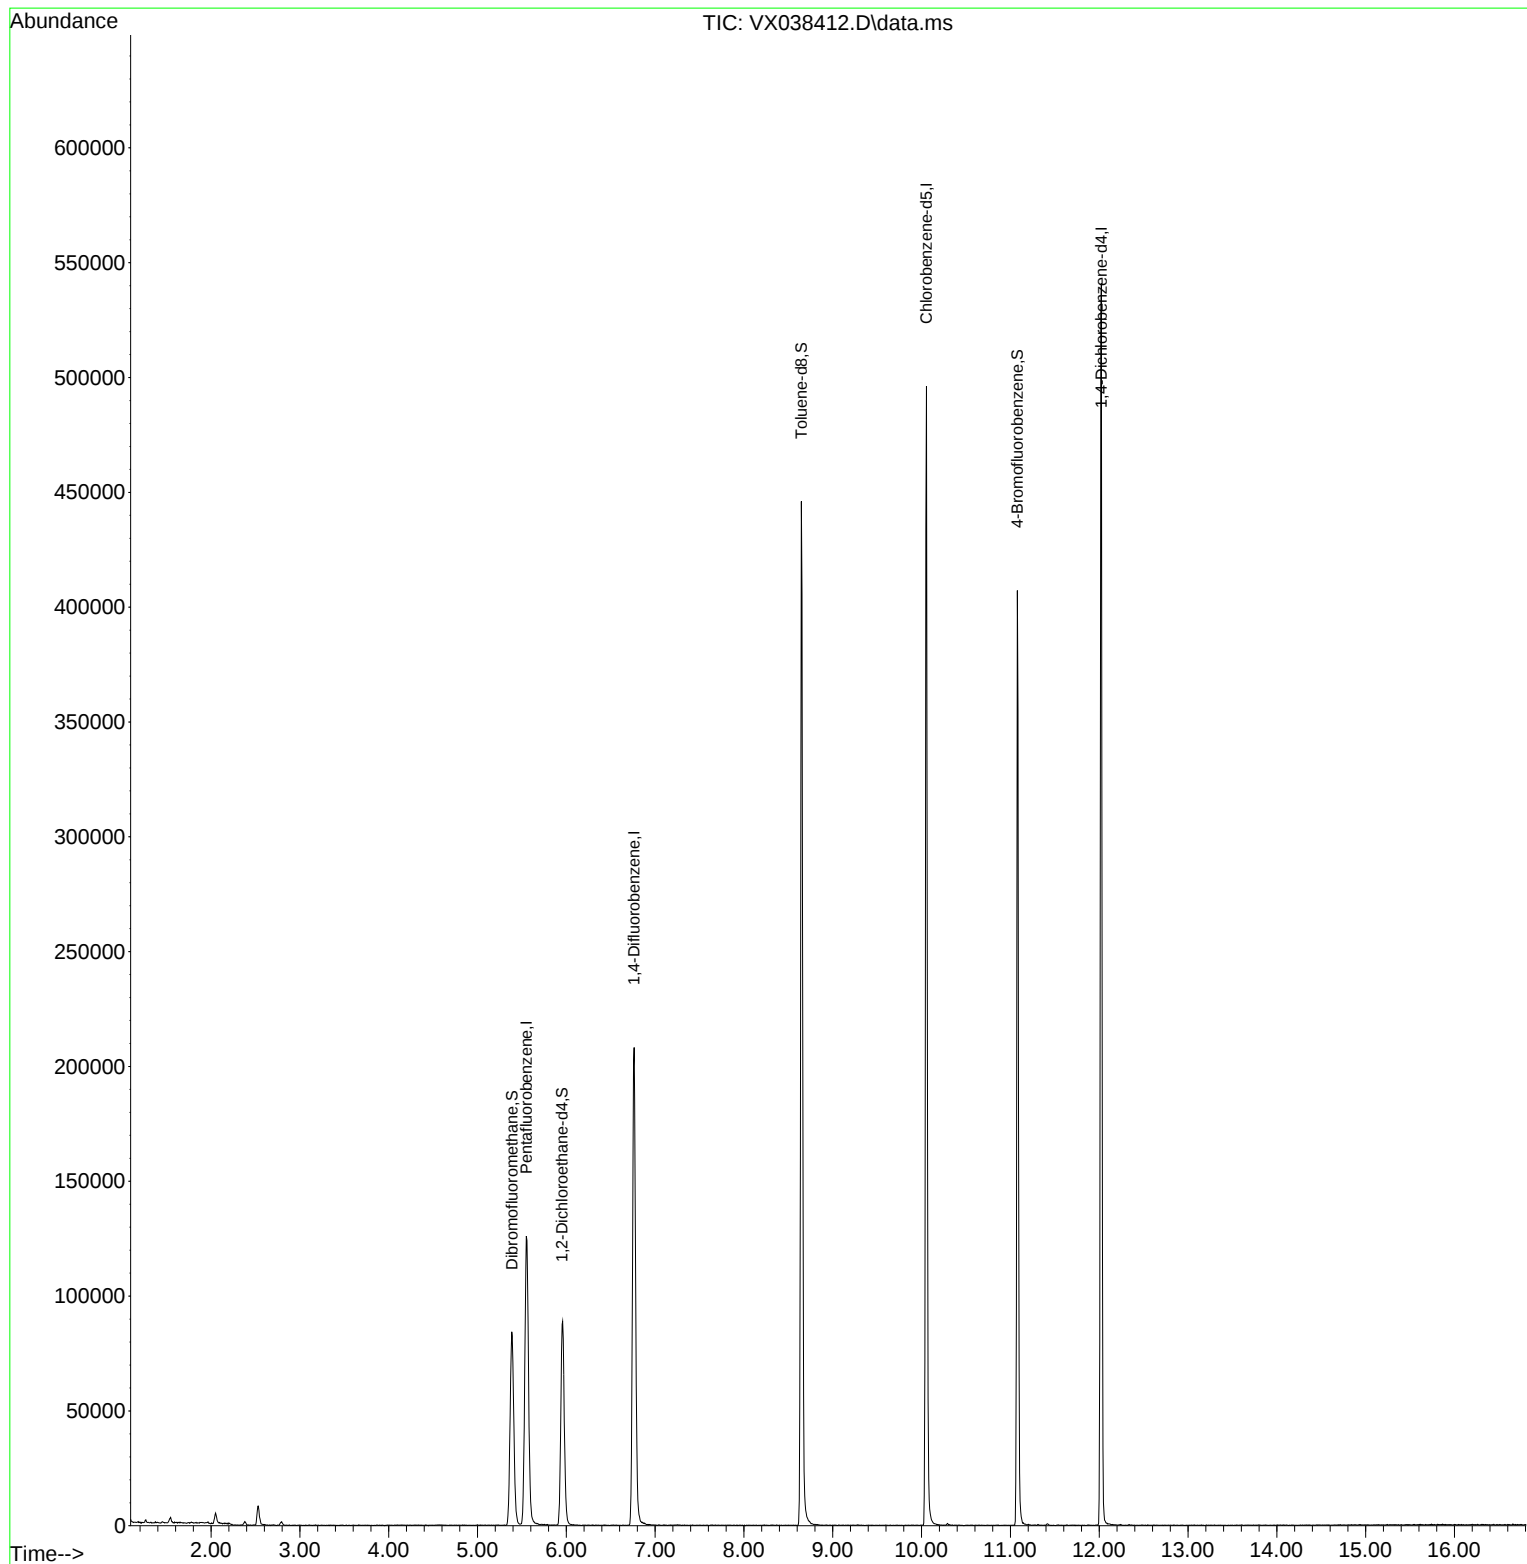


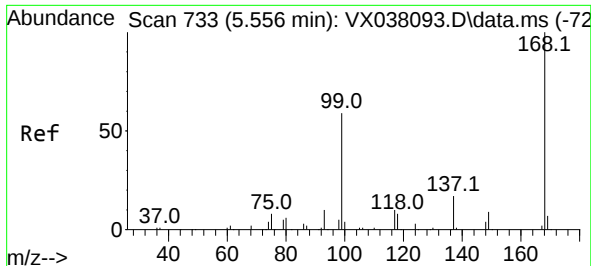

#1
Pentafluorobenzene
Concen: 50.000 ug/l
RT: 5.550 min Scan# 71
Delta R.T. -0.006 min
Lab File: VX038412.D
Acq: 20 Oct 2023 18:58




Instrument :
MSVOA_X
ClientSampleId :
STORAGE-BLANK-SAMPLE-MANAG


Tgt Ion:168 Resp: 122727
Ion Ratio Lower Upper
168 100
99 53.9 56.6 85.0#

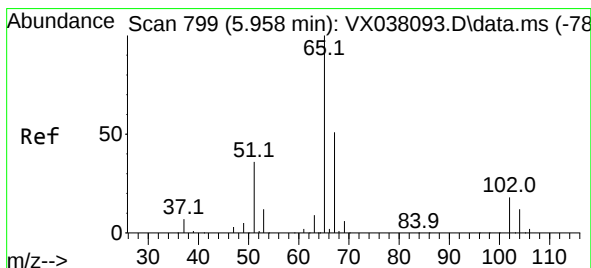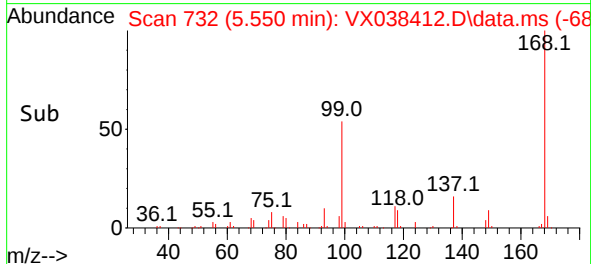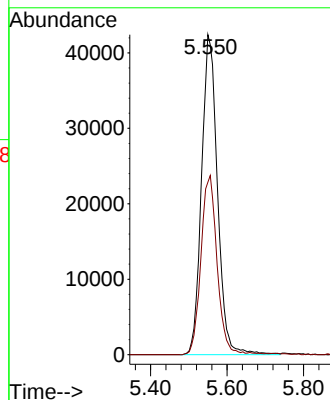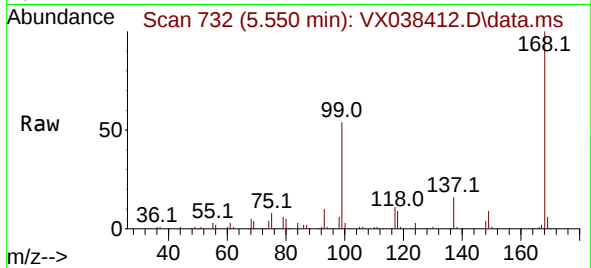

#33
1,2-Dichloroethane-d4
Concen: 44.149 ug/l
RT: 5.952 min Scan# 798
Delta R.T. -0.006 min
Lab File: VX038412.D
Acq: 20 Oct 2023 18:58

Tgt Ion: 65 Resp: 87150
Ion Ratio Lower Upper
65 100
67 52.4 0.0 100.2


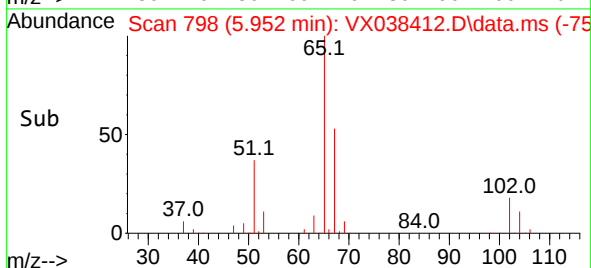
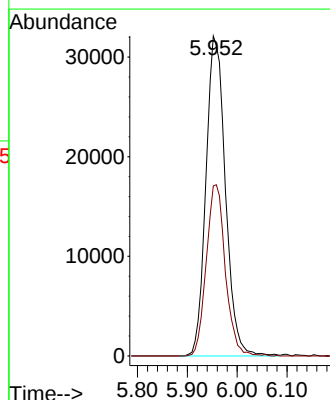
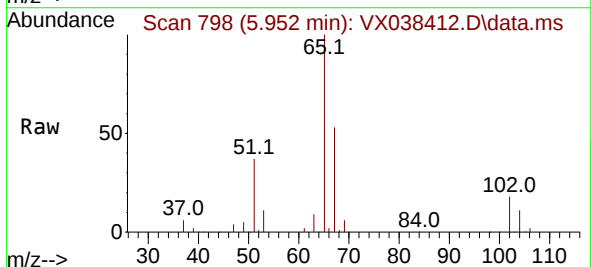


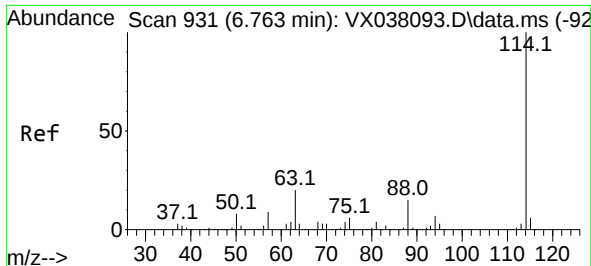

#34
1,4-Difluorobenzene
Concen: 50.000 ug/l
RT: 6.763 min Scan# 91
Delta R.T. -0.000 min
Lab File: VX038412.D
Acq: 20 Oct 2023 18:58




Instrument :
MSVOA_X
ClientSampleId :
STORAGE-BLANK-SAMPLE-MANAG


Tgt Ion:114 Resp: 219049
Ion Ratio Lower Upper
114 100
63 19.5 0.0 45.0
88 14.9 0.0 36.6

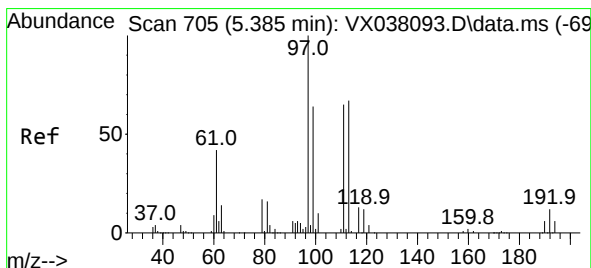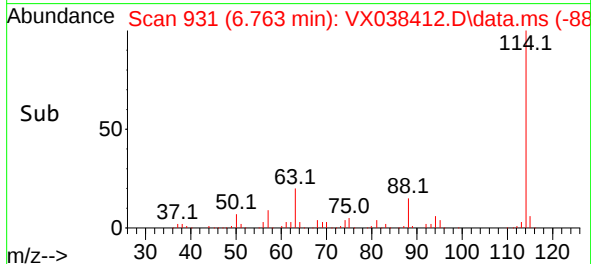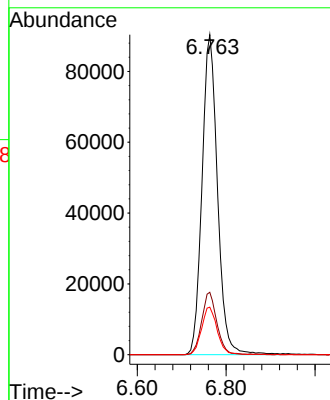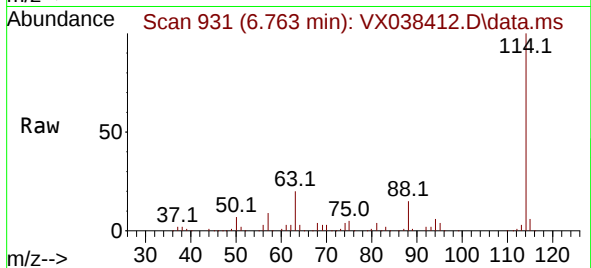

#35
Dibromofluoromethane
Concen: 45.365 ug/l
RT: 5.385 min Scan# 705
Delta R.T. 0.000 min
Lab File: VX038412.D
Acq: 20 Oct 2023 18:58

Tgt Ion:113 Resp: 71603
Ion Ratio Lower Upper
113 100
111 103.3 82.9 124.3
192 18.7 13.3 19.9


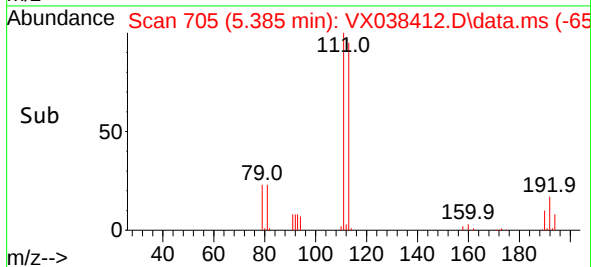
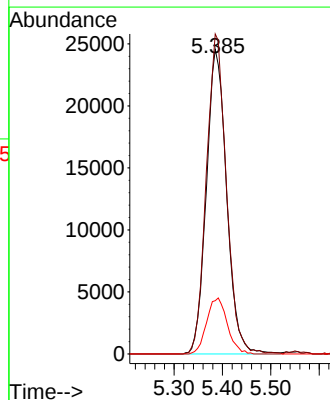
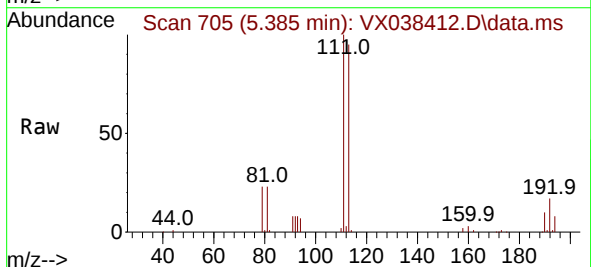


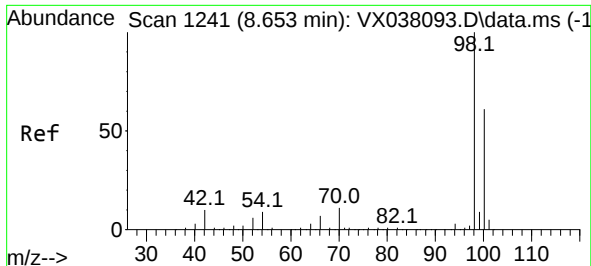

#50
Toluene-d8
Concen: 44.739 ug/l
RT: 8.647 min Scan# 11
Delta R.T. -0.006 min
Lab File: VX038412.D
Acq: 20 Oct 2023 18:58




Instrument :
MSVOA_X
ClientSampleId :
STORAGE-BLANK-SAMPLE-MANAG


Tgt Ion: 98 Resp: 269842
Ion Ratio Lower Upper
98 100
100 63.7 53.1 79.7

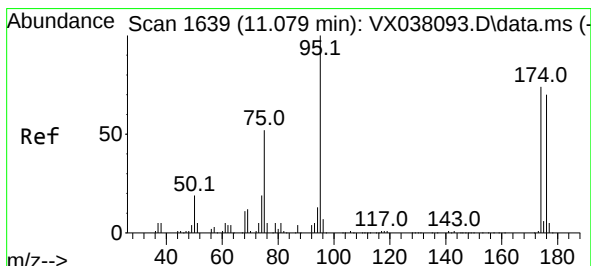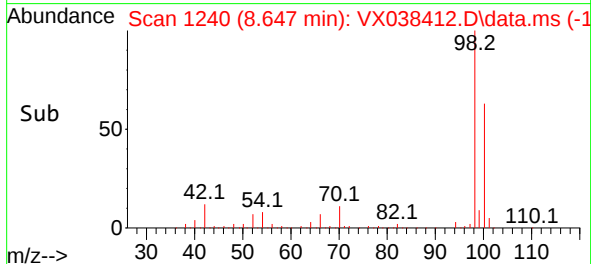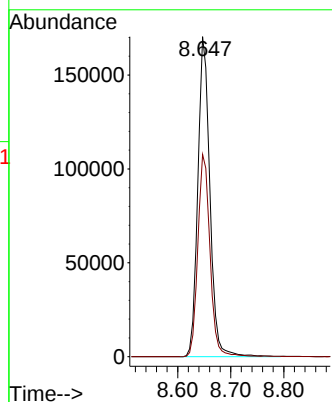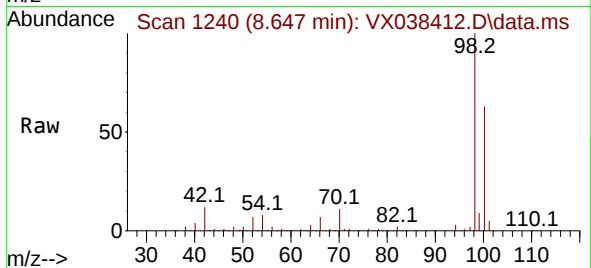

#62
4-Bromofluorobenzene
Concen: 44.848 ug/l
RT: 11.079 min Scan# 1639
Delta R.T. 0.000 min
Lab File: VX038412.D
Acq: 20 Oct 2023 18:58

Tgt Ion: 95 Resp: 102547
Ion Ratio Lower Upper
95 100
174 82.6 0.0 135.6
176 78.6 0.0 131.0


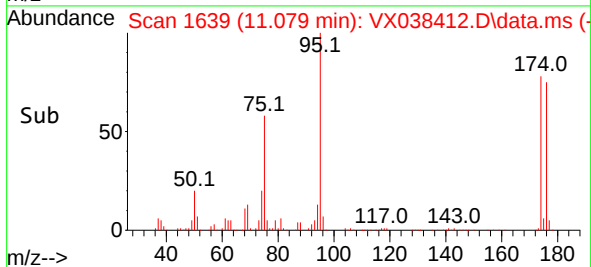
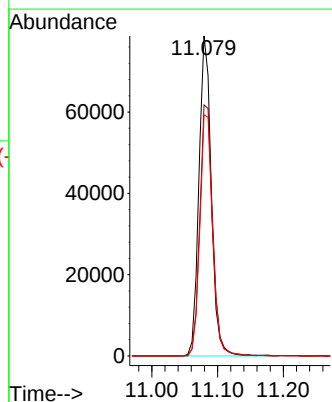
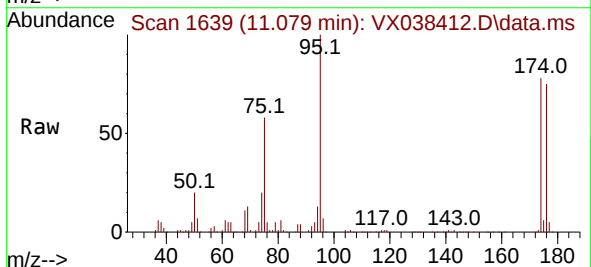


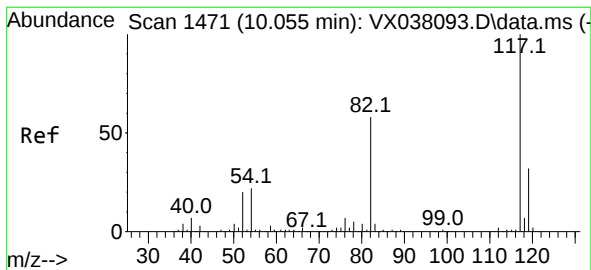

#63
Chlorobenzene-d5
Concen: 50.000 ug/l
RT: 10.055 min Scan# 1471
Delta R.T. 0.000 min
Lab File: VX038412.D
Acq: 20 Oct 2023 18:58

Instrument :
MSVOA_X
ClientSampleId :
STORAGE-BLANK-SAMPLE-MANAG

Tgt Ion:117 Resp: 219492
Ion Ratio Lower Upper
117 100
82 56.0 46.2 69.4
119 32.7 25.5 38.3

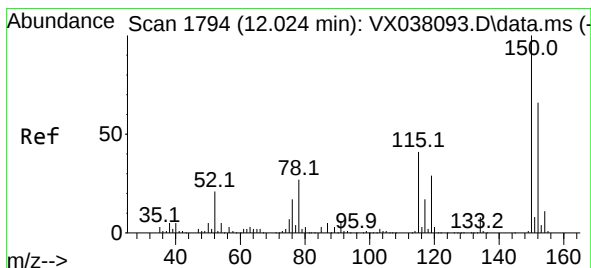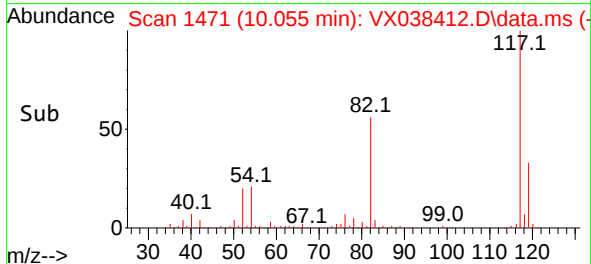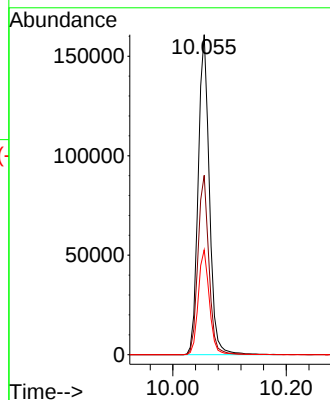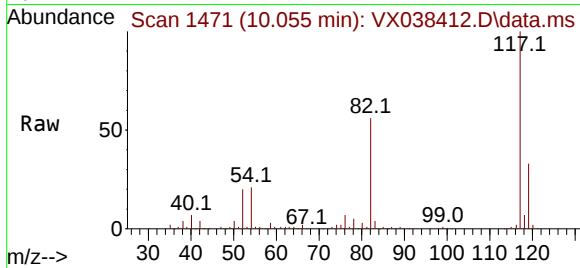

#72
1,4-Dichlorobenzene-d4
Concen: 50.000 ug/l
RT: 12.024 min Scan# 1794
Delta R.T. 0.000 min
Lab File: VX038412.D
Acq: 20 Oct 2023 18:58

Tgt Ion:152 Resp: 113751
Ion Ratio Lower Upper
152 100
115 60.0 43.3 129.9
150 156.9 0.0 345.0

