

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX102023\
 Data File : VX038404.D
 Acq On : 20 Oct 2023 15:53
 Operator : JC/MD
 Sample : 05003-01
 Misc : 5.0mL/MSVOA_X/WATER
 ALS Vial : 15 Sample Multiplier: 1

Instrument :
 MSVOA_X
 ClientSampleId :
 GWOW-BR-06-323-343-102023

Integration Parameters: RTEINT.P

Integrator: RTE

Smoothing : ON

Filtering: 5

Sampling : 1

Min Area: 3 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\82X100523W.M

Title : SW846 8260

Signal : TIC: VX038404.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	2.532	230	237	242	rBV2	6363	11458	1.59%	0.266%
2	5.385	692	705	721	rBV	82282	246021	34.05%	5.716%
3	5.556	722	733	745	rBV	127864	364083	50.40%	8.459%
4	5.958	790	799	813	rBV	90421	243566	33.71%	5.659%
5	6.763	922	931	948	rBV	211752	509139	70.48%	11.830%
6	8.647	1234	1240	1247	rBV	450216	720659	99.75%	16.744%
7	8.720	1247	1252	1264	rVB	158888	248382	34.38%	5.771%
8	10.055	1465	1471	1491	rBV	510902	689238	95.40%	16.014%
9	10.647	1564	1568	1576	rVB	5682	8168	1.13%	0.190%
10	11.079	1634	1639	1651	rBV	418704	540811	74.86%	12.565%
11	12.024	1788	1794	1809	rBV	552785	722438	100.00%	16.785%




Sum of corrected areas: 4303963

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX102023\
Data File : VX038404.D
Acq On : 20 Oct 2023 15:53
Operator : JC/MD
Sample : 05003-01
Misc : 5.0mL/MSVOA_X/WATER
ALS Vial : 15 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
GWOW-BR-06-323-343-102023

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\82X100523W.M
Quant Title : SW846 8260

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

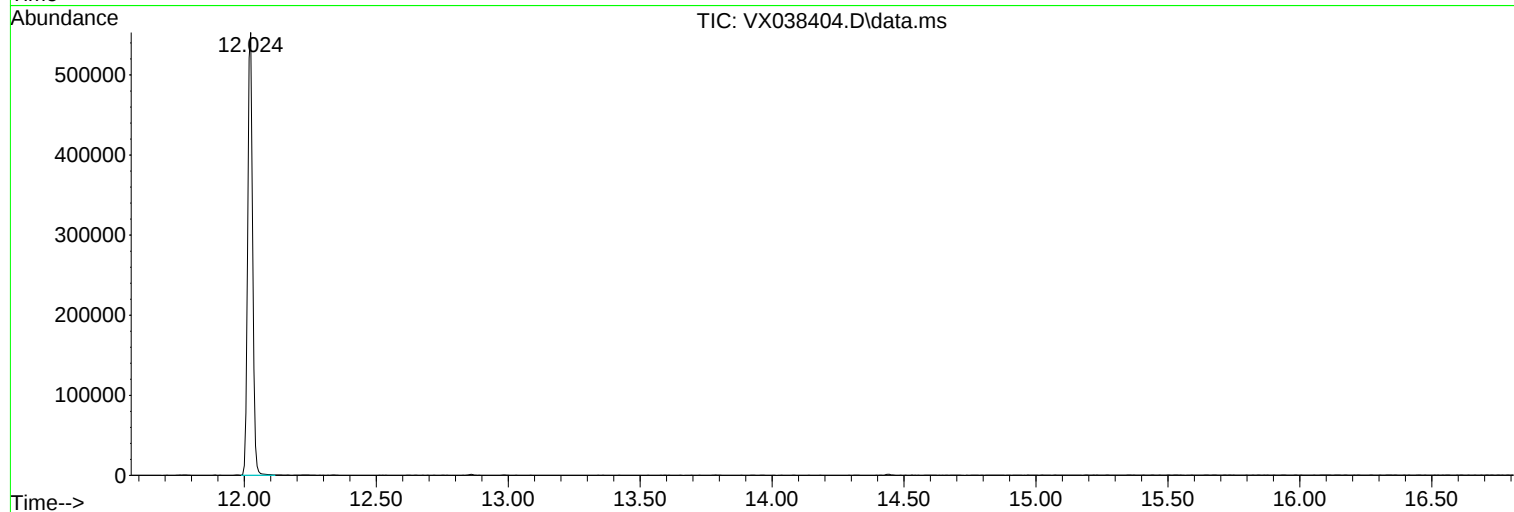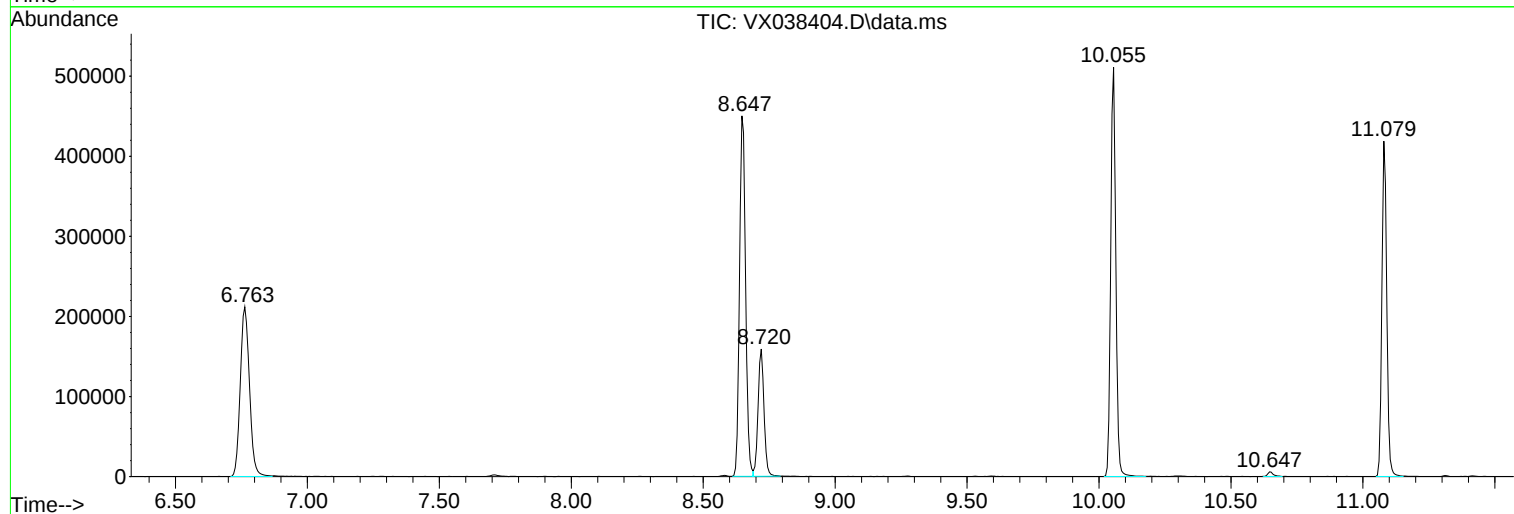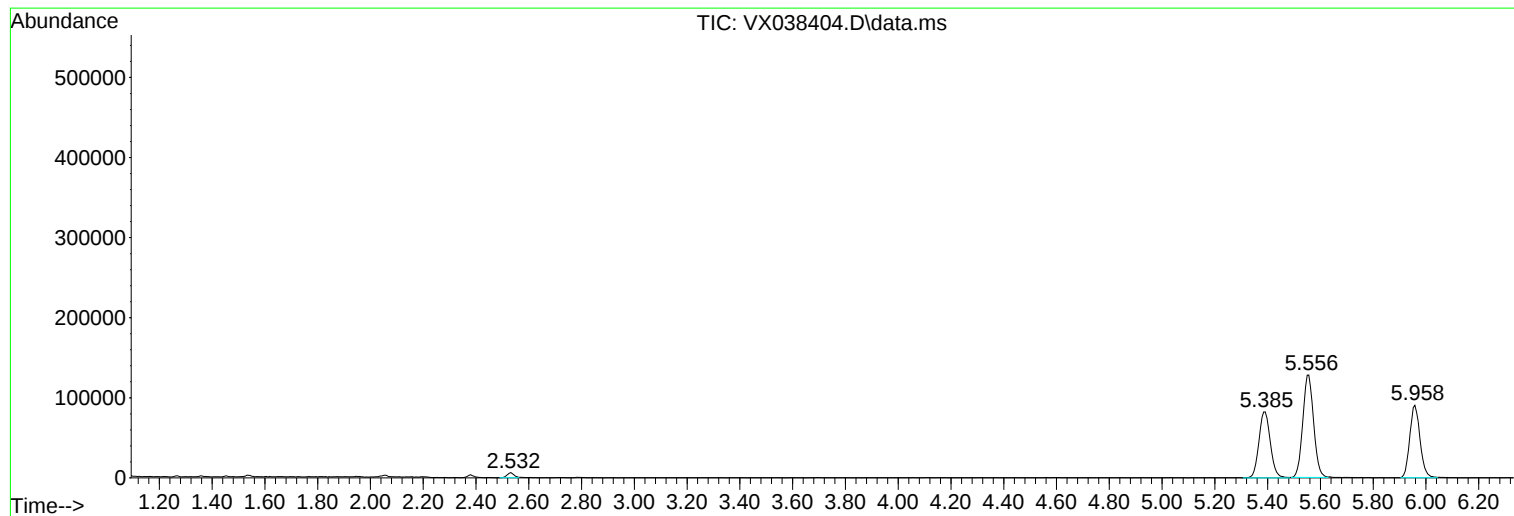

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX102023\
Data File : VX038404.D
Acq On : 20 Oct 2023 15:53
Operator : JC/MD
Sample : 05003-01
Misc : 5.0mL/MSVOA_X/WATER
ALS Vial : 15 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
GWOW-BR-06-323-343-102023

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\82X100523W.M
Quant Title : SW846 8260

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX102023\
Data File : VX038404.D
Acq On : 20 Oct 2023 15:53
Operator : JC/MD
Sample : 05003-01
Misc : 5.0mL/MSVOA_X/WATER
ALS Vial : 15 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
GWOW-BR-06-323-343-102023

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\82X100523W.M
Quant Title : SW846 8260

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	#	RT	Resp	Conc
------------------	----	---------	-------	----------	---	----	------	------