

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX102023\
Data File : VX038414.D
Acq On : 20 Oct 2023 19:45
Operator : JC/MD
Sample : 04991-03 50X
Misc : 5.0mL/MSVOA_X/WATER
ALS Vial : 25 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
1025

Integration Parameters: RTEINT.P

Integrator: RTE

Smoothing : ON

Filtering: 5

Sampling : 1

Min Area: 3 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\82X100523W.M

Title : SW846 8260

Signal : TIC: VX038414.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	2.380	206	212	218	rBV	13446	22930	3.05%	0.543%
2	4.568	560	571	587	rBV2	7548	27925	3.72%	0.661%
3	5.385	693	705	721	rBV	86912	253379	33.74%	6.001%
4	5.550	721	732	747	rBV	131373	378248	50.36%	8.958%
5	5.958	789	799	816	rBV	93536	251388	33.47%	5.954%
6	6.763	920	931	950	rBV	219595	530883	70.69%	12.573%
7	8.647	1233	1240	1265	rBV	459988	746578	99.41%	17.682%
8	10.055	1465	1471	1487	rBV	509448	707908	94.26%	16.766%
9	11.079	1634	1639	1654	rBV	425693	552081	73.51%	13.075%
10	12.024	1788	1794	1806	rBV	574533	751033	100.00%	17.787%




Sum of corrected areas: 4222353

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX102023\
Data File : VX038414.D
Acq On : 20 Oct 2023 19:45
Operator : JC/MD
Sample : 04991-03 50X
Misc : 5.0mL/MSVOA_X/WATER
ALS Vial : 25 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
1025

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\82X100523W.M
Quant Title : SW846 8260

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

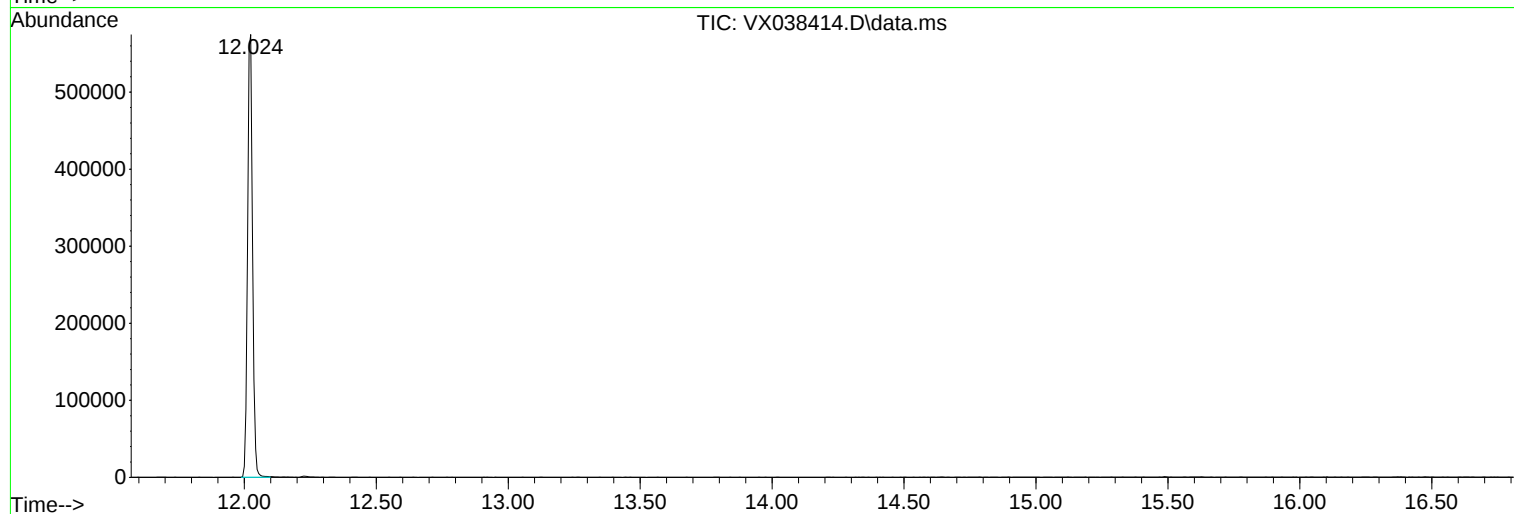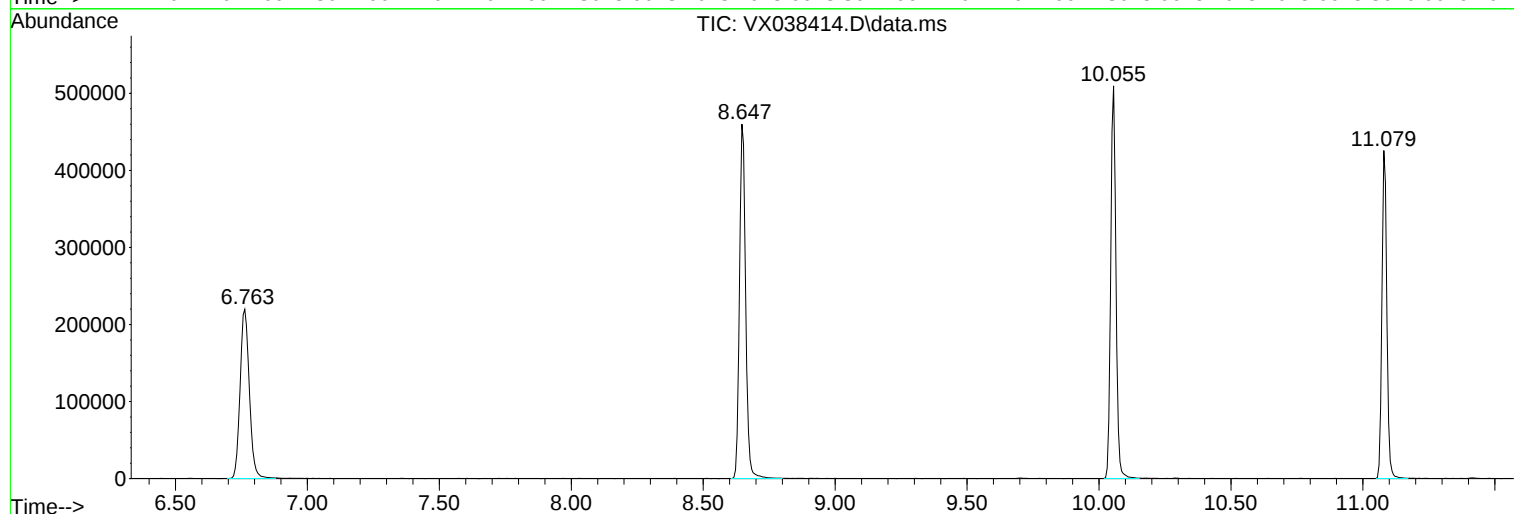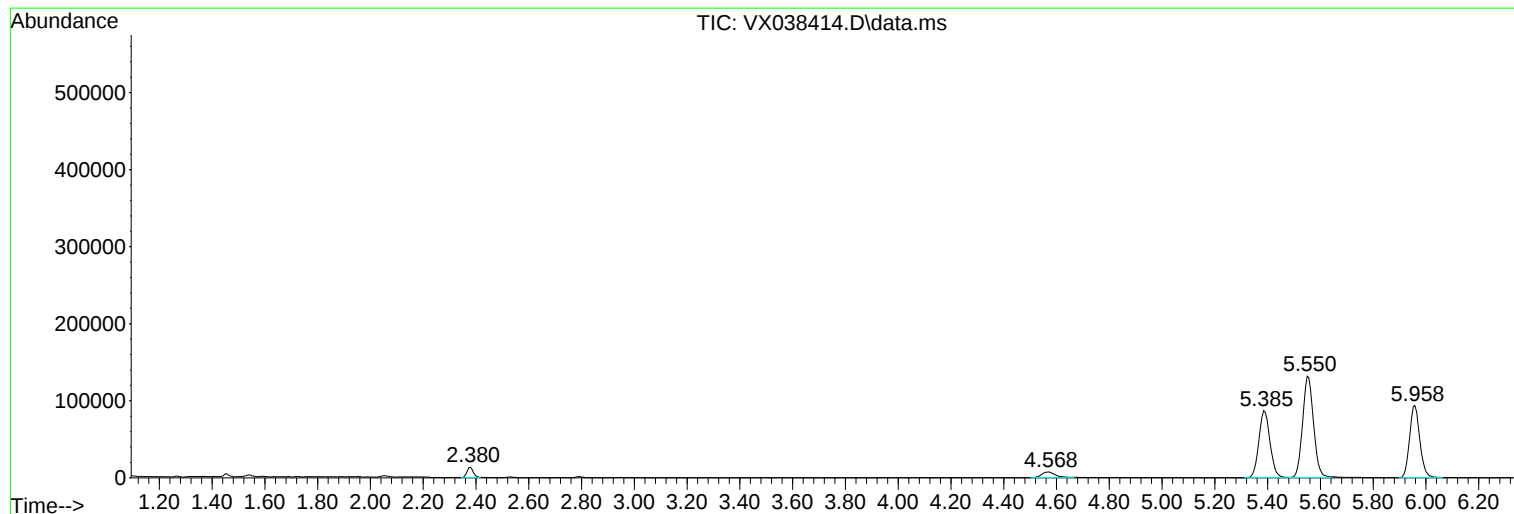

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX102023\
Data File : VX038414.D
Acq On : 20 Oct 2023 19:45
Operator : JC/MD
Sample : 04991-03 50X
Misc : 5.0mL/MSVOA_X/WATER
ALS Vial : 25 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
1025

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\82X100523W.M
Quant Title : SW846 8260

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX102023\
Data File : VX038414.D
Acq On : 20 Oct 2023 19:45
Operator : JC/MD
Sample : 04991-03 50X
Misc : 5.0mL/MSVOA_X/WATER
ALS Vial : 25 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
1025

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\82X100523W.M
Quant Title : SW846 8260

TIC Library : C:\Database\NIST0.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	#	RT	Resp	Conc
------------------	----	---------	-------	----------	---	----	------	------