

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX102023\
Data File : VX038415.D
Acq On : 20 Oct 2023 20:08
Operator : JC/MD
Sample : 04991-04 50X
Misc : 5.0mL/MSVOA_X/WATER
ALS Vial : 26 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
1026

Integration Parameters: RTEINT.P

Integrator: RTE

Smoothing : ON

Filtering: 5

Sampling : 1

Min Area: 3 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\82X100523W.M
Title : SW846 8260

Signal : TIC: VX038415.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	2.380	205	212	222	rBV	38847	64042	8.56%	1.499%
2	2.532	230	237	247	rBV	15413	32107	4.29%	0.751%
3	4.568	561	571	582	rBV2	6891	24015	3.21%	0.562%
4	5.385	693	705	721	rBV	86771	250428	33.49%	5.860%
5	5.550	721	732	752	rVV	129969	376450	50.34%	8.809%
6	5.958	788	799	813	rBV	96867	254394	34.02%	5.953%
7	6.763	922	931	949	rBV	213903	524552	70.14%	12.275%
8	8.647	1234	1240	1265	rBV	449513	741568	99.16%	17.353%
9	10.055	1465	1471	1488	rBV	512389	705528	94.35%	16.510%
10	11.079	1634	1639	1656	rBV	427296	552517	73.88%	12.929%
11	12.024	1788	1794	1804	rBV	580074	747813	100.00%	17.499%




Sum of corrected areas: 4273414

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX102023\
Data File : VX038415.D
Acq On : 20 Oct 2023 20:08
Operator : JC/MD
Sample : 04991-04 50X
Misc : 5.0mL/MSVOA_X/WATER
ALS Vial : 26 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
1026

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\82X100523W.M
Quant Title : SW846 8260

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

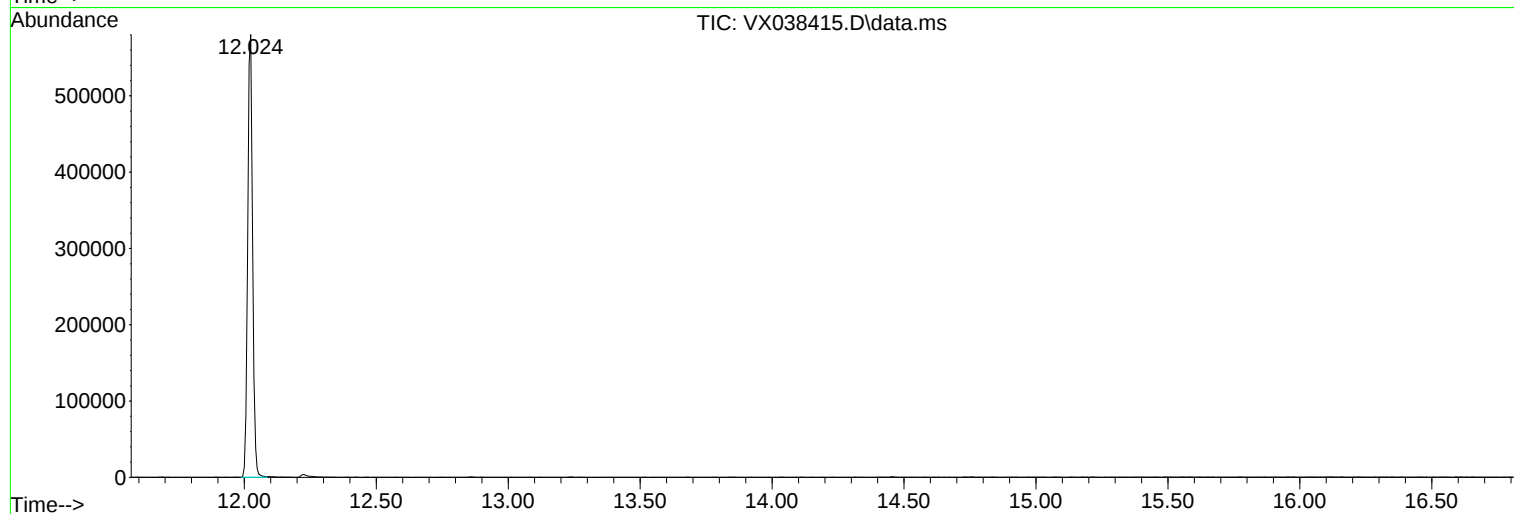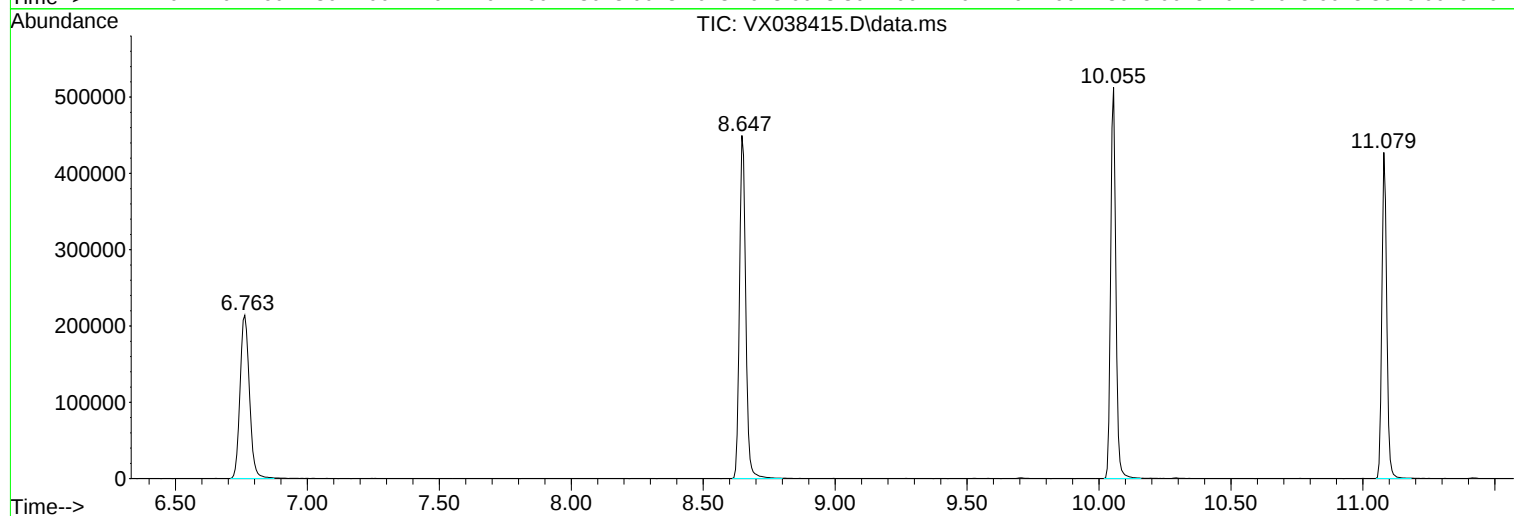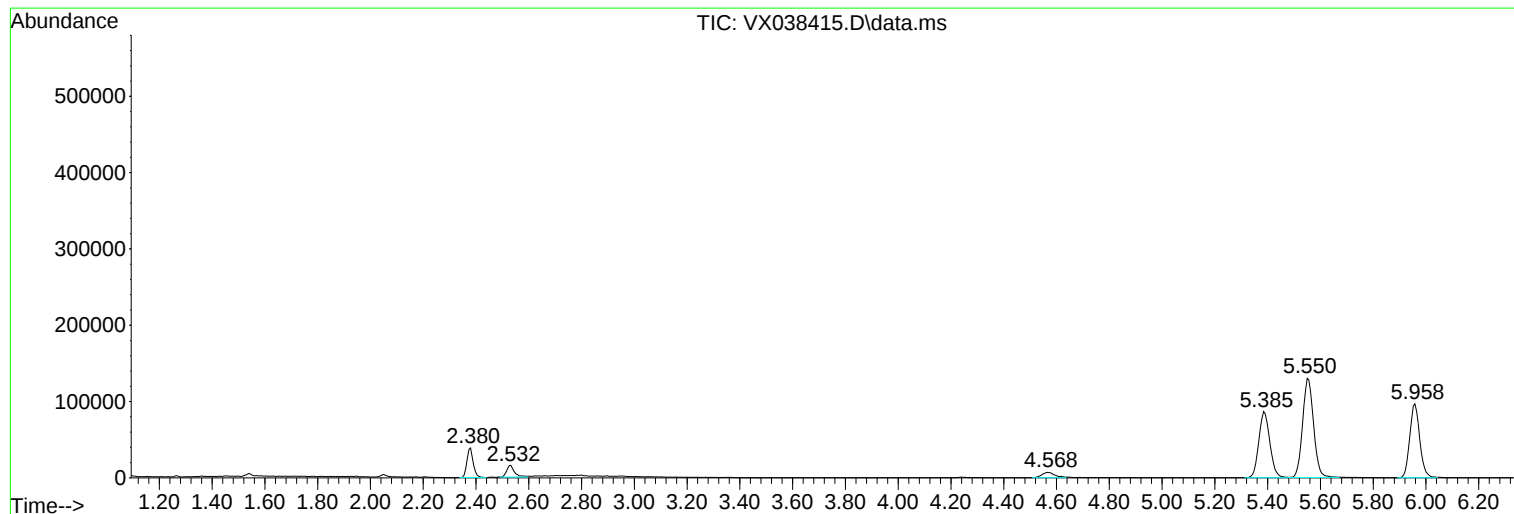

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX102023\
Data File : VX038415.D
Acq On : 20 Oct 2023 20:08
Operator : JC/MD
Sample : 04991-04 50X
Misc : 5.0mL/MSVOA_X/WATER
ALS Vial : 26 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
1026

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\82X100523W.M
Quant Title : SW846 8260

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX102023\
Data File : VX038415.D
Acq On : 20 Oct 2023 20:08
Operator : JC/MD
Sample : 04991-04 50X
Misc : 5.0mL/MSVOA_X/WATER
ALS Vial : 26 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
1026

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\82X100523W.M
Quant Title : SW846 8260

TIC Library : C:\Database\NIST0.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	#	RT	Resp	Conc
------------------	----	---------	-------	----------	---	----	------	------