

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX102023\
Data File : VX038416.D
Acq On : 20 Oct 2023 20:31
Operator : JC/MD
Sample : 04991-05 50X
Misc : 5.0mL/MSVOA_X/WATER
ALS Vial : 27 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
1027

Integration Parameters: RTEINT.P

Integrator: RTE

Smoothing : ON

Sampling : 1

Start Thrs: 0.2

Stop Thrs : 0

Filtering: 5

Min Area: 3 % of largest Peak

Max Peaks: 100

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\82X100523W.M

Title : SW846 8260

Signal : TIC: VX038416.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	4.556	559	569	570	rBV	5607	8945	1.16%	0.211%
2	5.385	693	705	721	rBV	85979	253256	32.75%	5.978%
3	5.550	721	732	746	rBV	129613	374053	48.37%	8.830%
4	5.958	789	799	815	rBV	97838	254629	32.93%	6.011%
5	6.763	921	931	948	rBV	217073	529723	68.51%	12.504%
6	8.647	1234	1240	1263	rBV	458072	751711	97.21%	17.745%
7	10.055	1465	1471	1488	rBV	521723	722769	93.47%	17.061%
8	11.079	1634	1639	1653	rBV	438100	567961	73.45%	13.407%
9	12.024	1788	1794	1806	rBV	596380	773252	100.00%	18.253%




Sum of corrected areas: 4236299

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX102023\
Data File : VX038416.D
Acq On : 20 Oct 2023 20:31
Operator : JC/MD
Sample : 04991-05 50X
Misc : 5.0mL/MSVOA_X/WATER
ALS Vial : 27 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
1027

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\82X100523W.M
Quant Title : SW846 8260

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

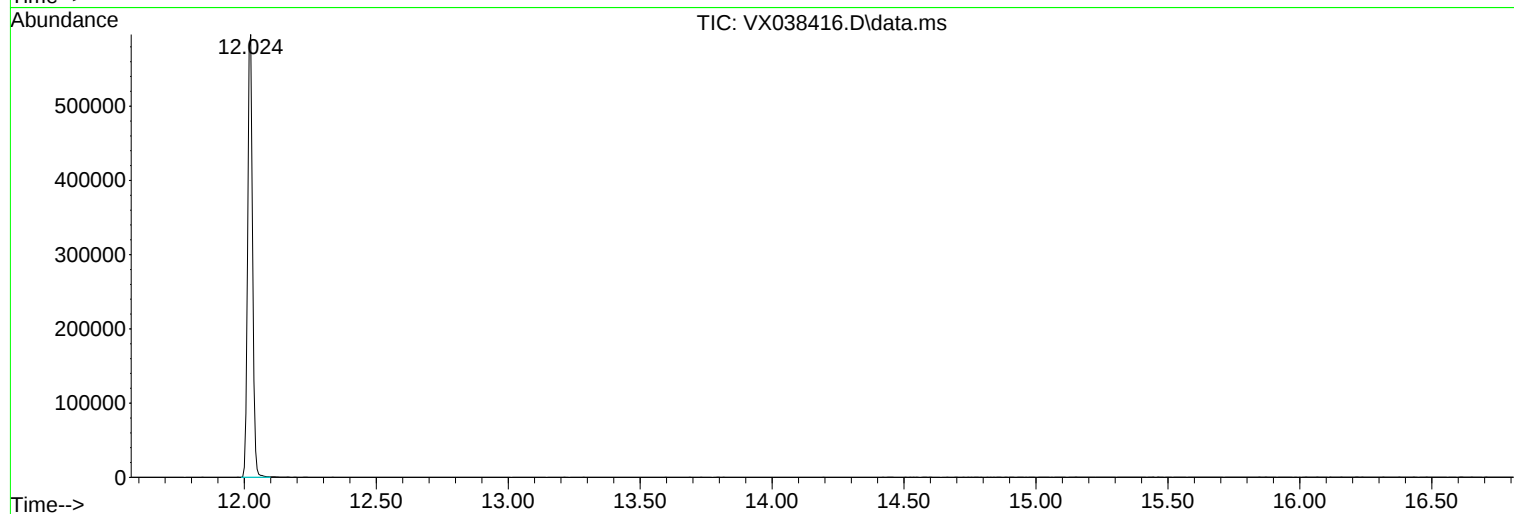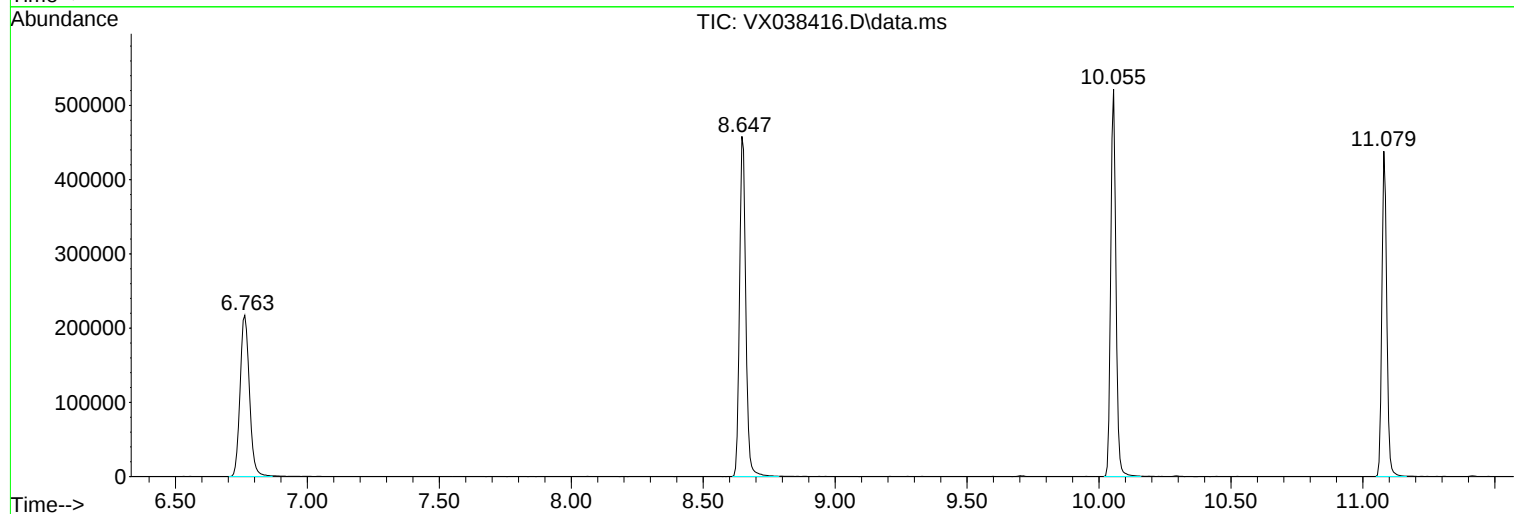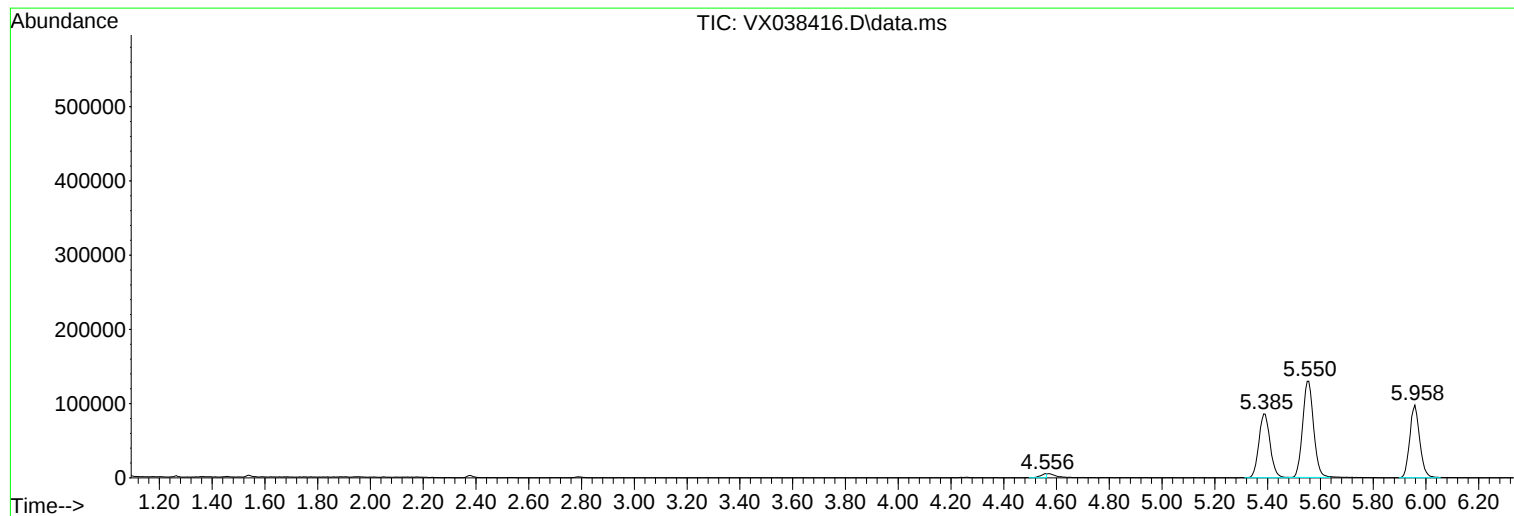

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX102023\
Data File : VX038416.D
Acq On : 20 Oct 2023 20:31
Operator : JC/MD
Sample : 04991-05 50X
Misc : 5.0mL/MSVOA_X/WATER
ALS Vial : 27 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
1027

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\82X100523W.M
Quant Title : SW846 8260

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX102023\
Data File : VX038416.D
Acq On : 20 Oct 2023 20:31
Operator : JC/MD
Sample : 04991-05 50X
Misc : 5.0mL/MSVOA_X/WATER
ALS Vial : 27 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
1027

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\82X100523W.M
Quant Title : SW846 8260

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	#	RT	Resp	Conc
------------------	----	---------	-------	----------	---	----	------	------