
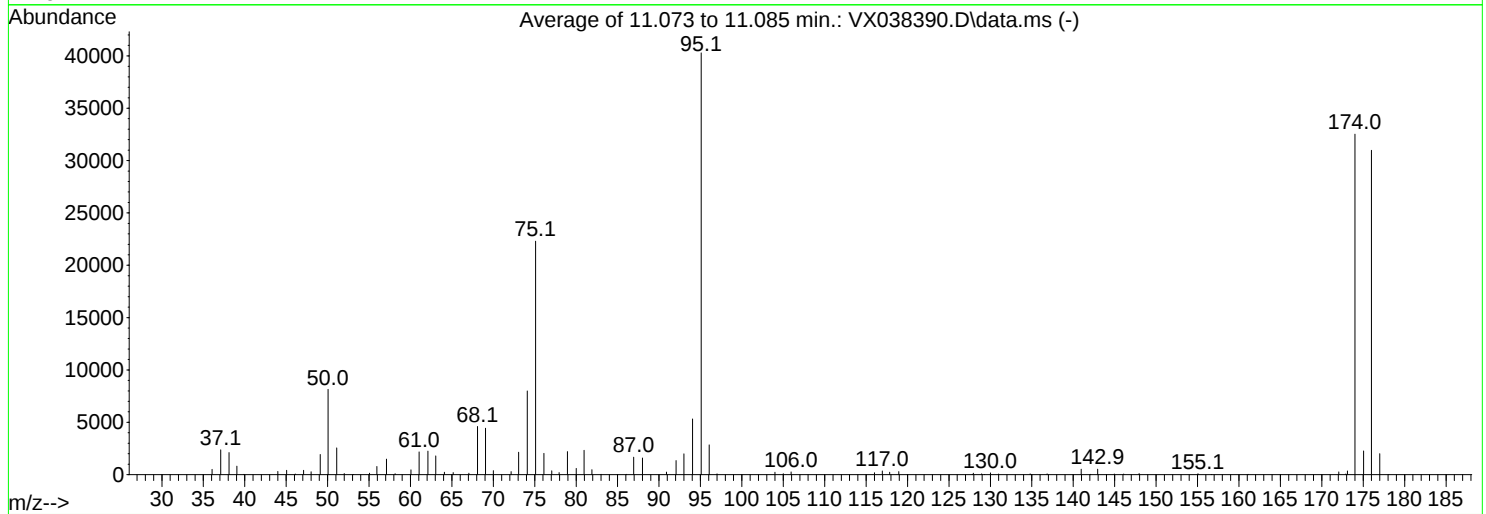


Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX102023\
Data File : VX038390.D
Acq On : 20 Oct 2023 09:09
Operator : JC/MD
Sample : BFB
Misc : 5.0mL/MSVOA_X/WATER
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
BFB

Integration File: RTEINT.P

Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\82X100523W.M
Title : SW846 8260
Last Update : Thu Oct 05 15:27:13 2023

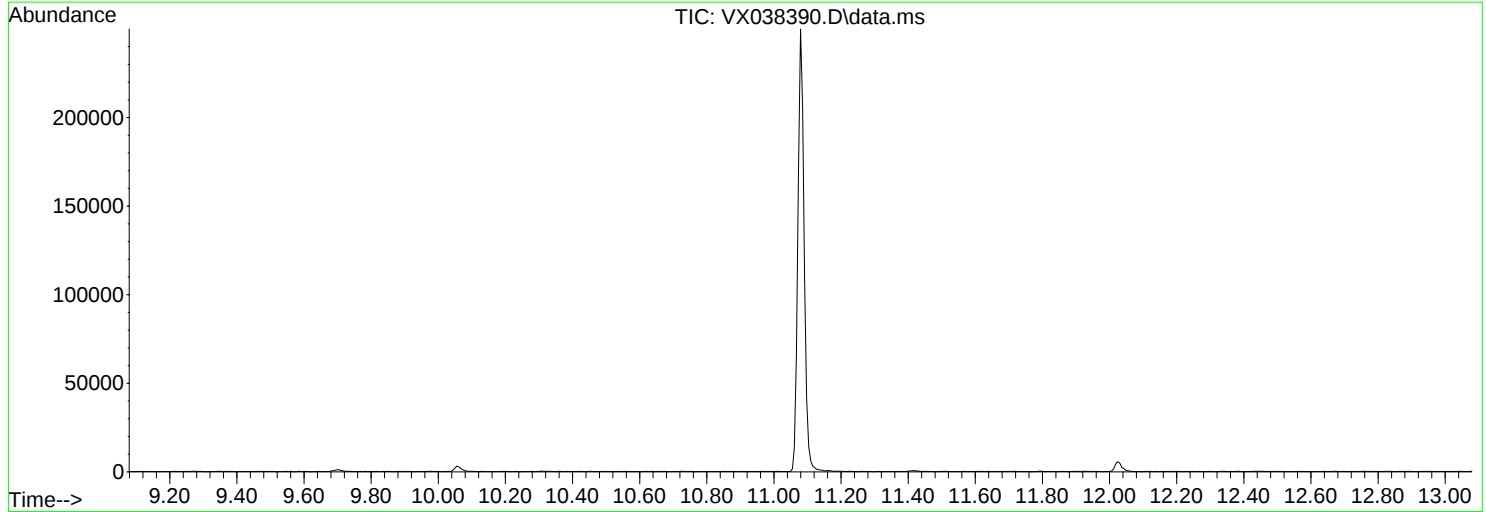

AutoFind: Scans 1638, 1639, 1640; Background Corrected with Scan 1632

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	15	40	20.2	8140	PASS
75	95	30	60	55.3	22296	PASS
95	95	100	100	100.0	40291	PASS
96	95	5	9	7.1	2850	PASS
173	174	0.00	2	1.1	353	PASS
174	95	50	100	80.7	32528	PASS
175	174	5	9	6.9	2256	PASS
176	174	95	101	95.3	30989	PASS
177	176	5	9	6.5	2000	PASS