


Data Path : Z:\VOASRV\HPCHEM1\MSVOA X\DATA\VX102120\  
 Data File : VX018997.D  
 Acq On : 21 Oct 2020 09:45  
 Operator : JC/SP  
 Sample : BFB  
 Misc : 5.0mL/MSVOA X/WATER  
 ALS Vial : 1 Sample Multiplier: 1

Instrument :  
 MSVOA\_X  
 ClientSampleId :  
 BFB

Integration File: RTEINT.P

Method : Z:\VOASRV\HPCHEM1\MSVOA\_X\METHOD\82X102120W.M  
 Title : SW846 8260  
 Last Update : Thu Oct 22 17:51:42 2020

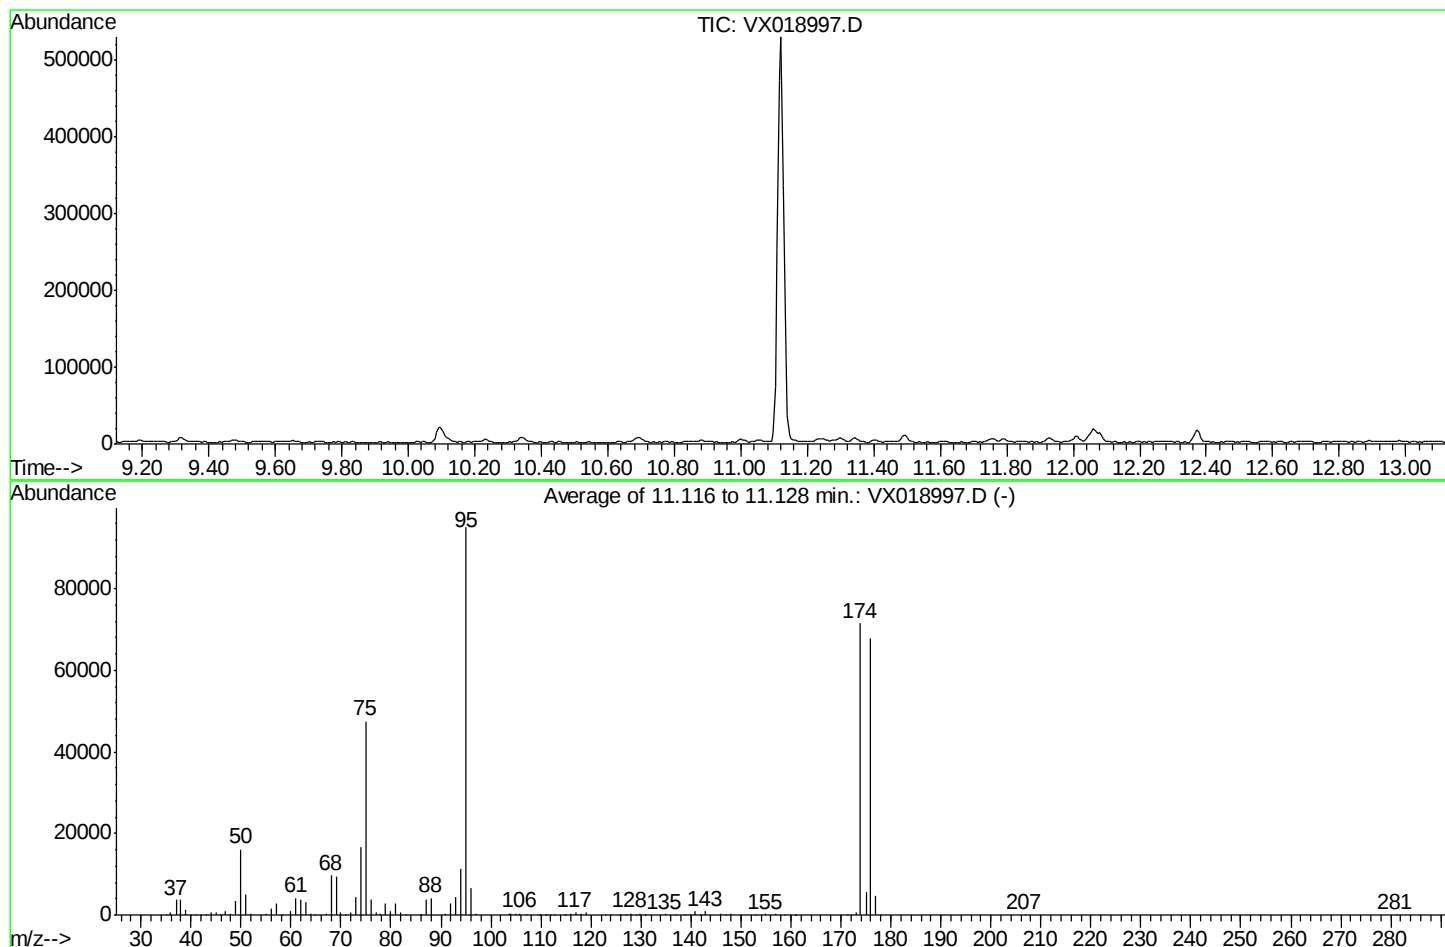

AutoFind: Scans 1645, 1646, 1647; Background Corrected with Scan 1638

| Target Mass | Rel. to Mass | Lower Limit% | Upper Limit% | Rel. Abn% | Raw Abn | Result Pass/Fail |
|-------------|--------------|--------------|--------------|-----------|---------|------------------|
| 50          | 95           | 15           | 40           | 16.9      | 16063   | PASS             |
| 75          | 95           | 30           | 60           | 49.9      | 47448   | PASS             |
| 95          | 95           | 100          | 100          | 100.0     | 95109   | PASS             |
| 96          | 95           | 5            | 9            | 6.9       | 6536    | PASS             |
| 173         | 174          | 0.00         | 2            | 1.0       | 741     | PASS             |
| 174         | 95           | 50           | 100          | 75.3      | 71597   | PASS             |
| 175         | 174          | 5            | 9            | 7.8       | 5620    | PASS             |
| 176         | 174          | 95           | 101          | 95.0      | 67994   | PASS             |
| 177         | 176          | 5            | 9            | 6.8       | 4631    | PASS             |