

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX102122\
 Data File : VX032316.D
 Acq On : 22 Oct 2022 03:15
 Operator : JC/MD
 Sample : N5248-15
 Misc : 5.0mL/MSVOA_X/WATER
 ALS Vial : 40 Sample Multiplier: 1

Instrument :
 MSVOA_X
 ClientSampleId :
 FSND-GEP-4-20221018

Quant Time: Oct 22 06:05:13 2022
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\82X101922W.M
 Quant Title : SW846 8260
 QLast Update : Sat Oct 22 04:56:40 2022
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) Pentafluorobenzene	5.556	168	145091	50.000	ug/l	0.00
34) 1,4-Difluorobenzene	6.763	114	227074	50.000	ug/l	0.00
63) Chlorobenzene-d5	10.055	117	192825	50.000	ug/l	0.00
72) 1,4-Dichlorobenzene-d4	12.024	152	84263	50.000	ug/l	0.00
System Monitoring Compounds						
33) 1,2-Dichloroethane-d4	5.958	65	91661	48.563	ug/l	0.00
Spiked Amount	50.000	Range	78 - 117	Recovery	=	97.120%
35) Dibromofluoromethane	5.385	113	71338	45.147	ug/l	0.00
Spiked Amount	50.000	Range	75 - 124	Recovery	=	90.300%
50) Toluene-d8	8.647	98	262734	46.191	ug/l	0.00
Spiked Amount	50.000	Range	92 - 112	Recovery	=	92.380%
62) 4-Bromofluorobenzene	11.079	95	89207	42.829	ug/l	0.00
Spiked Amount	50.000	Range	83 - 123	Recovery	=	85.660%
Target Compounds						
					Qvalue	
12) 1,1-Dichloroethene	2.325	96	782	0.604	ug/l	89
27) cis-1,2-Dichloroethene	4.495	96	479	0.290	ug/l	56
30) Chloroform	5.092	83	1169	0.417	ug/l	94
32) 1,1,1-Trichloroethane	5.391	97	33316	13.948	ug/l	99
36) 1,1-Dichloropropene	5.550	75	11292	5.555	ug/l #	49
38) Carbon Tetrachloride	5.672	117	1152	0.537	ug/l #	82
44) Trichloroethene	7.129	130	591377	364.535	ug/l	99
64) Tetrachloroethene	9.275	164	4572	3.591	ug/l	95


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX102122\
Data File : VX032316.D
Acq On : 22 Oct 2022 03:15
Operator : JC/MD
Sample : N5248-15
Misc : 5.0mL/MSVOA_X/WATER
ALS Vial : 40 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
FSND-GEP-4-20221018

Quant Time: Oct 22 06:05:13 2022
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\82X101922W.M
Quant Title : SW846 8260
QLast Update : Sat Oct 22 04:56:40 2022
Response via : Initial Calibration




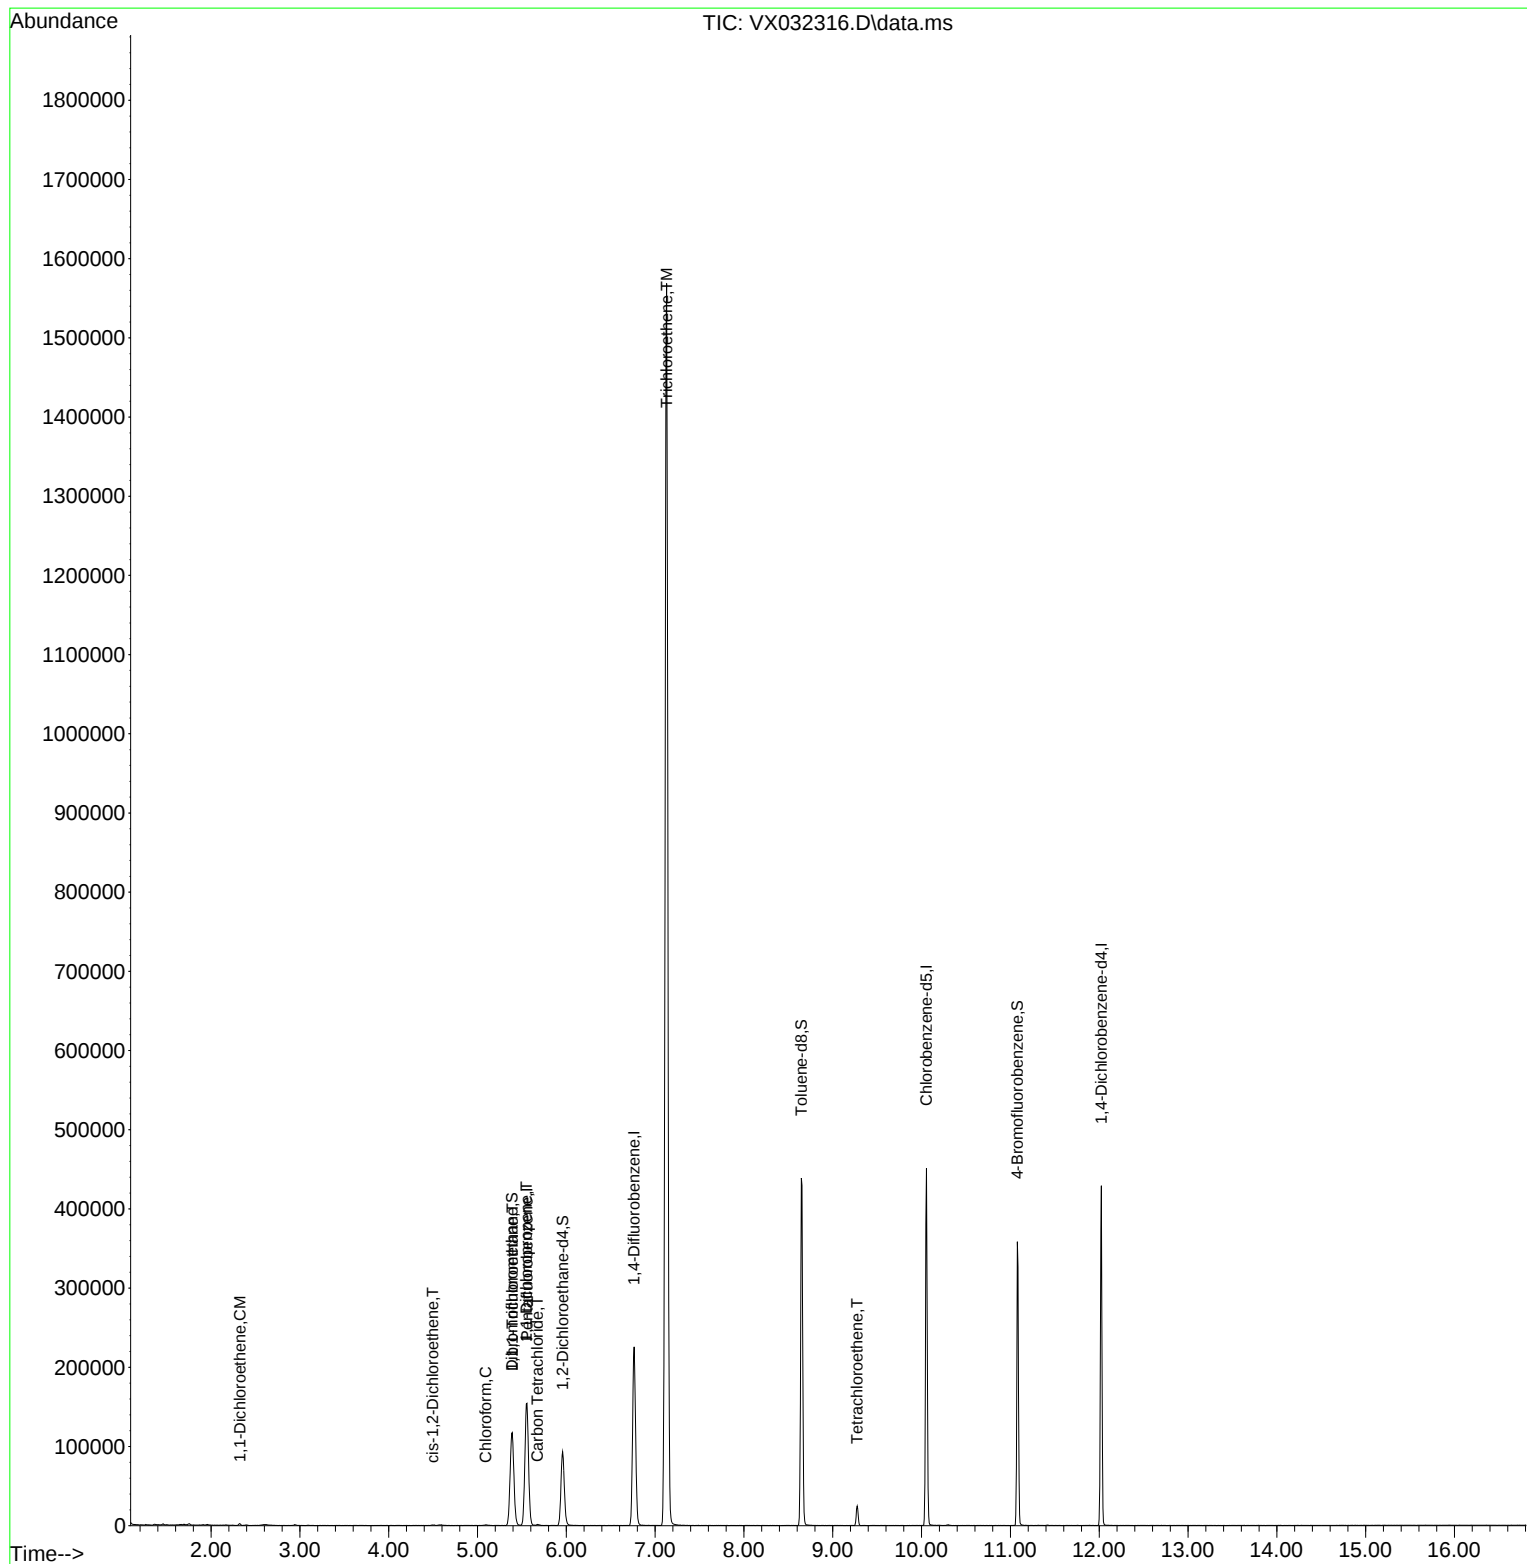


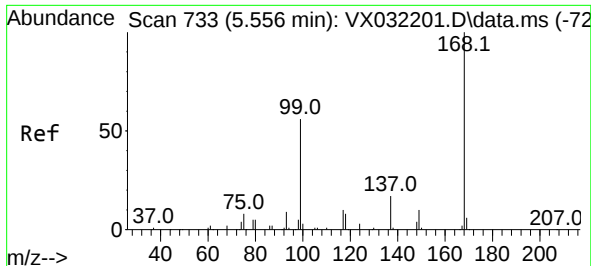

#1
Pentafluorobenzene
Concen: 50.000 ug/l
RT: 5.556 min Scan# 71
Delta R.T. -0.000 min
Lab File: VX032316.D
Acq: 22 Oct 2022 03:15




Instrument :
MSVOA_X
ClientSampleId :
FSND-GEP-4-20221018


Tgt Ion:168 Resp: 145091
Ion Ratio Lower Upper
168 100
99 58.3 44.8 67.2

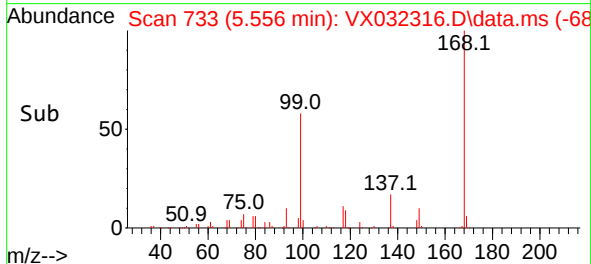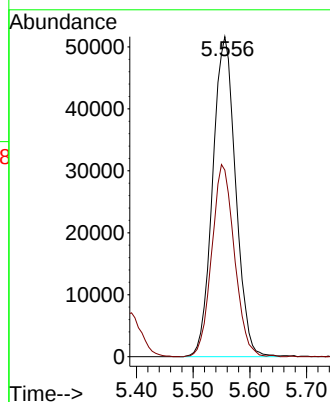

#12
1,1-Dichloroethene
Concen: 0.604 ug/l
RT: 2.325 min Scan# 203
Delta R.T. 0.006 min
Lab File: VX032316.D
Acq: 22 Oct 2022 03:15

Tgt Ion: 96 Resp: 782
Ion Ratio Lower Upper
96 100
61 140.4 124.0 186.0
98 71.6 50.0 75.0

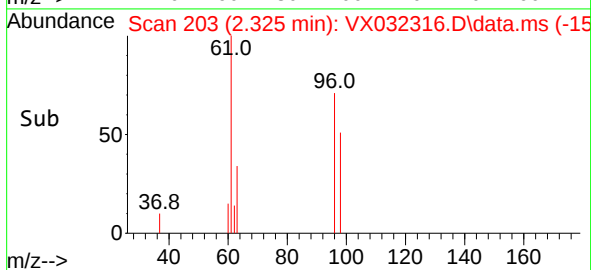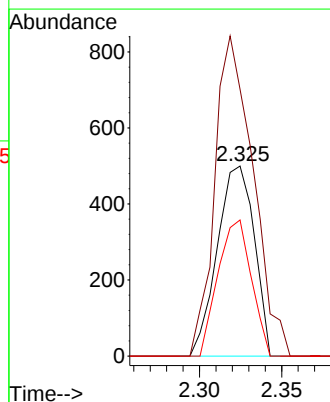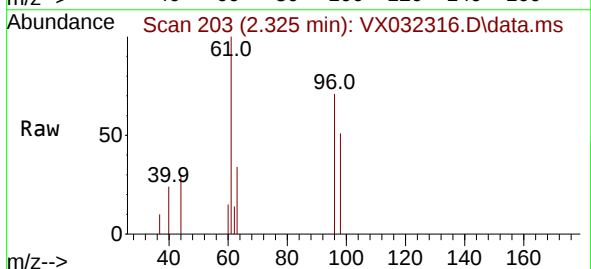



#27

cis-1,2-Dichloroethene

Concen: 0.290 ug/l

RT: 4.495 min Scan# 51

Delta R.T. 0.006 min

Lab File: VX032316.D

Acq: 22 Oct 2022 03:15

Instrument :

MSVOA_X

ClientSampleId :

FSND-GEP-4-20221018





Tgt Ion: 96 Resp: 479

Ion Ratio Lower Upper

96 100

61 70.8 0.0 279.2

98 52.2 0.0 128.0

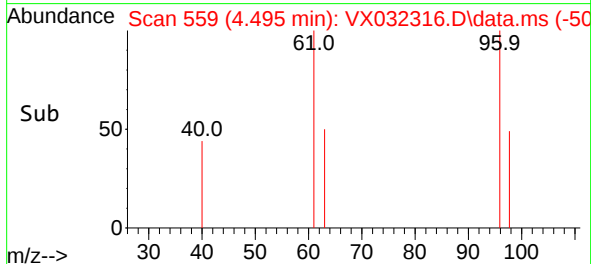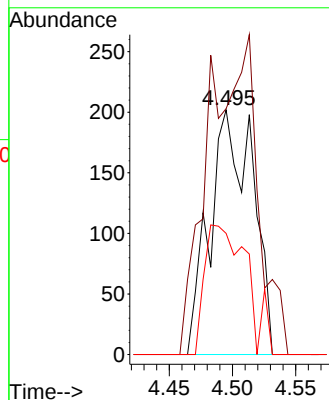

#30

Chloroform

Concen: 0.417 ug/l

RT: 5.092 min Scan# 657

Delta R.T. -0.001 min

Lab File: VX032316.D




Acq: 22 Oct 2022 03:15


Tgt Ion: 83 Resp: 1169

Ion Ratio Lower Upper

83 100

85 60.8 52.5 78.7



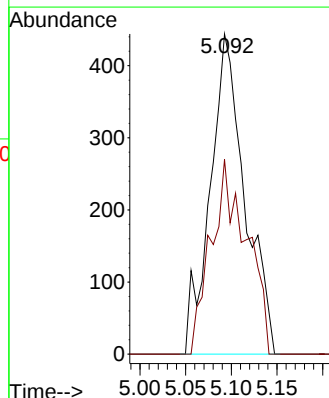
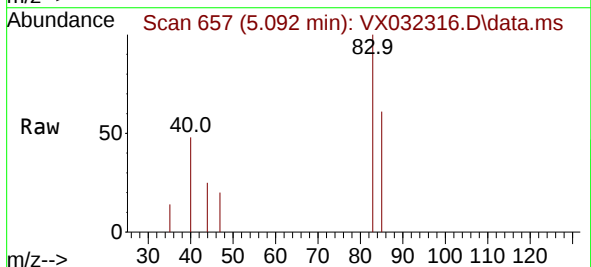


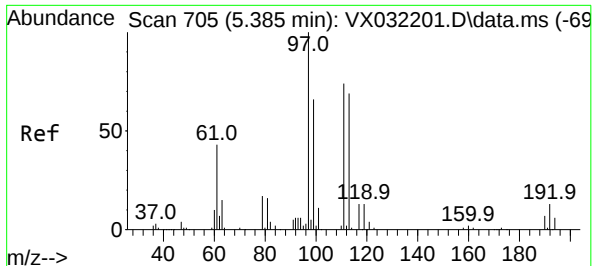

#32
1,1,1-Trichloroethane
Concen: 13.948 ug/l
RT: 5.391 min Scan# 705
Delta R.T. 0.006 min
Lab File: VX032316.D
Acq: 22 Oct 2022 03:15




Instrument :
MSVOA_X
ClientSampleId :
FSND-GEP-4-20221018


Tgt Ion: 97 Resp: 33316
Ion Ratio Lower Upper
97 100
99 64.5 51.8 77.8
61 45.2 35.7 53.5

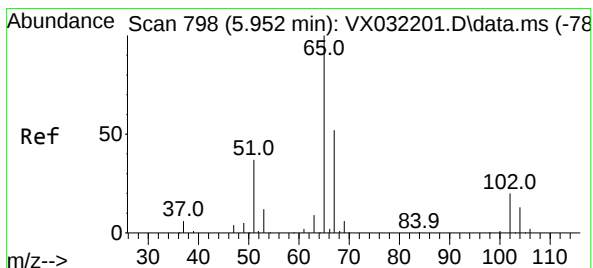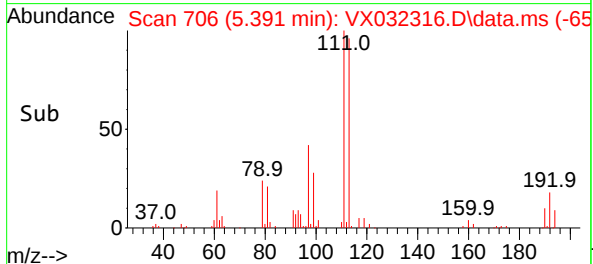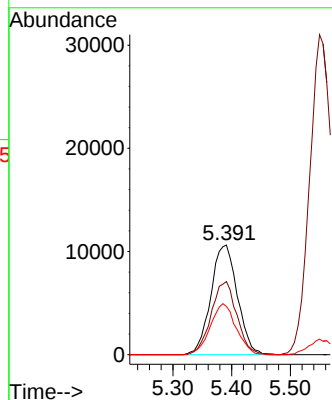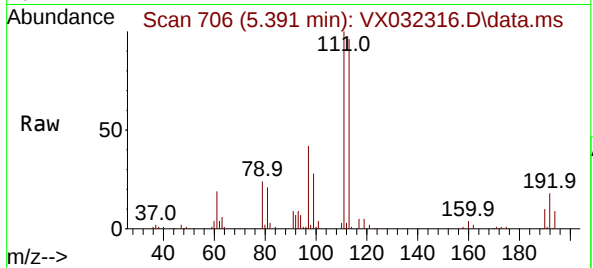

#33
1,2-Dichloroethane-d4
Concen: 48.563 ug/l
RT: 5.958 min Scan# 799
Delta R.T. 0.006 min
Lab File: VX032316.D
Acq: 22 Oct 2022 03:15

Tgt Ion: 65 Resp: 91661
Ion Ratio Lower Upper
65 100
67 50.4 0.0 103.6


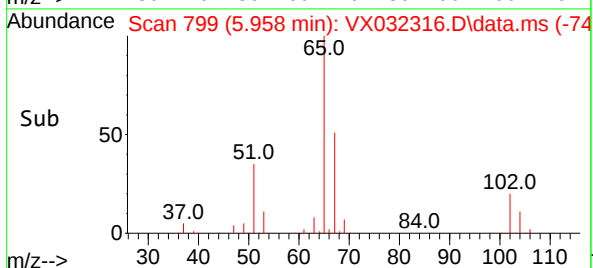
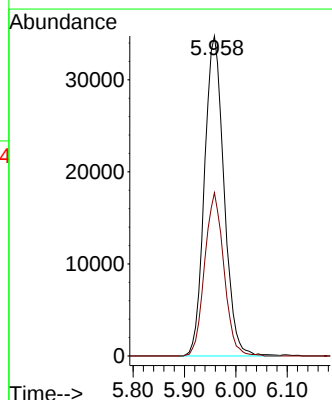
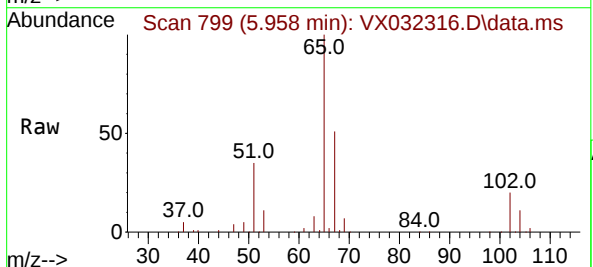




#34
1,4-Difluorobenzene
Concen: 50.000 ug/l
RT: 6.763 min Scan# 911
Delta R.T. -0.000 min
Lab File: VX032316.D
Acq: 22 Oct 2022 03:15




Instrument :
MSVOA_X
ClientSampleId :
FSND-GEP-4-20221018


Tgt Ion:114 Resp: 227074
Ion Ratio Lower Upper
114 100
63 19.5 0.0 38.6
88 16.4 0.0 32.6

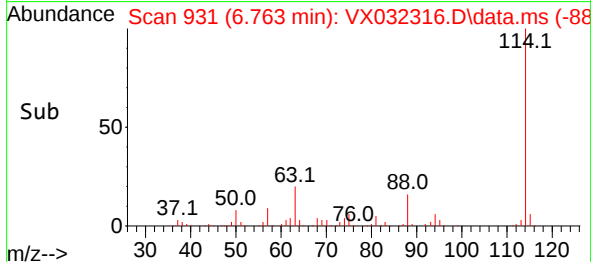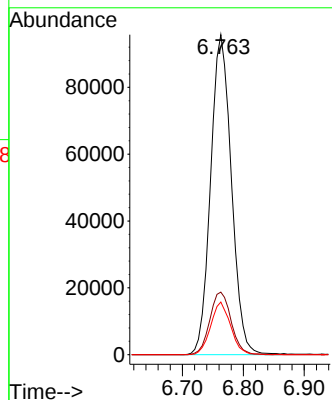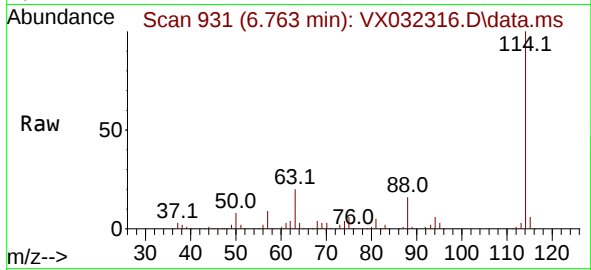

#35
Dibromofluoromethane
Concen: 45.147 ug/l
RT: 5.385 min Scan# 705
Delta R.T. 0.000 min
Lab File: VX032316.D
Acq: 22 Oct 2022 03:15

Tgt Ion:113 Resp: 71338
Ion Ratio Lower Upper
113 100
111 103.9 82.8 124.2
192 19.3 15.5 23.3


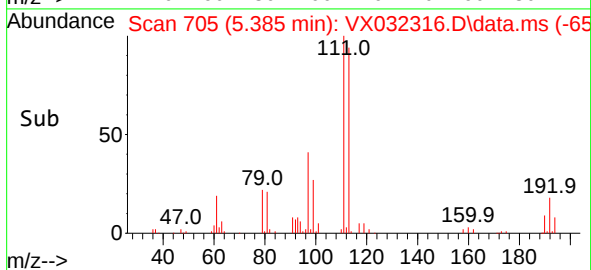
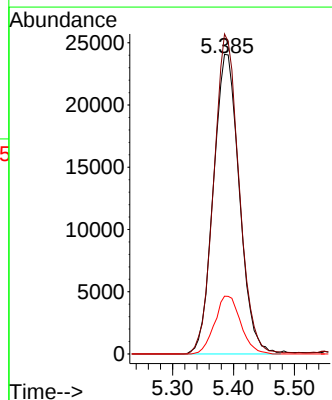
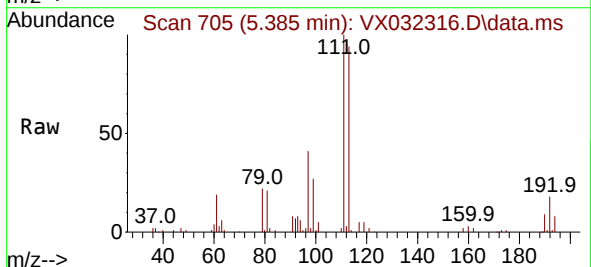


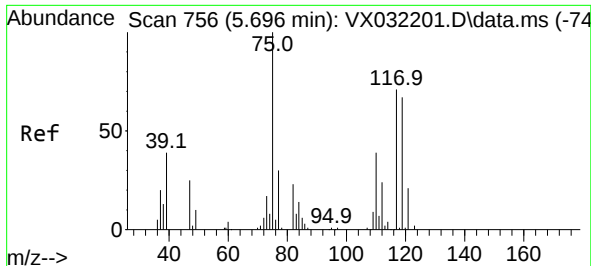

#36
1,1-Dichloropropene
Concen: 5.555 ug/l
RT: 5.550 min Scan# 711
Delta R.T. -0.146 min
Lab File: VX032316.D
Acq: 22 Oct 2022 03:15




Instrument :
MSVOA_X
ClientSampleId :
FSND-GEP-4-20221018


Tgt Ion: 75 Resp: 11292
Ion Ratio Lower Upper
75 100
110 9.6 18.4 55.0#
77 0.0 24.7 37.1#

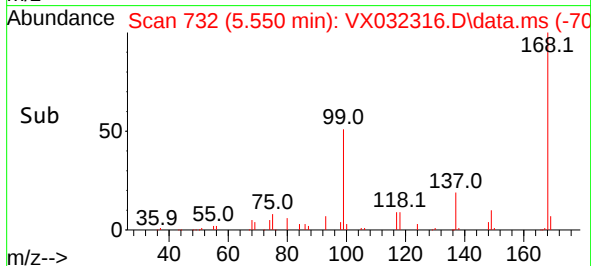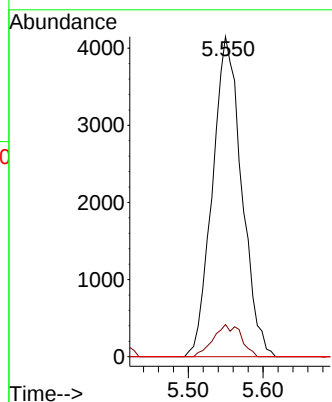

#38
Carbon Tetrachloride
Concen: 0.537 ug/l
RT: 5.672 min Scan# 752
Delta R.T. -0.006 min
Lab File: VX032316.D
Acq: 22 Oct 2022 03:15

Tgt Ion: 117 Resp: 1152
Ion Ratio Lower Upper
117 100
119 74.4 75.4 113.0#
121 23.4 23.9 35.9#


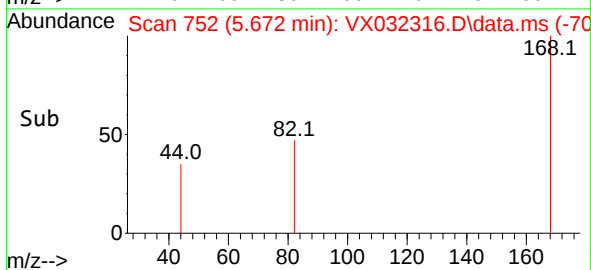
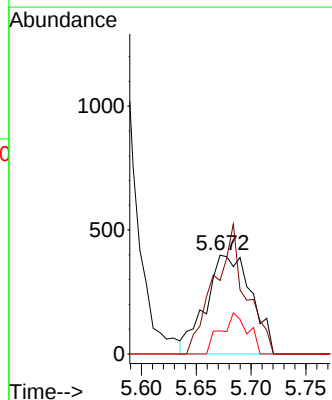
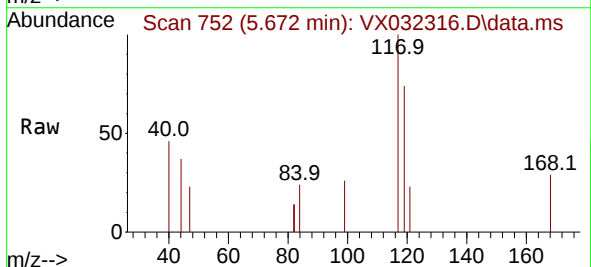


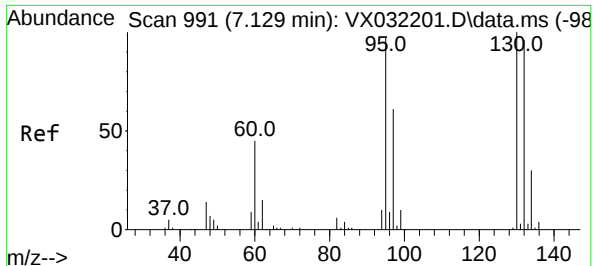

#44
Trichloroethene
Concen: 364.535 ug/l
RT: 7.129 min Scan# 991
Delta R.T. -0.000 min
Lab File: VX032316.D
Acq: 22 Oct 2022 03:15




Instrument :
MSVOA_X
ClientSampleId :
FSND-GEP-4-20221018


Tgt Ion:130 Resp: 591377
Ion Ratio Lower Upper
130 100
95 99.0 0.0 196.8

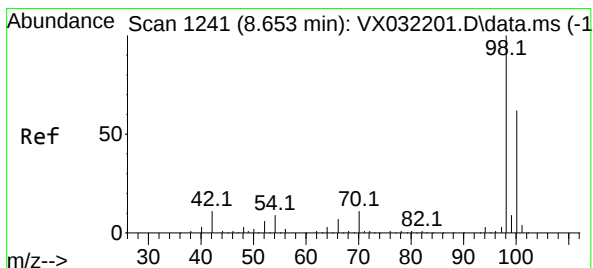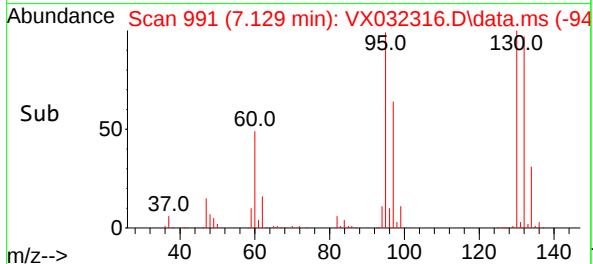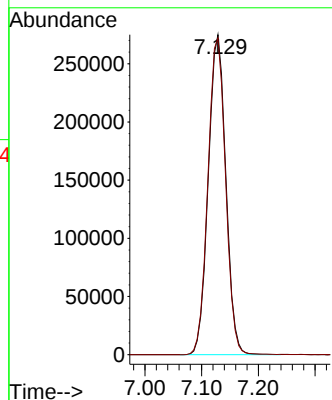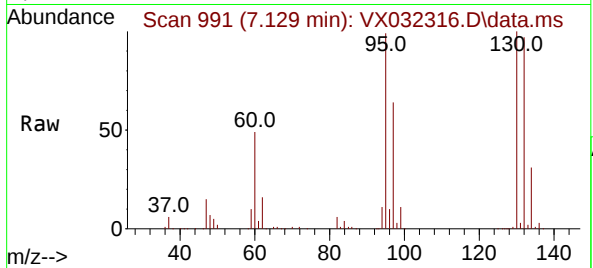

#50
Toluene-d8
Concen: 46.191 ug/l
RT: 8.647 min Scan# 1240
Delta R.T. -0.006 min
Lab File: VX032316.D
Acq: 22 Oct 2022 03:15

Tgt Ion: 98 Resp: 262734
Ion Ratio Lower Upper
98 100
100 63.8 50.7 76.1

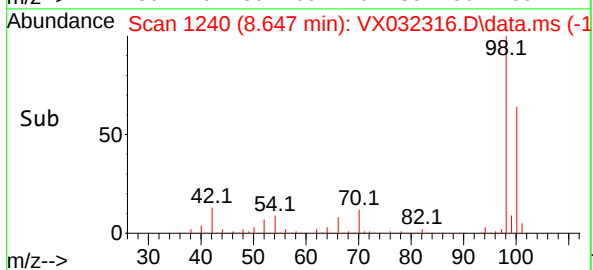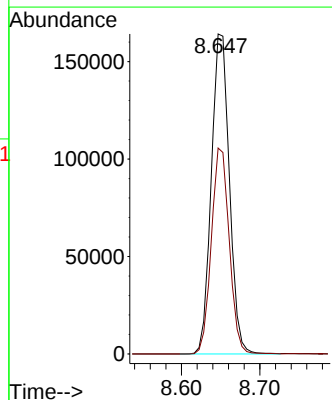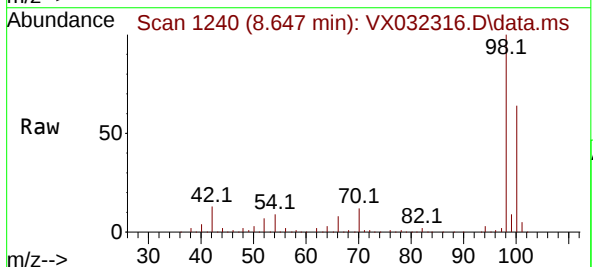

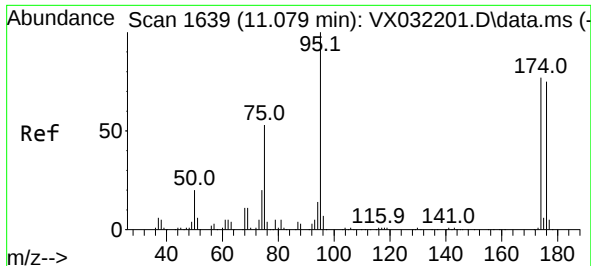

#62

4-Bromofluorobenzene

Concen: 42.829 ug/l

RT: 11.079 min Scan# 1

Delta R.T. 0.000 min

Lab File: VX032316.D

Acq: 22 Oct 2022 03:15

Instrument :

MSVOA_X

ClientSampleId :

FSND-GEP-4-20221018





Tgt Ion: 95 Resp: 89207

Ion Ratio Lower Upper

95 100

174 80.9 0.0 166.8

176 77.4 0.0 161.4

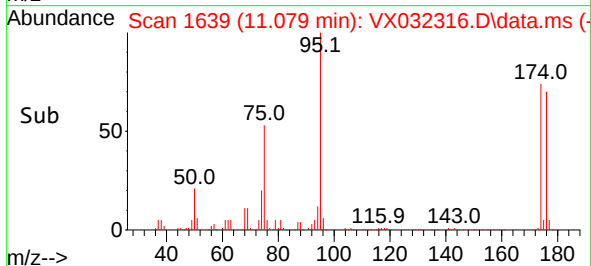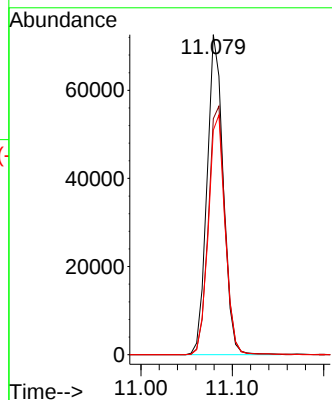

#63

Chlorobenzene-d5

Concen: 50.000 ug/l

RT: 10.055 min Scan# 1471

Delta R.T. -0.000 min

Lab File: VX032316.D

Acq: 22 Oct 2022 03:15




Tgt Ion: 117 Resp: 192825


Ion Ratio Lower Upper

117 100

82 55.5 44.2 66.4

119 31.7 25.8 38.8


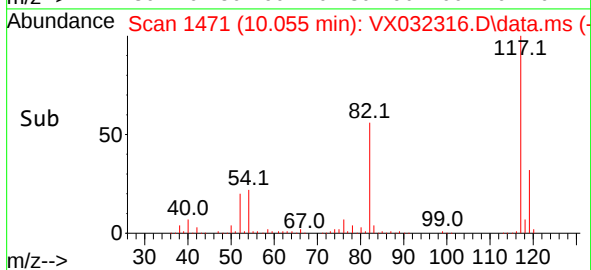
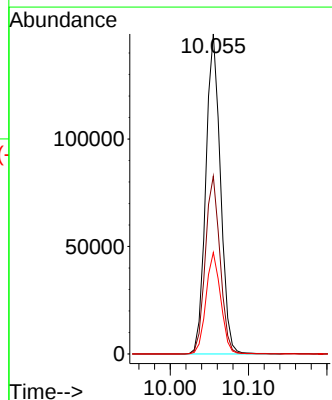
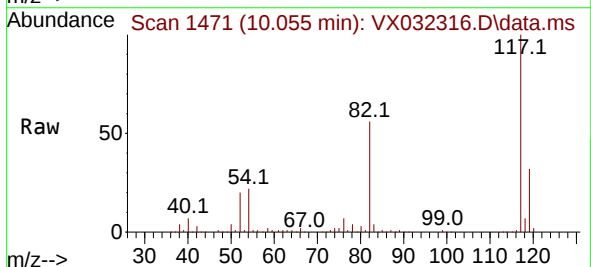




#64
Tetrachloroethene
Concen: 3.591 ug/l
RT: 9.275 min Scan# 11
Delta R.T. -0.000 min
Lab File: VX032316.D
Acq: 22 Oct 2022 03:15

Instrument :
MSVOA_X
ClientSampleId :
FSND-GEP-4-20221018

Tgt Ion:164 Resp: 4572
Ion Ratio Lower Upper
164 100
166 126.2 104.9 157.3
129 103.8 77.8 116.6
131 92.2 76.3 114.5

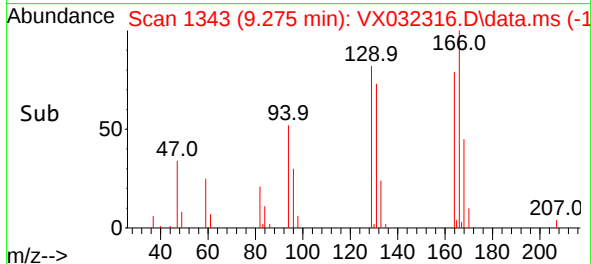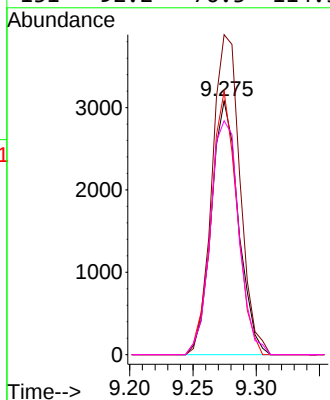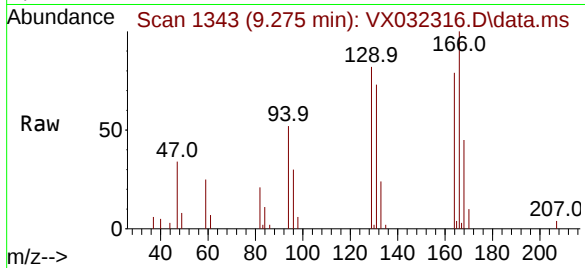

#72
1,4-Dichlorobenzene-d4
Concen: 50.000 ug/l
RT: 12.024 min Scan# 1794
Delta R.T. 0.000 min
Lab File: VX032316.D
Acq: 22 Oct 2022 03:15

Tgt Ion:152 Resp: 84263
Ion Ratio Lower Upper
152 100
115 60.3 43.1 129.4
150 158.0 0.0 348.6

