

Data Path : Z:\voasrv\HPCHEM1\MSVOA\_X\Data\VX102122\  
 Data File : VX032287.D  
 Acq On : 21 Oct 2022 14:39  
 Operator : JC/MD  
 Sample : N5185-17  
 Misc : 5.0mL/MSVOA\_X/WATER  
 ALS Vial : 9 Sample Multiplier: 1

Instrument :  
 MSVOA\_X  
 ClientSampleId :  
 PZ-02

Integration Parameters: RTEINT.P

Integrator: RTE

Smoothing : ON

Filtering: 5

Sampling : 1

Min Area: 3 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA\_X\Method\82X101922W.M

Title : SW846 8260

Signal : TIC: VX032287.D\data.ms

| peak<br># | R.T.<br>min | first<br>scan | max<br>scan | last<br>scan | PK<br>TY | peak<br>height | corr.<br>area | corr.<br>% max. | % of<br>total |
|-----------|-------------|---------------|-------------|--------------|----------|----------------|---------------|-----------------|---------------|
| 1         | 5.385       | 694           | 705         | 721          | rBV      | 77818          | 231015        | 33.88%          | 6.347%        |
| 2         | 5.550       | 721           | 732         | 746          | rVV      | 149829         | 421784        | 61.86%          | 11.587%       |
| 3         | 5.958       | 789           | 799         | 814          | rBV      | 89782          | 235449        | 34.53%          | 6.468%        |
| 4         | 6.763       | 922           | 931         | 949          | rVB      | 217360         | 510198        | 74.83%          | 14.016%       |
| 5         | 8.647       | 1234          | 1240        | 1252         | rBV      | 431715         | 681842        | 100.00%         | 18.732%       |
| 6         | 10.055      | 1465          | 1471        | 1482         | rBV      | 438738         | 579125        | 84.94%          | 15.910%       |
| 7         | 11.079      | 1634          | 1639        | 1648         | rBV      | 356507         | 449758        | 65.96%          | 12.356%       |
| 8         | 12.024      | 1788          | 1794        | 1807         | rBV      | 426307         | 530827        | 77.85%          | 14.583%       |




Sum of corrected areas: 3639998

Data Path : Z:\voasrv\HPCHEM1\MSVOA\_X\Data\VX102122\  
Data File : VX032287.D  
Acq On : 21 Oct 2022 14:39  
Operator : JC/MD  
Sample : N5185-17  
Misc : 5.0mL/MSVOA\_X/WATER  
ALS Vial : 9 Sample Multiplier: 1

Instrument :  
MSVOA\_X  
ClientSampleId :  
PZ-02

Quant Method : Z:\voasrv\HPCHEM1\MSVOA\_X\Method\82X101922W.M  
Quant Title : SW846 8260

TIC Library : C:\Database\NIST20.L  
TIC Integration Parameters: LSCINT.P

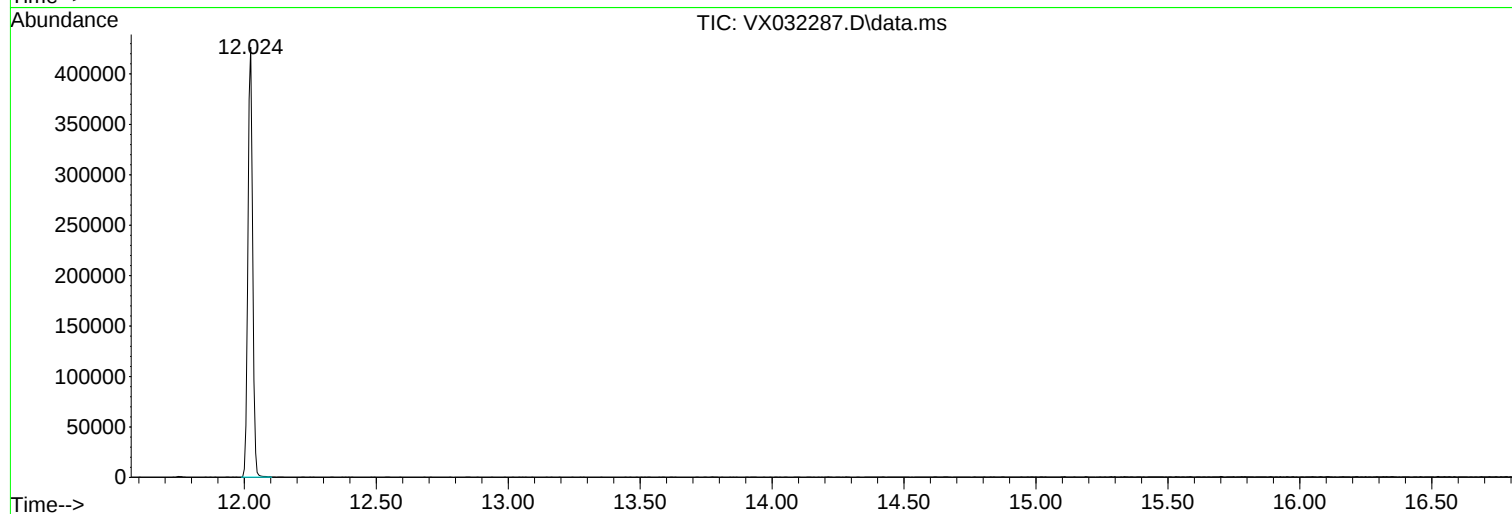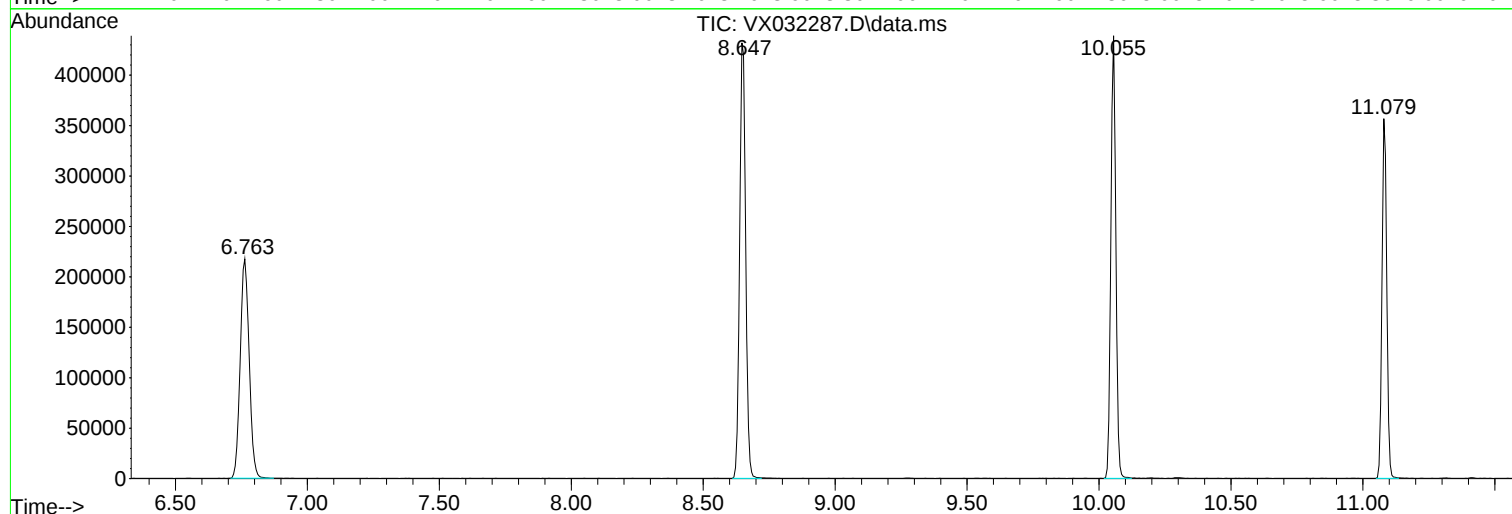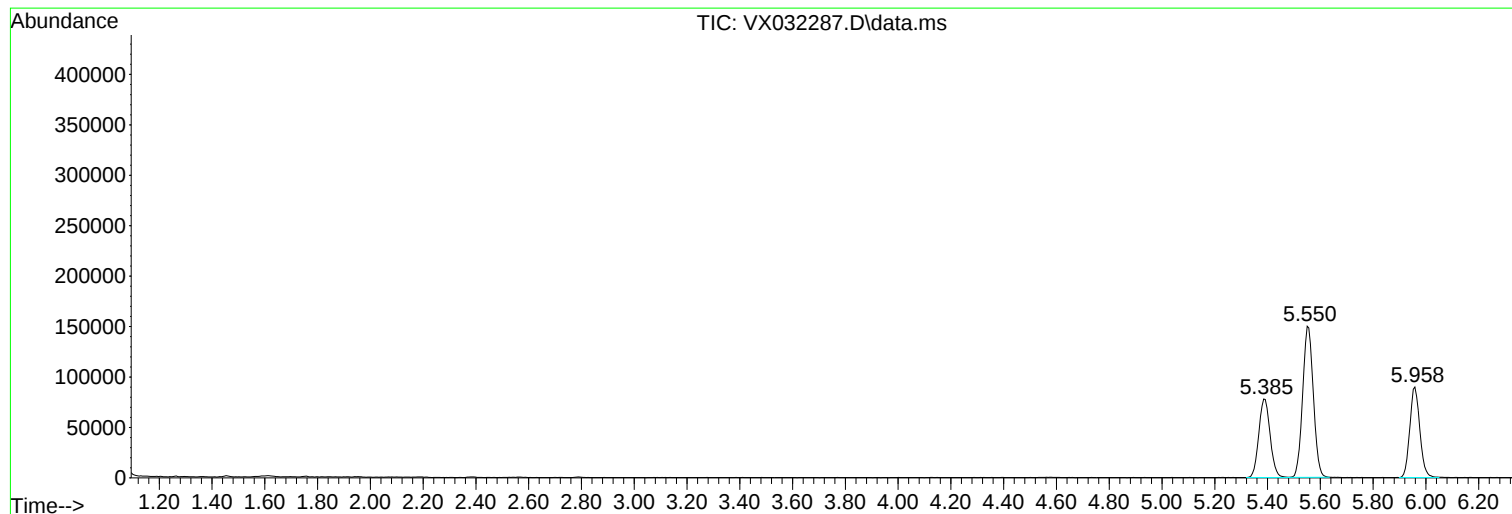

Data Path : Z:\voasrv\HPCHEM1\MSVOA\_X\Data\VX102122\  
Data File : VX032287.D  
Acq On : 21 Oct 2022 14:39  
Operator : JC/MD  
Sample : N5185-17  
Misc : 5.0mL/MSVOA\_X/WATER  
ALS Vial : 9 Sample Multiplier: 1

Instrument :  
MSVOA\_X  
ClientSampleId :  
PZ-02

Quant Method : Z:\voasrv\HPCHEM1\MSVOA\_X\Method\82X101922W.M  
Quant Title : SW846 8260

TIC Library : C:\Database\NIST20.L  
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

\*\*\*\*\*

Data Path : Z:\voasrv\HPCHEM1\MSVOA\_X\Data\VX102122\  
Data File : VX032287.D  
Acq On : 21 Oct 2022 14:39  
Operator : JC/MD  
Sample : N5185-17  
Misc : 5.0mL/MSVOA\_X/WATER  
ALS Vial : 9 Sample Multiplier: 1

Instrument :  
MSVOA\_X  
ClientSampleId :  
PZ-02

Quant Method : Z:\voasrv\HPCHEM1\MSVOA\_X\Method\82X101922W.M  
Quant Title : SW846 8260

TIC Library : C:\Database\NIST0.L  
TIC Integration Parameters: LSCINT.P

| TIC Top Hit name | RT | EstConc | Units | Response | # | RT | Resp | Conc |
|------------------|----|---------|-------|----------|---|----|------|------|
|------------------|----|---------|-------|----------|---|----|------|------|