

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX102122\
 Data File : VX032313.D
 Acq On : 22 Oct 2022 02:06
 Operator : JC/MD
 Sample : N5248-12
 Misc : 5.0mL/MSVOA_X/WATER
 ALS Vial : 37 Sample Multiplier: 1

Instrument :
 MSVOA_X
 ClientSampleId :
 FSND-FD-01-20221018

Integration Parameters: RTEINT.P

Integrator: RTE

Smoothing : ON

Filtering: 5

Sampling : 1

Min Area: 3 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\82X101922W.M
 Title : SW846 8260

Signal : TIC: VX032313.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	5.099	647	658	670	rBV3	6566	20138	2.82%	0.512%
2	5.385	695	705	720	rBV2	84623	247318	34.68%	6.294%
3	5.556	722	733	745	rVV	155882	443897	62.25%	11.296%
4	5.958	786	799	816	rBV	93292	248394	34.83%	6.321%
5	6.763	920	931	945	rBV	226184	540964	75.86%	13.766%
6	7.824	1097	1105	1116	rBV	11341	21491	3.01%	0.547%
7	8.647	1233	1240	1250	rBV	458765	713098	100.00%	18.146%
8	9.525	1379	1384	1392	rBV	13700	20741	2.91%	0.528%
9	10.055	1465	1471	1482	rBV	472816	618346	86.71%	15.735%
10	11.079	1634	1639	1652	rBV	371373	482196	67.62%	12.271%
11	12.024	1788	1794	1802	rBV	453435	573098	80.37%	14.584%


Sum of corrected areas: 3929681

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX102122\
Data File : VX032313.D
Acq On : 22 Oct 2022 02:06
Operator : JC/MD
Sample : N5248-12
Misc : 5.0mL/MSVOA_X/WATER
ALS Vial : 37 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
FSND-FD-01-20221018

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\82X101922W.M
Quant Title : SW846 8260

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

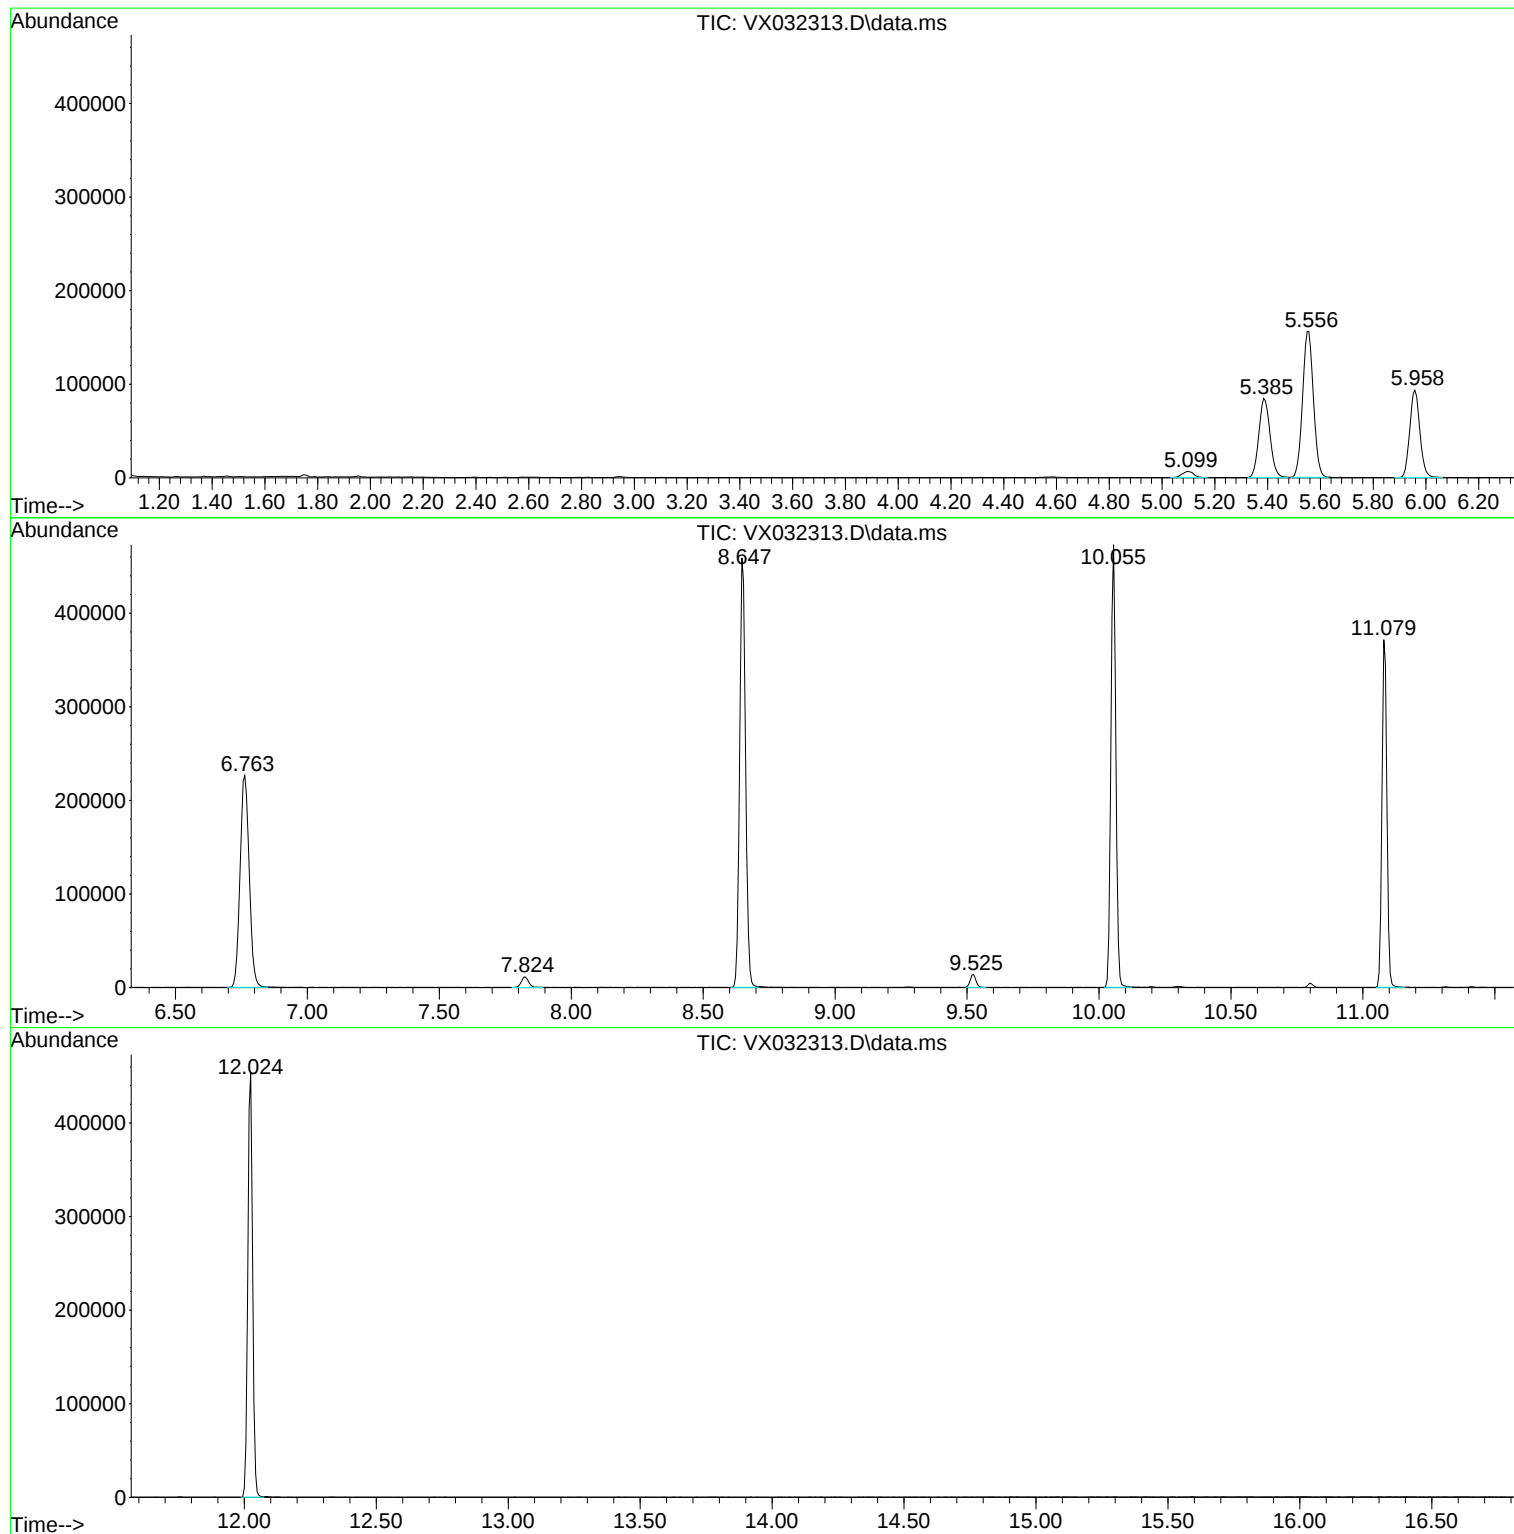

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX102122\
Data File : VX032313.D
Acq On : 22 Oct 2022 02:06
Operator : JC/MD
Sample : N5248-12
Misc : 5.0mL/MSVOA_X/WATER
ALS Vial : 37 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
FSND-FD-01-20221018

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\82X101922W.M
Quant Title : SW846 8260

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX102122\
Data File : VX032313.D
Acq On : 22 Oct 2022 02:06
Operator : JC/MD
Sample : N5248-12
Misc : 5.0mL/MSVOA_X/WATER
ALS Vial : 37 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
FSND-FD-01-20221018

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\82X101922W.M
Quant Title : SW846 8260

TIC Library : C:\Database\NIST0.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	#	RT	Resp	Conc
------------------	----	---------	-------	----------	---	----	------	------