

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX102122\
 Data File : VX032315.D
 Acq On : 22 Oct 2022 02:52
 Operator : JC/MD
 Sample : N5248-14
 Misc : 5.0mL/MSVOA_X/WATER
 ALS Vial : 39 Sample Multiplier: 1

Instrument :
 MSVOA_X
 ClientSampleId :
 FSND-MW-19-20221018

Integration Parameters: RTEINT.P

Integrator: RTE

Smoothing : ON

Filtering: 5

Sampling : 1

Min Area: 3 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\82X101922W.M

Title : SW846 8260

Signal : TIC: VX032315.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	2.941	298	304	313	rVB2	3924	9362	1.22%	0.218%
2	4.568	562	571	584	rBV2	2753	8775	1.14%	0.205%
3	5.391	691	706	722	rBV	97931	288975	37.52%	6.740%
4	5.550	722	732	748	rVB	167187	477914	62.05%	11.146%
5	5.958	789	799	816	rBV	100735	263495	34.21%	6.145%
6	6.763	920	931	945	rBV	244576	578199	75.07%	13.485%
7	7.129	984	991	1005	rBV2	32198	68741	8.92%	1.603%
8	8.647	1234	1240	1252	rBV	485797	770239	100.00%	17.964%
9	10.055	1465	1471	1483	rBV	513264	667312	86.64%	15.563%
10	11.079	1634	1639	1650	rBV	412137	522437	67.83%	12.184%
11	12.024	1788	1794	1803	rBV	507115	632311	82.09%	14.747%




Sum of corrected areas: 4287760

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX102122\
Data File : VX032315.D
Acq On : 22 Oct 2022 02:52
Operator : JC/MD
Sample : N5248-14
Misc : 5.0mL/MSVOA_X/WATER
ALS Vial : 39 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
FSND-MW-19-20221018

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\82X101922W.M
Quant Title : SW846 8260

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

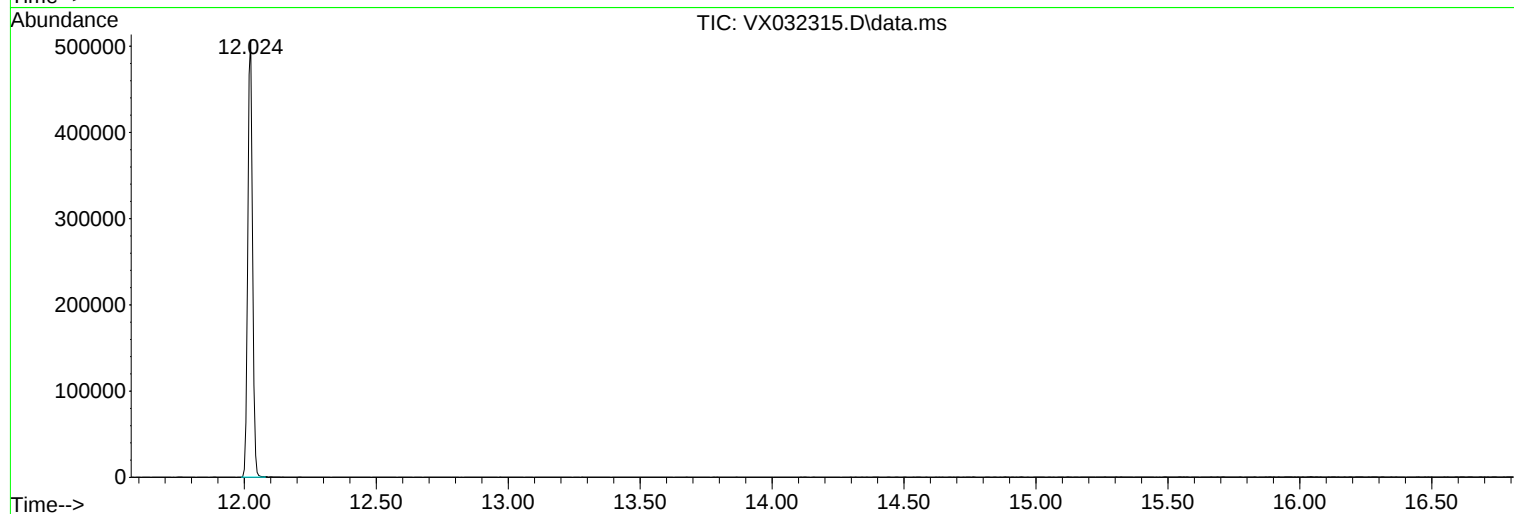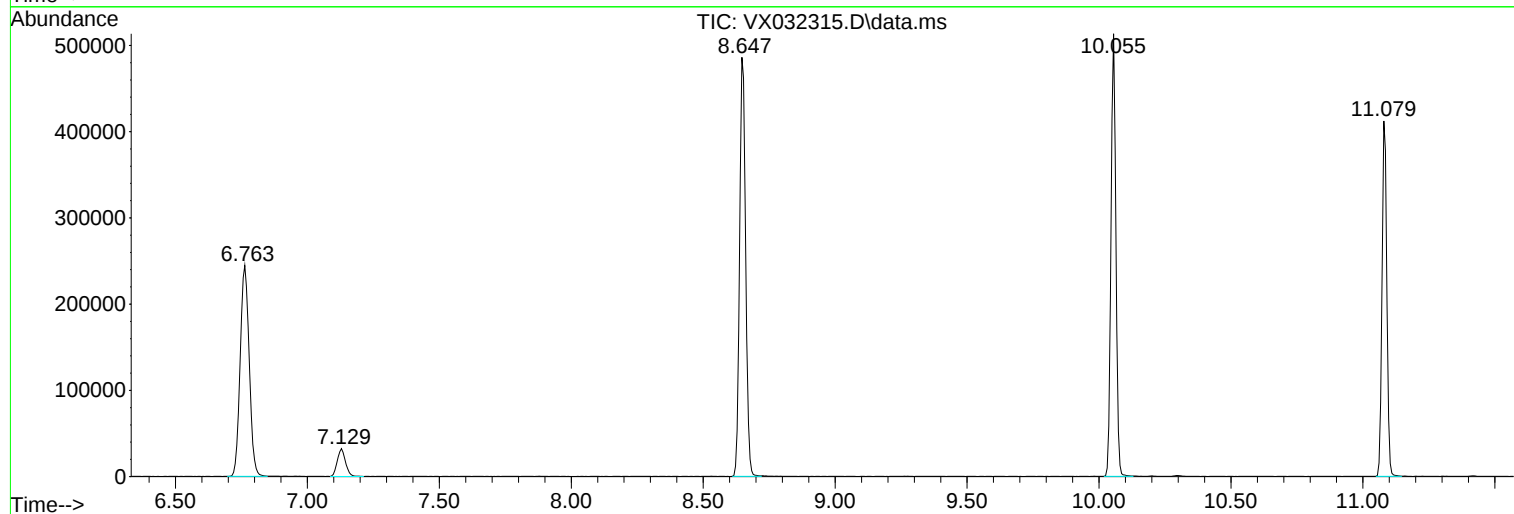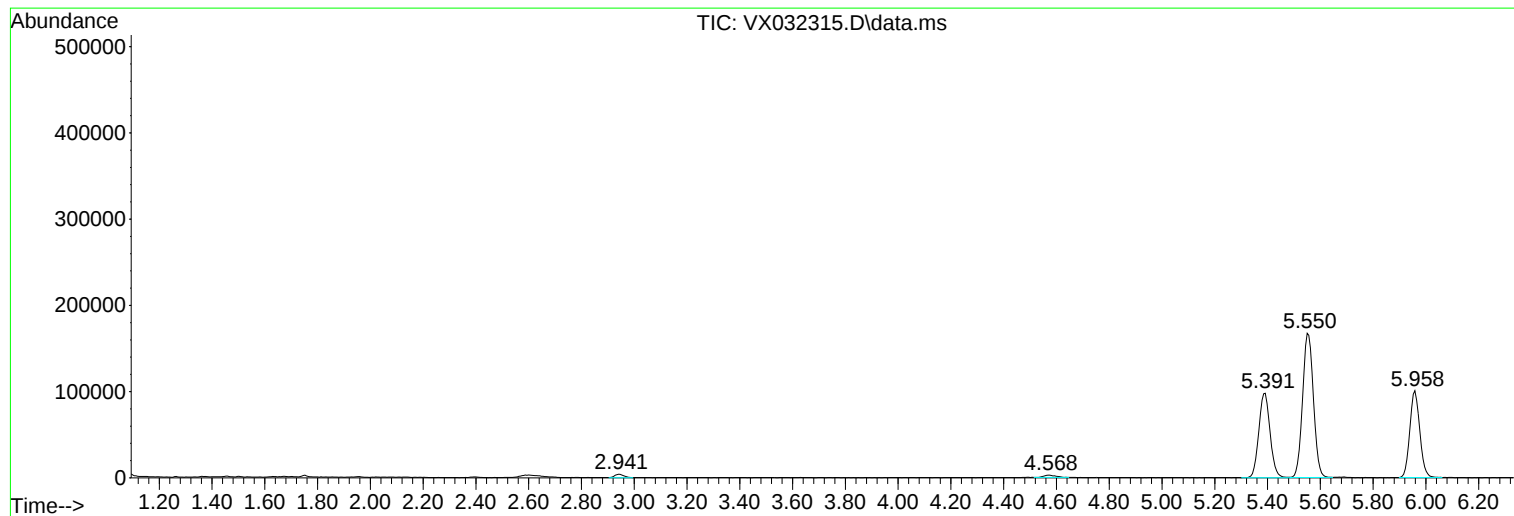

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX102122\
Data File : VX032315.D
Acq On : 22 Oct 2022 02:52
Operator : JC/MD
Sample : N5248-14
Misc : 5.0mL/MSVOA_X/WATER
ALS Vial : 39 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
FSND-MW-19-20221018

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\82X101922W.M
Quant Title : SW846 8260

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX102122\
Data File : VX032315.D
Acq On : 22 Oct 2022 02:52
Operator : JC/MD
Sample : N5248-14
Misc : 5.0mL/MSVOA_X/WATER
ALS Vial : 39 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
FSND-MW-19-20221018

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\82X101922W.M
Quant Title : SW846 8260

TIC Library : C:\Database\NIST0.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	#	RT	Resp	Conc
------------------	----	---------	-------	----------	---	----	------	------