

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX102122\
Data File : VX032320.D
Acq On : 22 Oct 2022 04:48
Operator : JC/MD
Sample : N5248-19
Misc : 5.0mL/MSVOA_X/WATER
ALS Vial : 44 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
FSND-MW-15-20221019

Integration Parameters: RTEINT.P

Integrator: RTE

Smoothing : ON

Filtering: 5

Sampling : 1

Min Area: 3 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\82X101922W.M

Title : SW846 8260

Signal : TIC: VX032320.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	5.385	694	705	718	rBV2	97736	287292	19.85%	5.315%
2	5.556	721	733	747	rVV	156463	443511	30.64%	8.206%
3	5.958	788	799	817	rBV	95961	249447	17.23%	4.615%
4	6.763	919	931	944	rBV	229731	543500	37.54%	10.056%
5	7.129	980	991	1008	rBV	661245	1447619	100.00%	26.783%
6	8.647	1234	1240	1250	rBV	455777	720887	49.80%	13.338%
7	10.055	1465	1471	1482	rBV	471650	629444	43.48%	11.646%
8	11.079	1634	1639	1651	rBV	379404	489909	33.84%	9.064%
9	12.024	1788	1794	1803	rBV	484867	593320	40.99%	10.977%




Sum of corrected areas: 5404929

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX102122\
Data File : VX032320.D
Acq On : 22 Oct 2022 04:48
Operator : JC/MD
Sample : N5248-19
Misc : 5.0mL/MSVOA_X/WATER
ALS Vial : 44 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
FSND-MW-15-20221019

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\82X101922W.M
Quant Title : SW846 8260

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

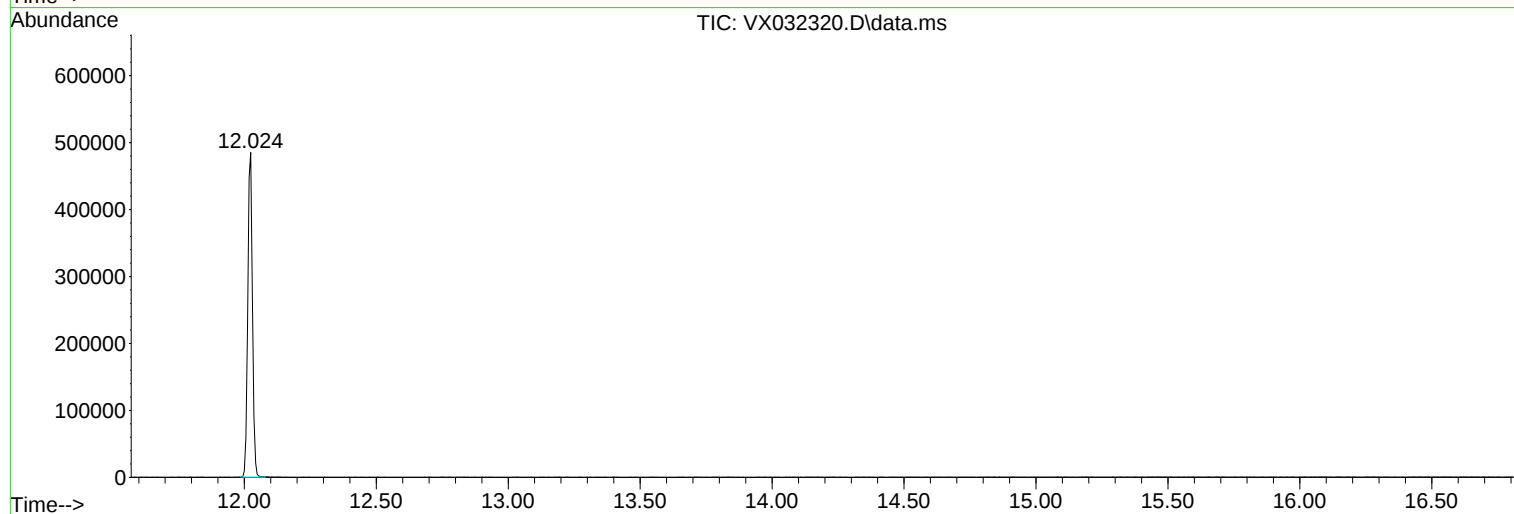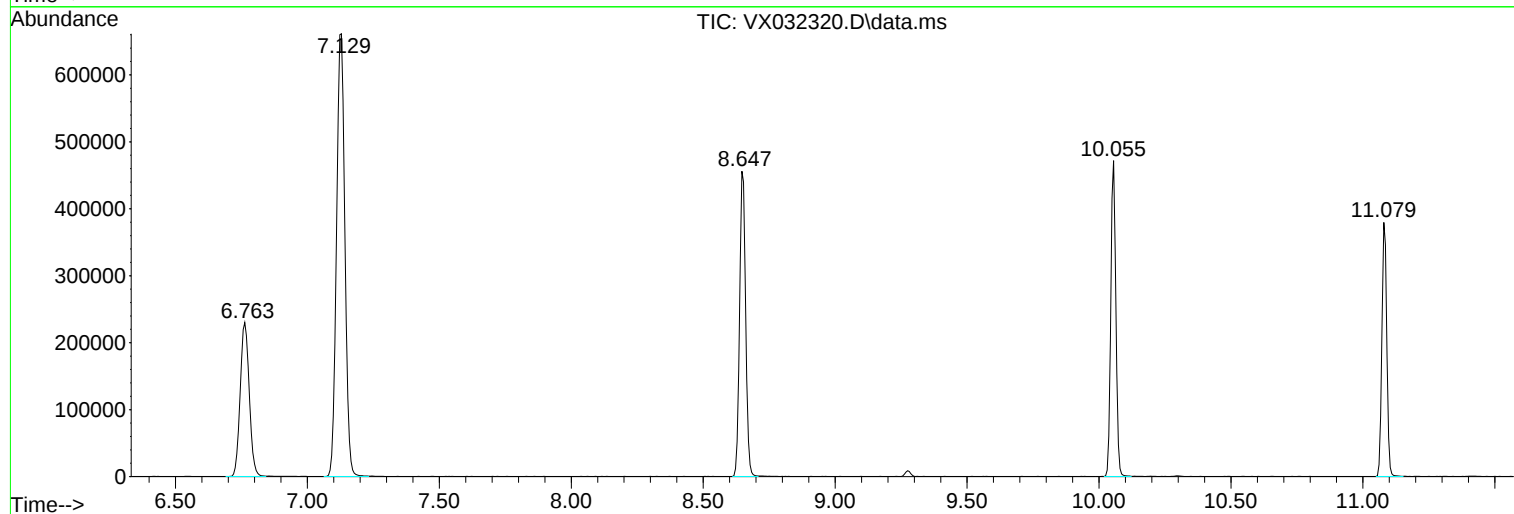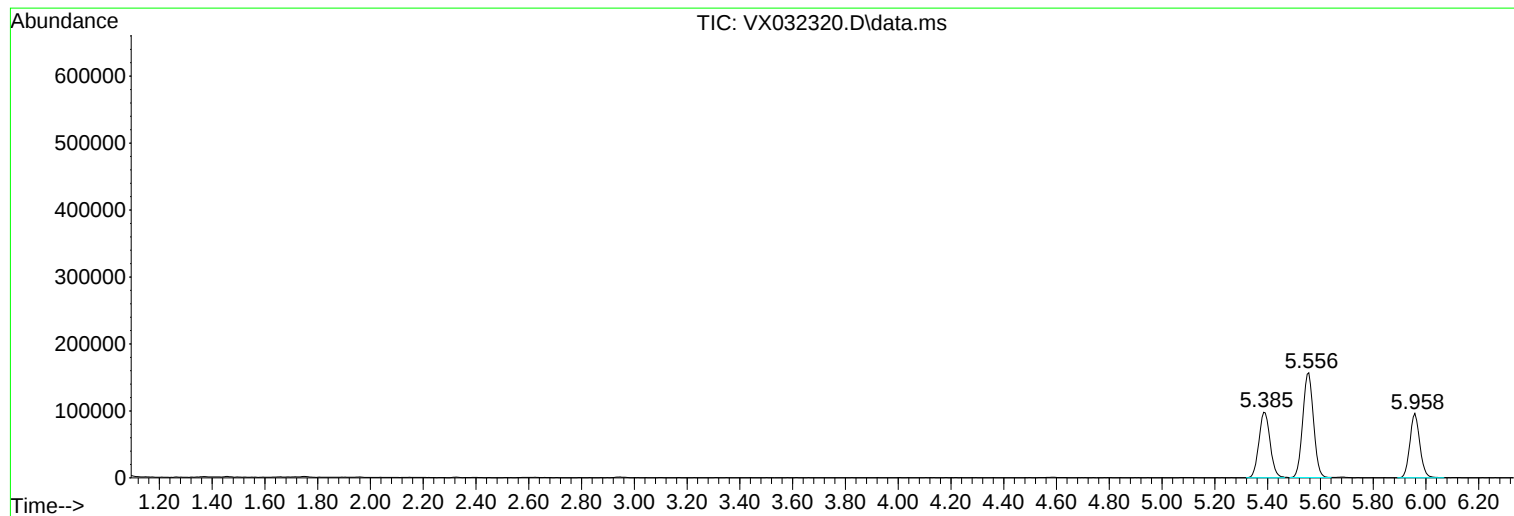

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX102122\
Data File : VX032320.D
Acq On : 22 Oct 2022 04:48
Operator : JC/MD
Sample : N5248-19
Misc : 5.0mL/MSVOA_X/WATER
ALS Vial : 44 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
FSND-MW-15-20221019

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\82X101922W.M
Quant Title : SW846 8260

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX102122\
Data File : VX032320.D
Acq On : 22 Oct 2022 04:48
Operator : JC/MD
Sample : N5248-19
Misc : 5.0mL/MSVOA_X/WATER
ALS Vial : 44 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
FSND-MW-15-20221019

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\82X101922W.M
Quant Title : SW846 8260

TIC Library : C:\Database\NIST0.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	#	RT	Resp	Conc
------------------	----	---------	-------	----------	---	----	------	------