
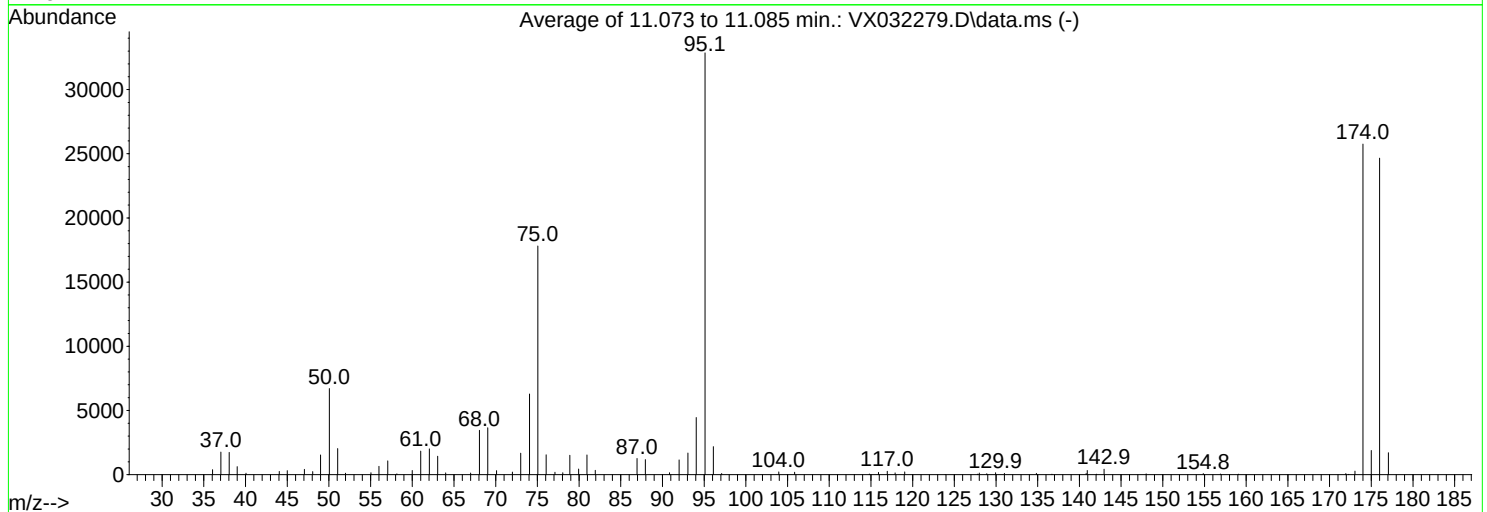


Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX102122\
Data File : VX032279.D
Acq On : 21 Oct 2022 10:38
Operator : JC/MD
Sample : BFB
Misc : 5.0mL/MSVOA_X/WATER
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
BFB

Integration File: RTEINT.P

Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\82X101922W.M
Title : SW846 8260
Last Update : Sat Oct 22 04:56:40 2022

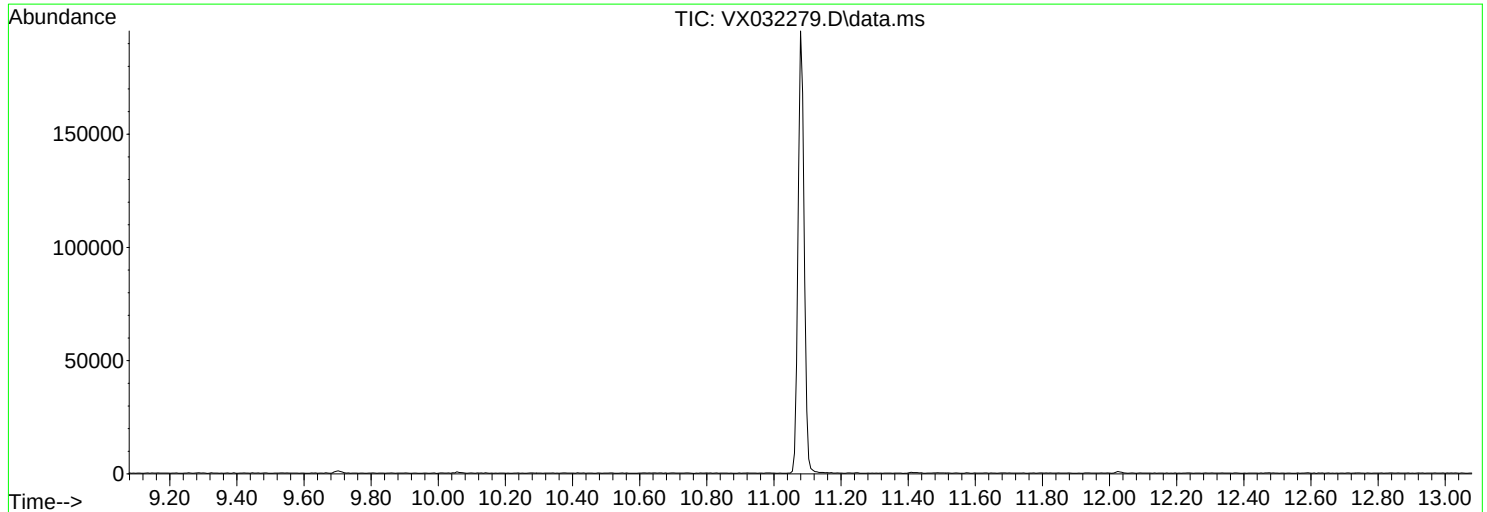

AutoFind: Scans 1638, 1639, 1640; Background Corrected with Scan 1632

Target	Rel. to	Lower	Upper	Rel.	Raw	Result
Mass	Mass	Limit%	Limit%	Abn%	Abn	Pass/Fail
50	95	15	40	20.4	6704	PASS
75	95	30	60	54.2	17817	PASS
95	95	100	100	100.0	32861	PASS
96	95	5	9	6.6	2181	PASS
173	174	0.00	2	1.1	278	PASS
174	95	50	100	78.4	25757	PASS
175	174	5	9	7.3	1885	PASS
176	174	95	101	95.7	24659	PASS
177	176	5	9	6.9	1705	PASS