


Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX102122\
Data File : VX032306.D
Acq On : 21 Oct 2022 22:21
Operator : JC/MD
Sample : BFB
Misc : 5.0mL/MSVOA_X/WATER
ALS Vial : 29 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
BFB

Integration File: RTEINT.P

Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\82X101922W.M
Title : SW846 8260
Last Update : Sat Oct 22 04:56:40 2022

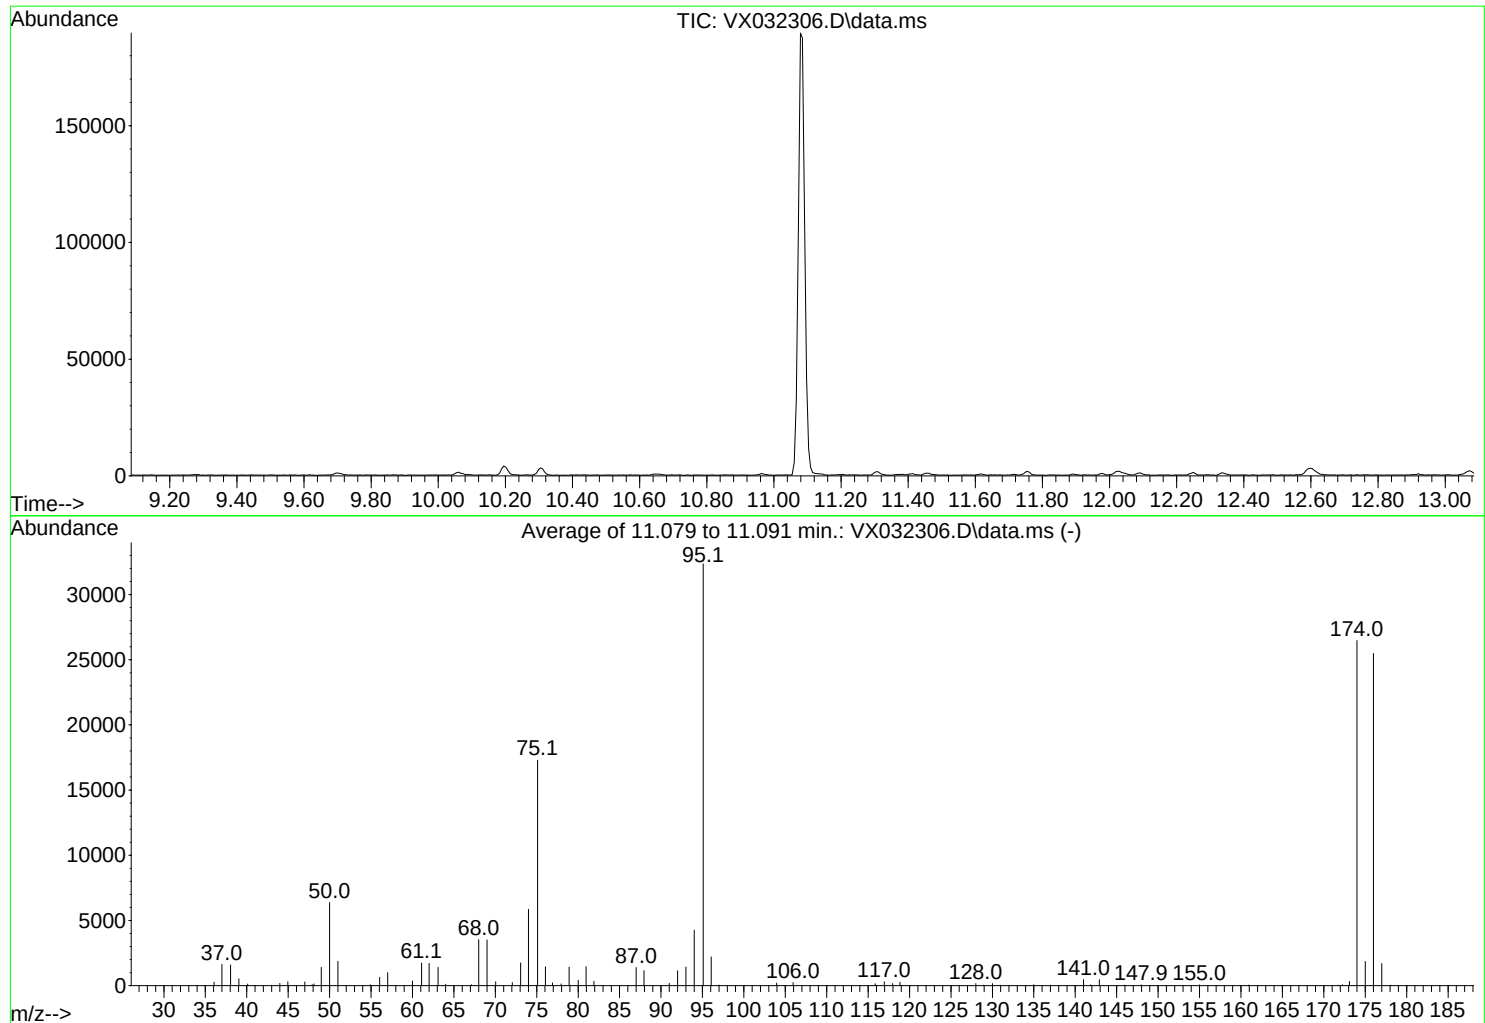

AutoFind: Scans 1639, 1640, 1641; Background Corrected with Scan 1632

Target	Rel. to	Lower	Upper	Rel.	Raw	Result
Mass	Mass	Limit%	Limit%	Abn%	Abn	Pass/Fail
50	95	15	40	19.7	6370	PASS
75	95	30	60	53.4	17293	PASS
95	95	100	100	100.0	32355	PASS
96	95	5	9	6.8	2206	PASS
173	174	0.00	2	1.2	316	PASS
174	95	50	100	81.8	26472	PASS
175	174	5	9	7.0	1849	PASS
176	174	95	101	96.2	25475	PASS
177	176	5	9	6.6	1688	PASS