


Data Path : Z:\voasrv\HPCHEM1\MSVOA X\Data\VX102218\
 Data File : VX005489.D
 Acq On : 23 Oct 2018 00:06
 Operator : JC/MD
 Sample : BFB
 Misc : 5.0mL/MSVOA X/WATER
 ALS Vial : 26 Sample Multiplier: 1

Instrument :
 MSVOA_X
 ClientSampleId :
 BFB

Integration File: RTEINT.P

Method : Z:\VOASRV\HPCHEM1\MSVOA_X\METHOD\82X101218W.M
 Title : SW846 8260
 Last Update : Fri Oct 12 11:28:43 2018

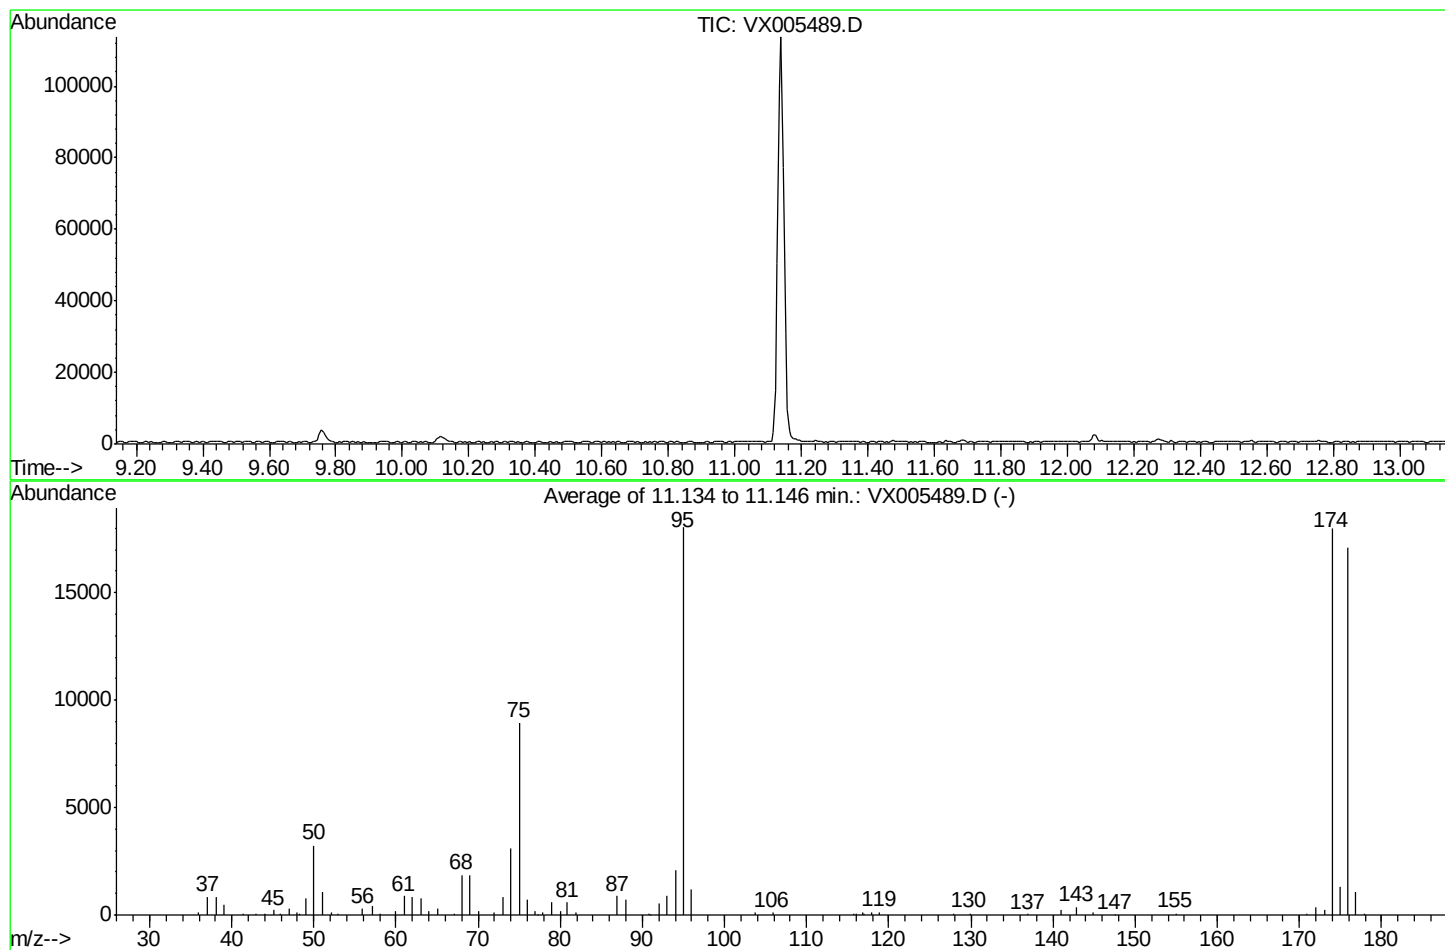

AutoFind: Scans 1637, 1638, 1639; Background Corrected with Scan 1631

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	15	40	17.9	3229	PASS
75	95	30	60	49.5	8937	PASS
95	95	100	100	100.0	18041	PASS
96	95	5	9	6.6	1192	PASS
173	174	0.00	2	1.5	262	PASS
174	95	50	100	99.7	17979	PASS
175	174	5	9	7.4	1327	PASS
176	174	95	101	95.0	17072	PASS
177	176	5	9	6.4	1101	PASS