

Data Path : Z:\VOASRV\HPCHEM1\MSVOA X\DATA\VX102220\
 Data File : VX019063.D
 Acq On : 23 Oct 2020 05:48
 Operator : JC/SP
 Sample : L4484-02
 Misc : 5.0mL/MSVOA X/WATER
 ALS Vial : 54 Sample Multiplier: 1

Instrument :
 MSVOA_X
 ClientSampleId :
 72-11998

Quant Time: Oct 23 08:42:45 2020
 Quant Method : Z:\VOASRV\HPCHEM1\MSVOA_X\METHOD\82X102120W.M
 Quant Title : SW846 8260
 QLast Update : Thu Oct 22 17:51:42 2020
 Response via : Initial Calibration

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) Pentafluorobenzene	5.63	168	278475	50.00	ug/l	0.00
34) 1,4-Difluorobenzene	6.83	114	479700	50.00	ug/l	0.00
63) Chlorobenzene-d5	10.10	117	470210	50.00	ug/l	0.00
72) 1,4-Dichlorobenzene-d4	12.06	152	237290	50.00	ug/l	0.00

System Monitoring Compounds	R.T.	QIon	Response	Conc	Units	Dev(Min)
33) 1,2-Dichloroethane-d4	6.03	65	169961	50.95	ug/l	0.00
Spiked Amount			Recovery	=	101.90%	
35) Dibromofluoromethane	5.46	113	150277	49.48	ug/l	0.00
Spiked Amount			Recovery	=	98.96%	
50) Toluene-d8	8.70	98	597553	51.56	ug/l	0.00
Spiked Amount			Recovery	=	103.12%	
62) 4-Bromofluorobenzene	11.12	95	214814	52.11	ug/l	0.00
Spiked Amount			Recovery	=	104.22%	


Target Compounds	R.T.	QIon	Response	Conc	Units	Qvalue
5) Bromomethane	1.64	94	163	Below Cal		91
6) Chloroethane	1.67	64	157	1.328	ug/l #	66
10) Methyl Iodide	2.48	142	20	4.775	ug/l #	42
11) Tert butyl alcohol	3.00	59	2276	3.369	ug/l #	73
13) Acrolein	2.34	56	164	14.234	ug/l	97
16) Acetone	2.42	43	10587	9.318	ug/l	99
18) Methyl Acetate	2.75	43	2781	0.986	ug/l	99
20) Methylene Chloride	2.84	84	6121	1.935	ug/l	95
25) 2-Butanone	4.65	43	2091	1.165	ug/l #	86
29) Tetrahydrofuran	5.11	42	759	0.707	ug/l #	48
36) 1,1-Dichloropropene	5.62	75	19859	4.614	ug/l #	44
38) Carbon Tetrachloride	5.63	117	26895	5.953	ug/l #	16
43) Isopropyl Acetate	6.41	43	62161	9.991	ug/l	99
48) Methyl methacrylate	7.65	41	3306	1.078	ug/l #	5
49) 1,4-Dioxane	7.84	88	228	3.292	ug/l #	1
51) 4-Methyl-2-Pentanone	8.59	43	61412	16.750	ug/l #	46
52) Toluene	8.77	92	4378	0.523	ug/l	99
54) cis-1,3-Dichloropropene	8.59	75	35218	6.504	ug/l #	60
57) 1,3-Dichloropropane	9.52	76	5988	1.105	ug/l #	42
59) 2-Hexanone	9.42	43	55592	20.347	ug/l #	17
67) Ethyl Benzene	10.23	91	6858	0.403	ug/l	99
68) m/p-Xylenes	10.34	106	2354	0.361	ug/l	96
74) N-ethyl acetate	10.81	43	2832	0.518	ug/l #	41
76) 1,2,3-Trichloropropane	11.12	75	107872	22.745	ug/l #	36
81) trans-1,4-Dichloro-2-buten	11.12	75	107872	57.948	ug/l #	15
84) 1,2,4-Trimethylbenzene	11.79	105	3560	0.252	ug/l	98


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\V0ASRV\HPCHEM1\MSVOA X\DATA\VX102220\
Data File : VX019063.D
Acq On : 23 Oct 2020 05:48
Operator : JC/SP
Sample : L4484-02
Misc : 5.0mL/MSVOA X/WATER
ALS Vial : 54 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
72-11998

Quant Time: Oct 23 08:42:45 2020
Quant Method : Z:\V0ASRV\HPCHEM1\MSVOA_X\METHOD\82X102120W.M
Quant Title : SW846 8260
QLast Update : Thu Oct 22 17:51:42 2020
Response via : Initial Calibration

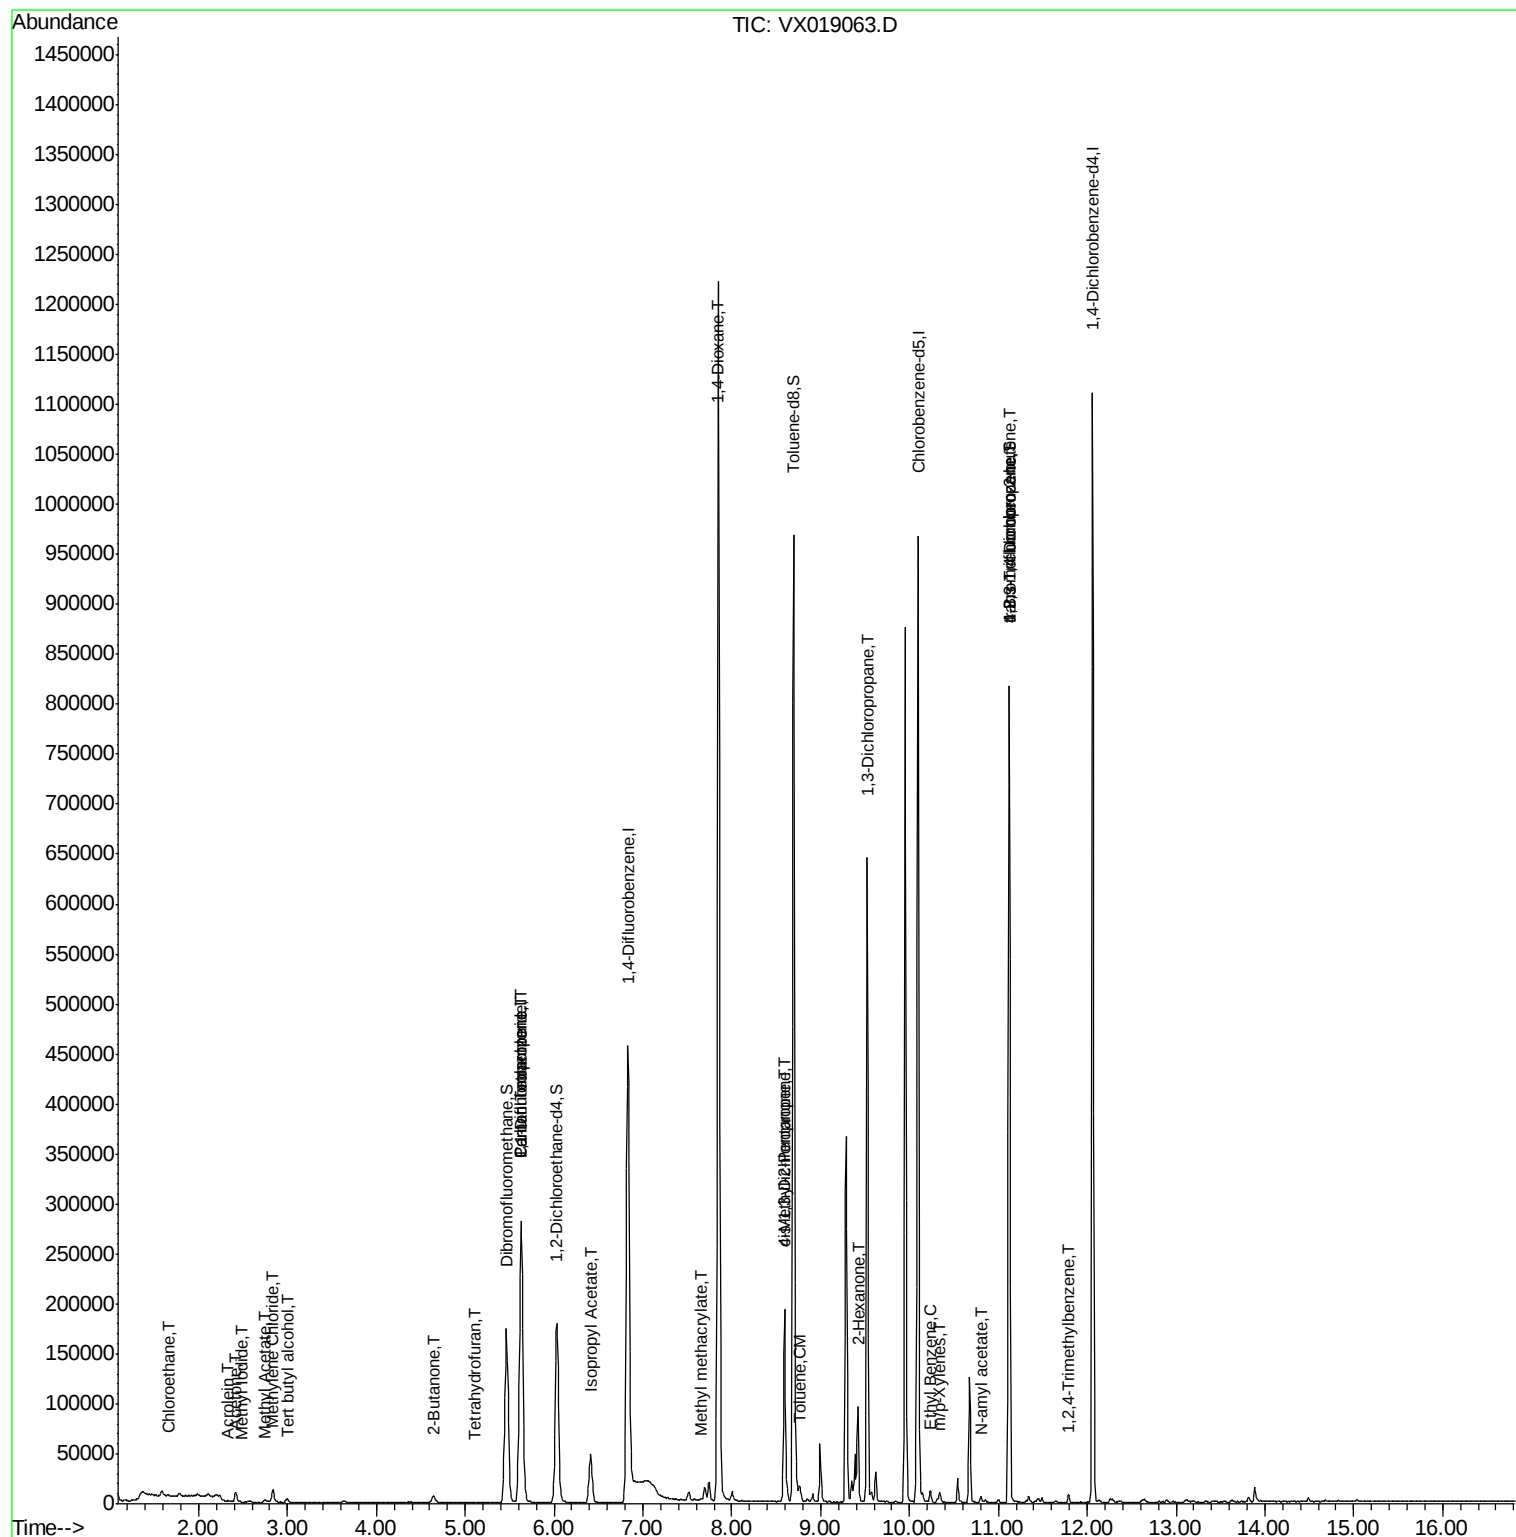

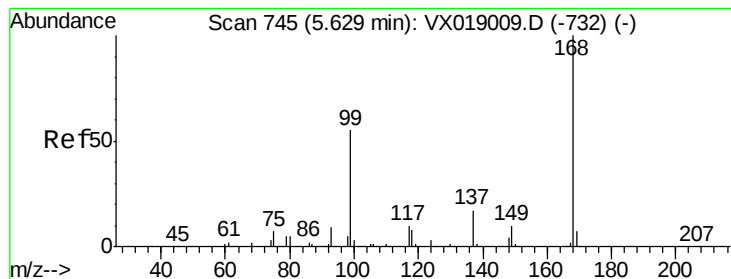

#1

Pentafluorobenzene

Concen: 50.000 ug/l

RT: 5.63 min Scan# 745

Delta R.T. 0.00 min

Lab File: VX019063.D

Acq: 23 Oct 2020 05:48

Instrument :

MSVOA_X

ClientSampleId :


72-11998

Tot Ion:168 Resp: 278475

Ion Ratio Lower Upper




168 100

99 54.9 44.2 66.2



Abundance Ion 167.90 (167.60 to 168.60): V

Ion 98.90 (98.60 to 99.60): VX0

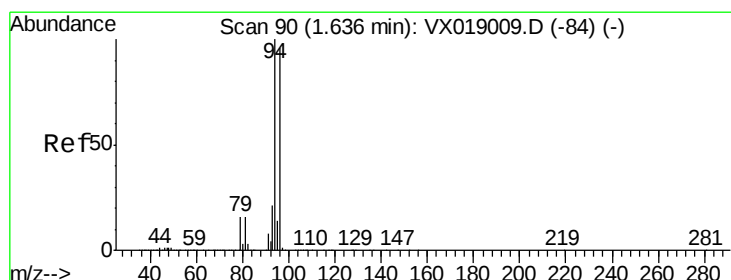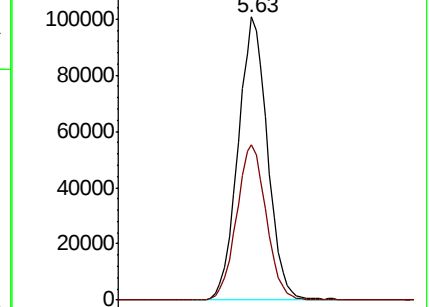

#5

Bromomethane

Concen: Below Cal

RT: 1.64 min Scan# 91

Delta R.T. 0.01 min

Lab File: VX019063.D


Acq: 23 Oct 2020 05:48

Tgt Ion: 94 Resp: 163

Ion Ratio Lower Upper



94 100


96 87.5 77.1 115.7



Abundance Ion 93.90 (93.60 to 94.60): VX0

Ion 95.90 (95.60 to 96.60): VX0




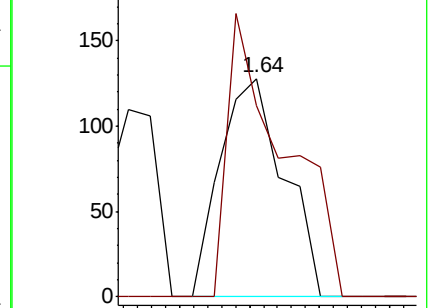




#6
Chloroethane
Concen: 1.328 ug/l
RT: 1.67 min Scan# 95
Delta R.T. -0.04 min
Lab File: VX019063.D
Acq: 23 Oct 2020 05:48




Instrument :
MSVOA_X
ClientSampleId :
72-11998


Tot Ion: 64 Resp: 157
Ion Ratio Lower Upper
64 100
66 13.1 25.7 38.5#

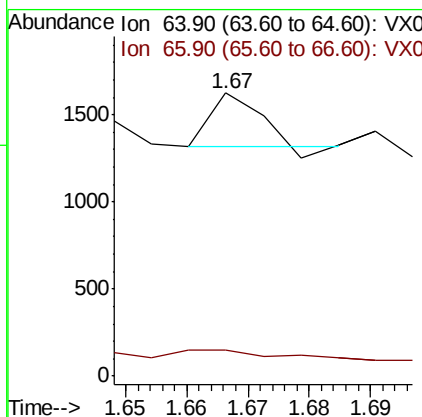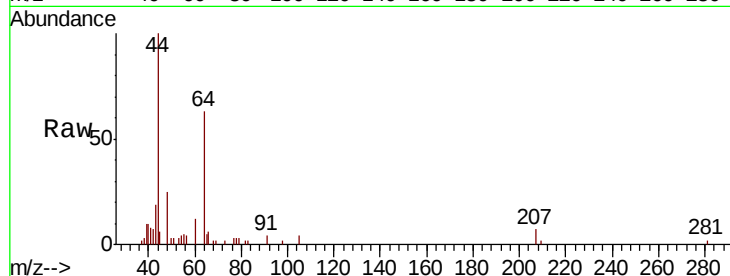

#10
Methyl Iodide
Concen: 4.775 ug/l
RT: 2.48 min Scan# 229
Delta R.T. -0.01 min
Lab File: VX019063.D
Acq: 23 Oct 2020 05:48

Tgt Ion: 142 Resp: 20
Ion Ratio Lower Upper
142 100
127 0.0 33.6 50.4#
141 0.0 11.2 16.8#



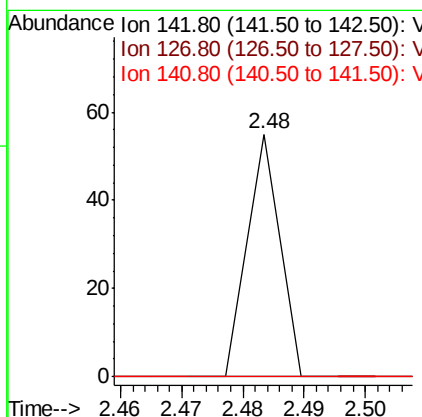



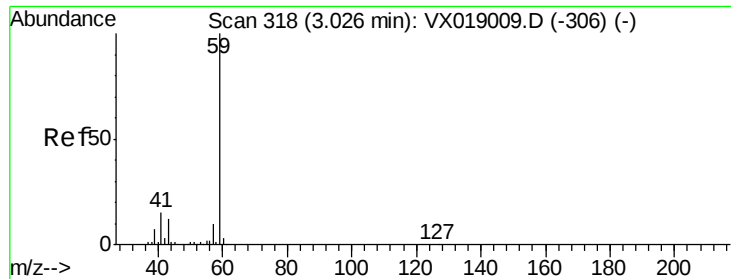

#11
Tert butyl alcohol
Concen: 3.369 ug/l
RT: 3.00 min Scan# 313
Delta R.T. -0.03 min
Lab File: VX019063.D
Acq: 23 Oct 2020 05:48




Instrument :
MSVOA_X
ClientSampleId :
72-11998


Tot Ion: 59 Resp: 2276
Ion Ratio Lower Upper
59 100
57 0.0 8.2 12.2#

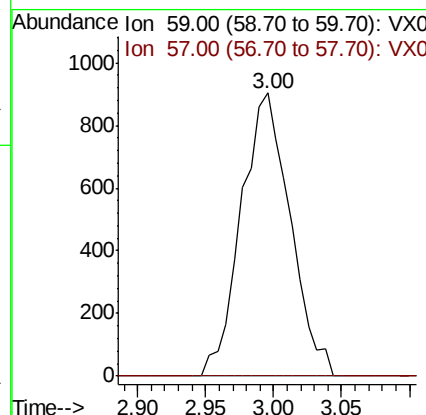

#13
Acrolein
Concen: 14.234 ug/l
RT: 2.34 min Scan# 205
Delta R.T. 0.06 min
Lab File: VX019063.D
Acq: 23 Oct 2020 05:48

Tgt Ion: 56 Resp: 164
Ion Ratio Lower Upper
56 100
55 70.1 54.2 81.4

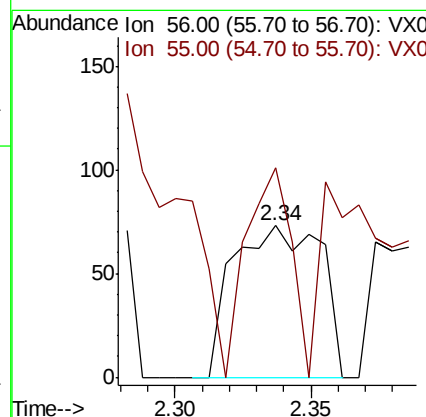

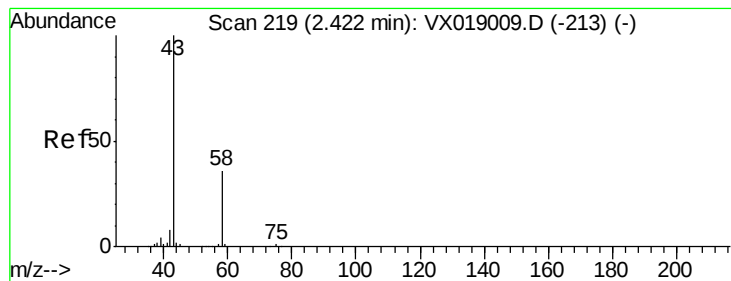

#16

Acetone

Concen: 9.318 ug/l

RT: 2.42 min Scan# 218

Delta R.T. -0.01 min

Lab File: VX019063.D

Acq: 23 Oct 2020 05:48

Instrument :

MSVOA_X

ClientSampleId :





72-11998

Tot Ion: 43 Resp: 10587

Ion Ratio Lower Upper

43 100

58 36.3 28.6 42.8

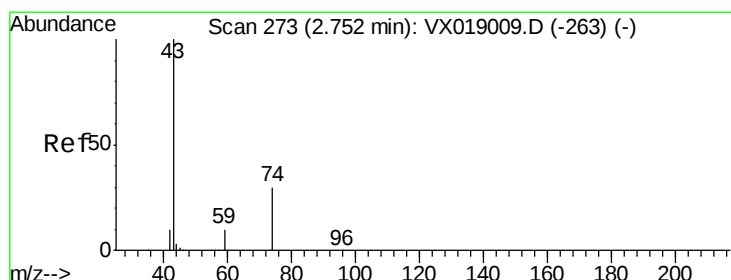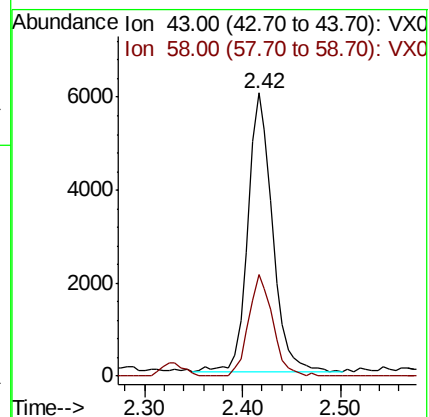

#18

Methyl Acetate

Concen: 0.986 ug/l

RT: 2.75 min Scan# 272

Delta R.T. -0.01 min

Lab File: VX019063.D




Acq: 23 Oct 2020 05:48


Tgt Ion: 43 Resp: 2781

Ion Ratio Lower Upper

43 100

74 31.9 24.9 37.3



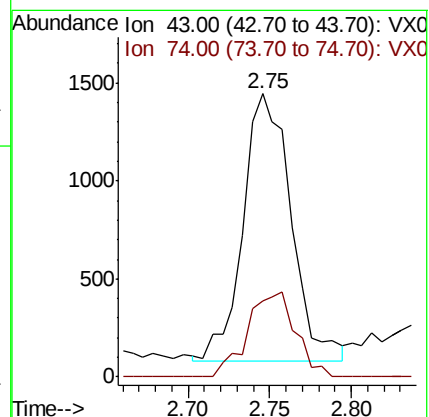





#20
Methvlene Chloride
Concen: 1.935 ug/l
RT: 2.84 min Scan# 287
Delta R.T. 0.00 min
Lab File: VX019063.D
Acq: 23 Oct 2020 05:48




Instrument :
MSVOA_X
ClientSampled :
72-11998


Tot Ion:	84	Resp:	6121
Ion	Ratio	Lower	Upper
84	100		
49	108.6	81.6	122.4
51	33.5	25.6	38.4
86	69.8	53.3	79.9

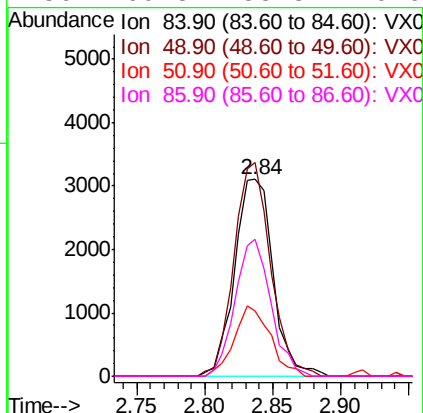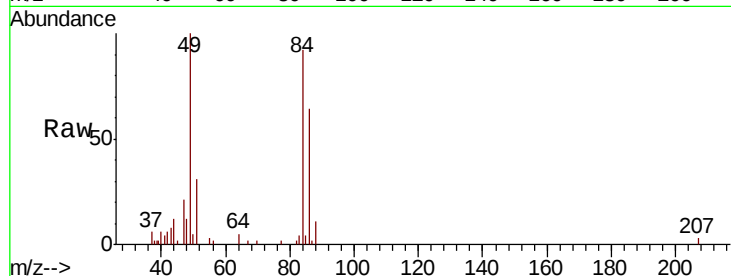

#25
2-Butanone
Concen: 1.165 ug/l
RT: 4.65 min Scan# 584
Delta R.T. 0.01 min
Lab File: VX019063.D
Acq: 23 Oct 2020 05:48

Tgt Ion:	43	Resp:	2091
Ion	Ratio	Lower	Upper
43	100		
72	26.4	27.8	41.6#


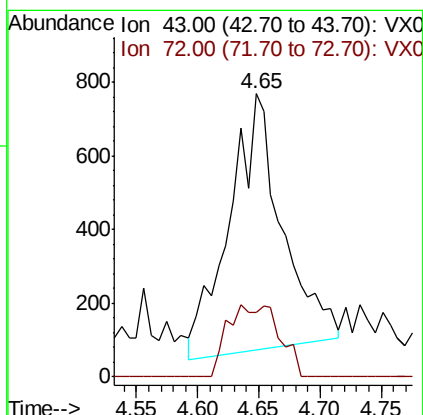






#29
Tetrahydrofuran
Concen: 0.707 ug/l
RT: 5.11 min Scan# 660
Delta R.T. 0.02 min
Lab File: VX019063.D
Acq: 23 Oct 2020 05:48




Instrument :
MSVOA_X
ClientSampleId :
72-11998


Tot Ion: 42 Resp: 759
Ion Ratio Lower Upper
42 100
72 20.8 49.1 73.7#
71 17.9 44.2 66.4#

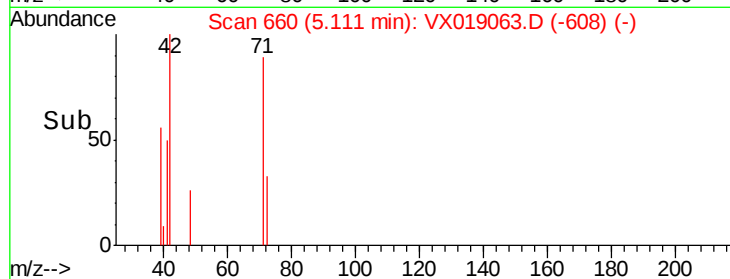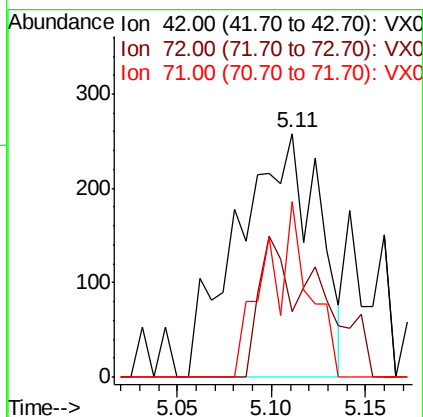

#33
1,2-Dichloroethane-d4
Concen: 50.952 ug/l
RT: 6.03 min Scan# 811
Delta R.T. 0.00 min
Lab File: VX019063.D
Acq: 23 Oct 2020 05:48

Tgt Ion: 65 Resp: 169961
Ion Ratio Lower Upper
65 100
67 52.4 0.0 107.0

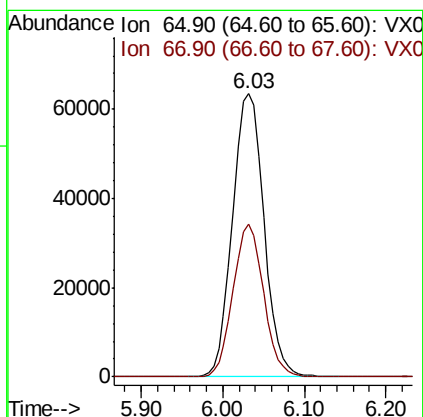


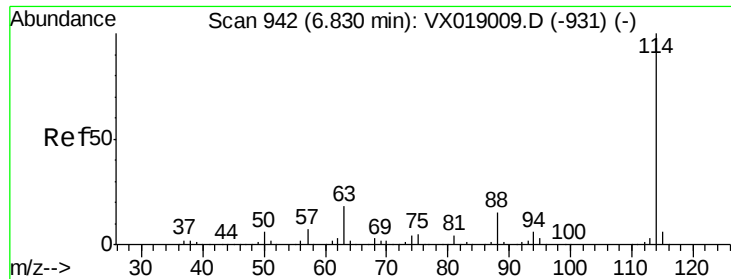




#34
1,4-Difluorobenzene
Concen: 50.000 ug/l
RT: 6.83 min Scan# 942
Delta R.T. 0.00 min
Lab File: VX019063.D
Acq: 23 Oct 2020 05:48

Instrument :
MSVOA_X
ClientSampled :
72-11998

Tot Ion:114 Resp: 479700
Ion Ratio Lower Upper
114 100
63 18.0 0.0 36.8
88 15.2 0.0 30.2




Abundance Ion 113.90 (113.60 to 114.60): V
Ion 63.00 (62.70 to 63.70): VX0
Ion 87.90 (87.60 to 88.60): VX0

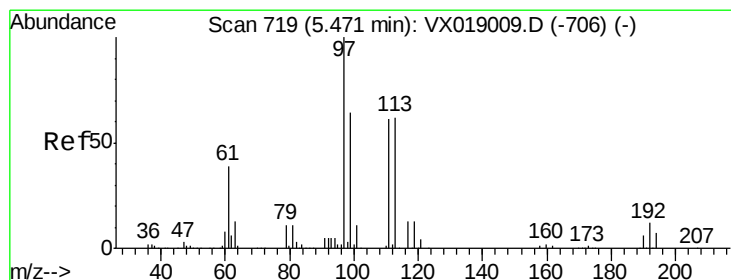
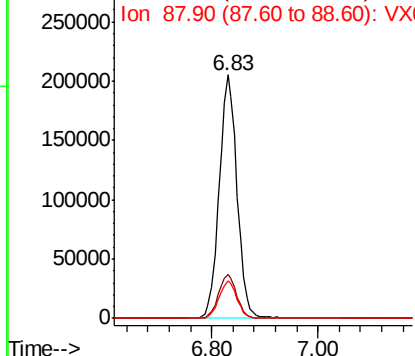



#35
Dibromofluoromethane
Concen: 49.480 ug/l
RT: 5.46 min Scan# 718
Delta R.T. -0.01 min
Lab File: VX019063.D
Acq: 23 Oct 2020 05:48

Tgt Ion:113 Resp: 150277
Ion Ratio Lower Upper
113 100
111 102.2 81.5 122.3
192 20.5 16.3 24.5



Abundance Ion 112.80 (112.50 to 113.50): V
Ion 110.80 (110.50 to 111.50): V
Ion 191.70 (191.40 to 192.40): V

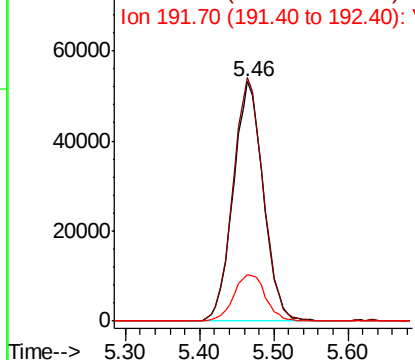

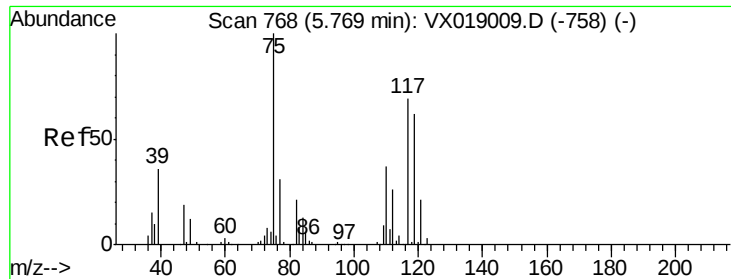

#36

1,1-Dichloropropene

Concen: 4.614 ug/l

RT: 5.62 min Scan# 744

Delta R.T. -0.15 min

Lab File: VX019063.D

Acq: 23 Oct 2020 05:48

Instrument :

MSVOA_X

ClientSampleId :

72-11998


Tot Ion: 75 Resp: 19859

Ion Ratio Lower Upper

75 100

110 5.3 19.4 58.2#




77 0.0 25.2 37.8#

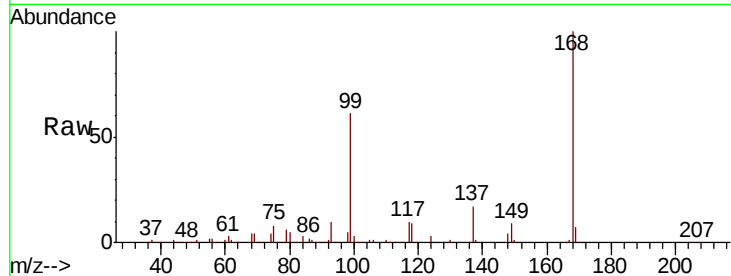

Abundance Ion 74.90 (74.60 to 75.60): VX0

Ion 109.90 (109.60 to 110.60): V

Ion 76.90 (76.60 to 77.60): VX0

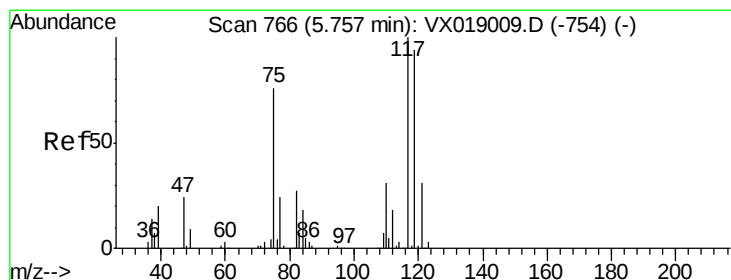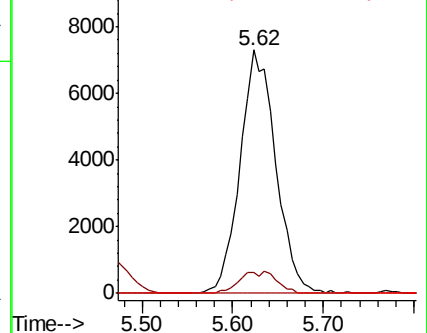

#38

Carbon Tetrachloride

Concen: 5.953 ug/l

RT: 5.63 min Scan# 745

Delta R.T. -0.13 min

Lab File: VX019063.D

Acq: 23 Oct 2020 05:48


Tgt Ion: 117 Resp: 26895

Ion Ratio Lower Upper

117 100

119 3.7 75.4 113.0#



121 0.0 25.0 37.6#




Abundance Ion 116.80 (116.50 to 117.50): V

Ion 118.80 (118.50 to 119.50): V

Ion 120.80 (120.50 to 121.50): V

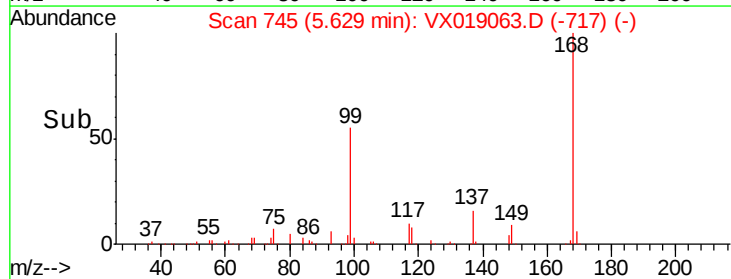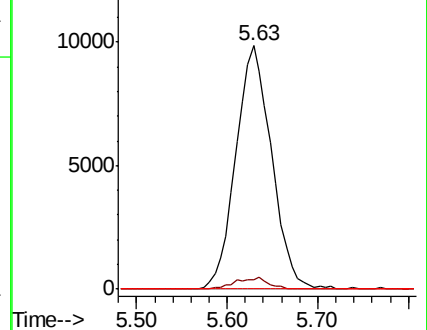

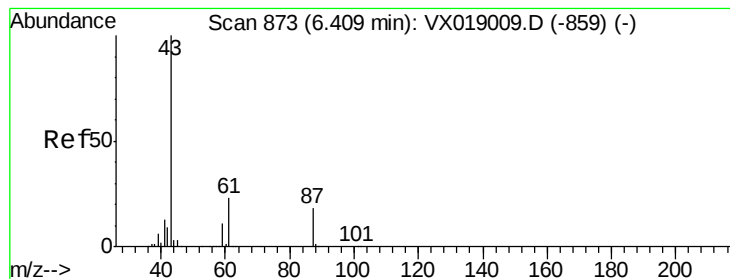

#43

Isopropyl Acetate

Concen: 9.991 ug/l

RT: 6.41 min Scan# 873

Delta R.T. 0.00 min

Lab File: VX019063.D

Acq: 23 Oct 2020 05:48

Instrument :

MSVOA_X

ClientSampleId :

72-11998


Tot Ion: 43 Resp: 62161

Ion Ratio Lower Upper




43 100

61 24.3 18.7 28.1

87 17.8 14.2 21.4



Abundance Ion 43.00 (42.70 to 43.70): VX0
Ion 61.00 (60.70 to 61.70): VX0
Ion 87.00 (86.70 to 87.70): VX0

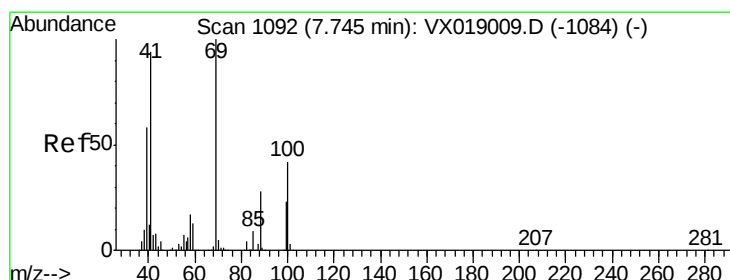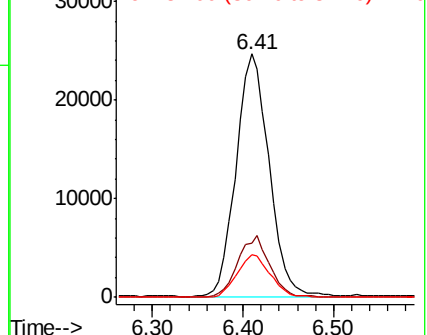

#48

Methyl methacrylate

Concen: 1.078 ug/l

RT: 7.65 min Scan# 1077

Delta R.T. -0.09 min

Lab File: VX019063.D

Acq: 23 Oct 2020 05:48


Tgt Ion: 41 Resp: 3306

Ion Ratio Lower Upper



41 100


69 0.0 85.5 128.3#

39 0.0 49.3 73.9#



Abundance Ion 41.00 (40.70 to 41.70): VX0
Ion 69.00 (68.70 to 69.70): VX0
Ion 39.00 (38.70 to 39.70): VX0

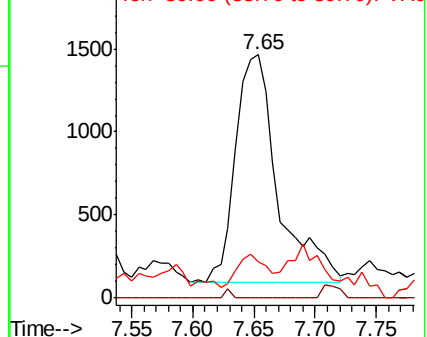

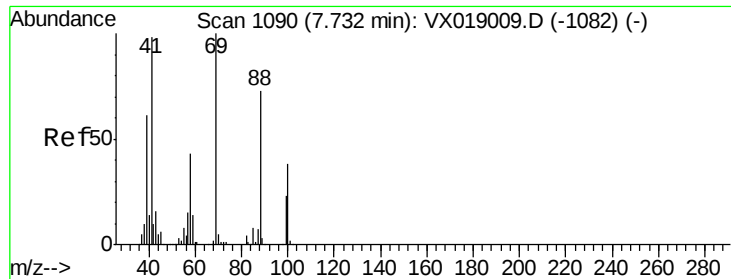

#49

1,4-Dioxane

Concen: 3.292 ug/l

RT: 7.84 min Scan# 1108

Delta R.T. 0.11 min

Lab File: VX019063.D

Acq: 23 Oct 2020 05:48

Instrument :

MSVOA_X

ClientSampleId :

72-11998


Tot Ion: 88 Resp: 228

Ion Ratio Lower Upper

88 100

43 450520.2 20.3 30.5#




58 2168.4 48.4 72.6#



Abundance Ion 88.00 (87.70 to 88.70): VX0

Ion 43.00 (42.70 to 43.70): VX0

Ion 58.00 (57.70 to 58.70): VX0

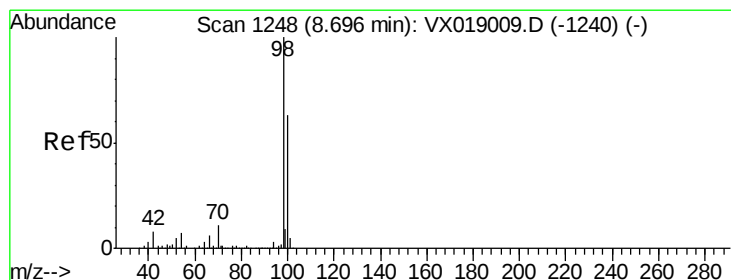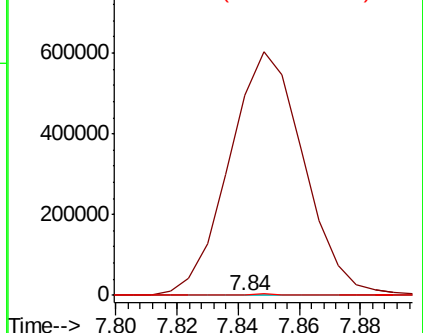

#50

Toluene-d8

Concen: 51.559 ug/l

RT: 8.70 min Scan# 1248

Delta R.T. 0.00 min

Lab File: VX019063.D


Acq: 23 Oct 2020 05:48

Tgt Ion: 98 Resp: 597553

Ion Ratio Lower Upper



98 100


100 65.3 52.1 78.1

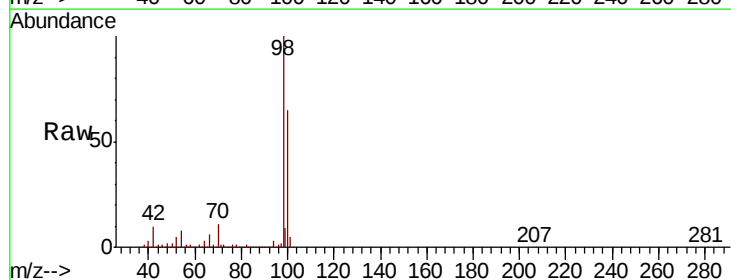

Abundance Ion 98.00 (97.70 to 98.70): VX0

Ion 100.00 (99.70 to 100.70): VX0

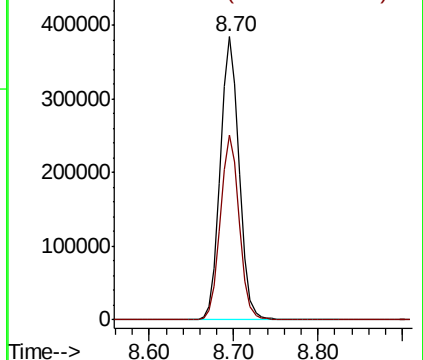



#51

4-Methyl-2-Pentanone

Concen: 16.750 ug/l

RT: 8.59 min Scan# 1231

Delta R.T. -0.03 min

Lab File: VX019063.D

Acq: 23 Oct 2020 05:48

Instrument :

MSVOA_X

ClientSampleId :


72-11998

Tot Ion: 43 Resp: 61412

Ion Ratio Lower Upper




43 100

58 10.4 37.4 56.0#



Abundance Ion 43.00 (42.70 to 43.70): VX0

Ion 58.00 (57.70 to 58.70): VX0

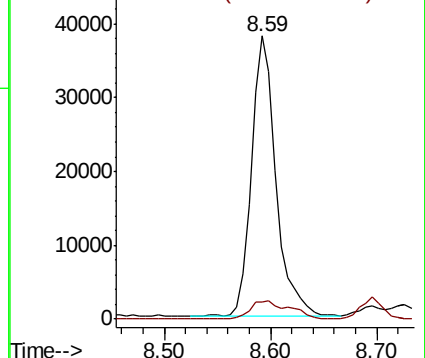

#52

Toluene

Concen: 0.523 ug/l

RT: 8.77 min Scan# 1260

Delta R.T. 0.01 min

Lab File: VX019063.D


Acq: 23 Oct 2020 05:48

Tgt Ion: 92 Resp: 4378

Ion Ratio Lower Upper



92 100


91 172.5 138.6 208.0



Abundance Ion 92.00 (91.70 to 92.70): VX0

Ion 91.00 (90.70 to 91.70): VX0

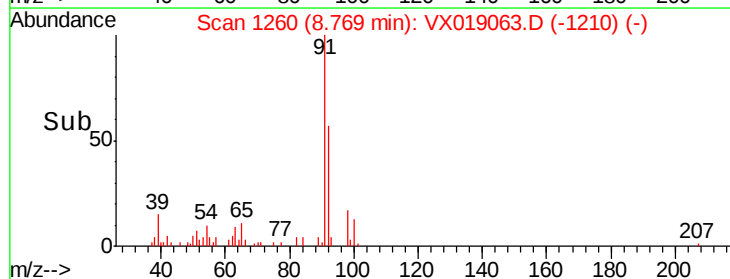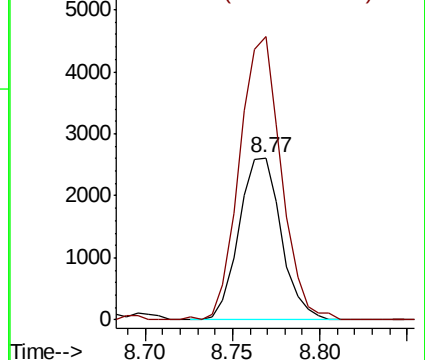




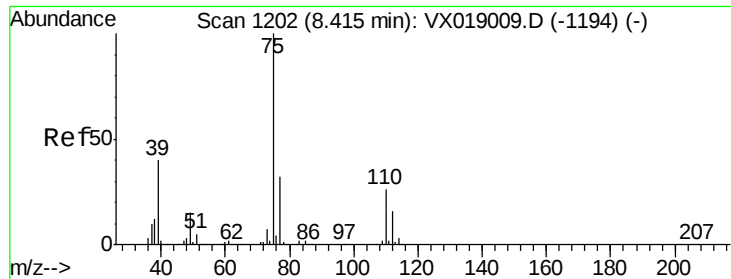


#54

cis-1,3-Dichloropropene
 Concen: 6.504 ug/l
 RT: 8.59 min Scan# 1231
 Delta R.T. 0.18 min
 Lab File: VX019063.D
 Acq: 23 Oct 2020 05:48

Instrument :
 MSVOA_X
 ClientSampleId :
 72-11998




Tot Ion: 75 Resp: 35218
 Ion Ratio Lower Upper
 75 100
 77 0.7 25.9 38.9#
 39 23.3 31.7 47.5#

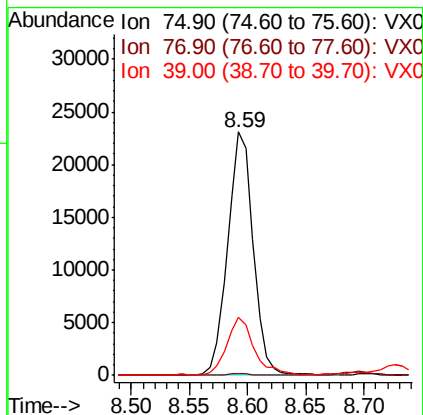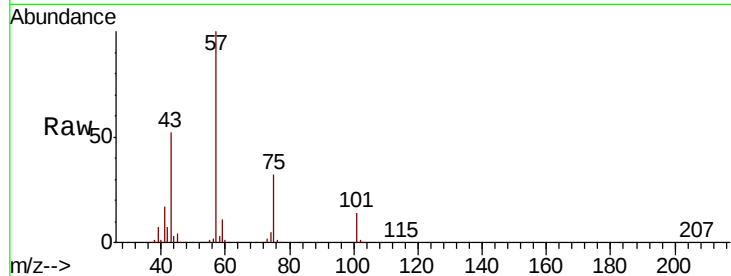


#57

1,3-Dichloropropane
 Concen: 1.105 ug/l
 RT: 9.52 min Scan# 1384
 Delta R.T. 0.17 min
 Lab File: VX019063.D
 Acq: 23 Oct 2020 05:48

Tgt Ion: 76 Resp: 5988
 Ion Ratio Lower Upper
 76 100
 78 0.0 26.2 39.4#


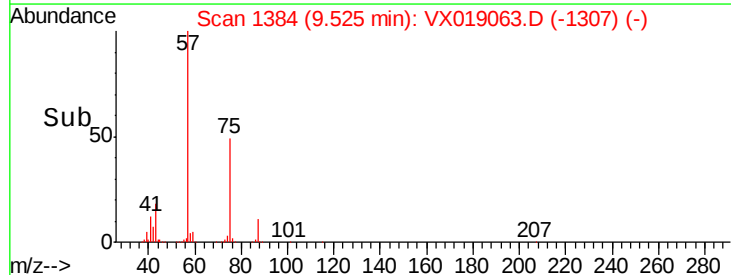
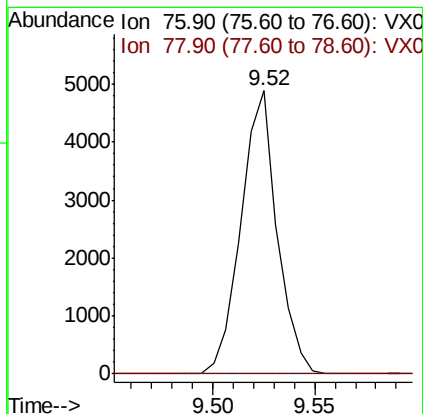





#59
2-Hexanone
Concen: 20.347 ug/l
RT: 9.42 min Scan# 1367
Delta R.T. -0.05 min
Lab File: VX019063.D
Acq: 23 Oct 2020 05:48




Instrument :
MSVOA_X
ClientSampleId :
72-11998


Tot Ion: 43 Resp: 55592
Ion Ratio Lower Upper
43 100
58 0.0 32.8 98.4#

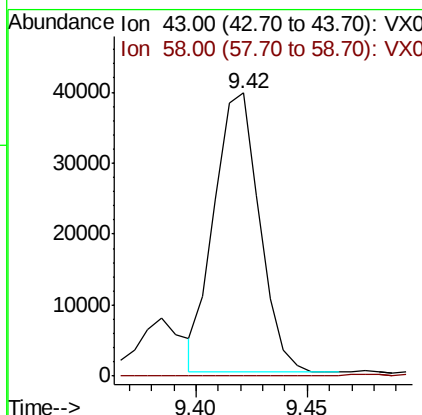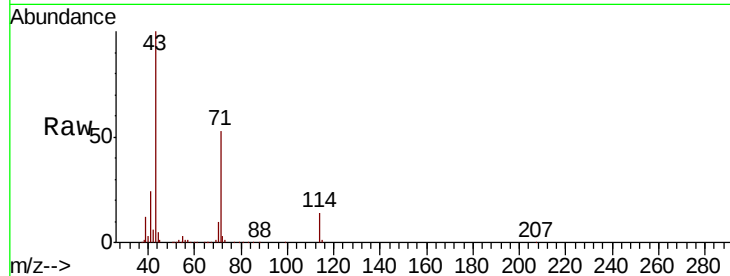

#62
4-Bromofluorobenzene
Concen: 52.107 ug/l
RT: 11.12 min Scan# 1646
Delta R.T. 0.00 min
Lab File: VX019063.D
Acq: 23 Oct 2020 05:48

Tgt Ion: 95 Resp: 214814
Ion Ratio Lower Upper
95 100
174 84.3 0.0 167.6
176 82.1 0.0 165.2



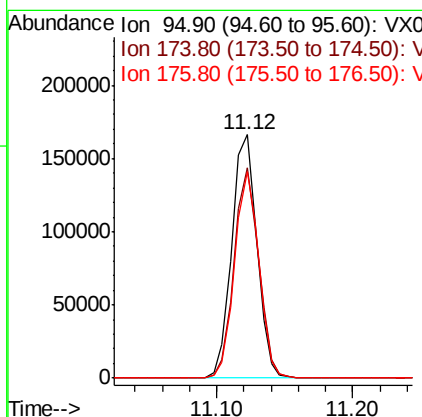
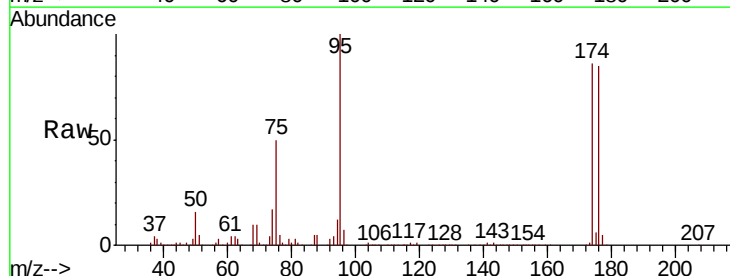




#63
Chlorobenzene-d5
Concen: 50.000 ug/l
RT: 10.10 min Scan# 1478
Delta R.T. 0.00 min
Lab File: VX019063.D
Acq: 23 Oct 2020 05:48




Instrument :
MSVOA_X
ClientSampleId :
72-11998


Tot Ion:117 Resp: 470210
Ion Ratio Lower Upper
117 100
82 52.0 42.4 63.6
119 32.0 25.6 38.4

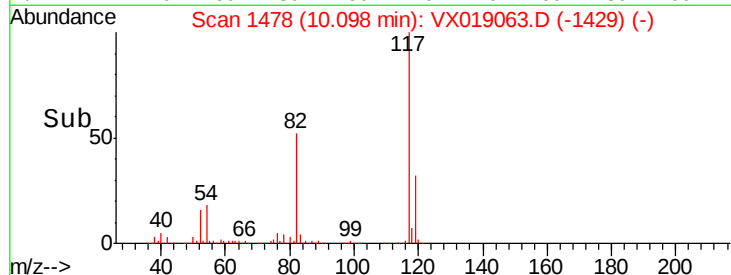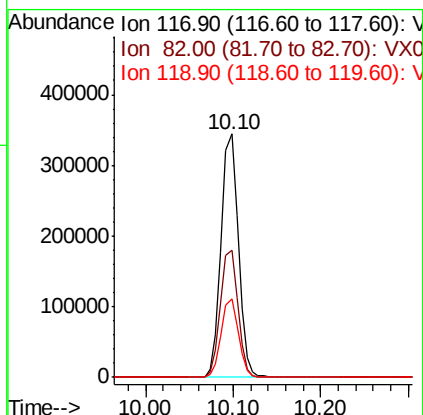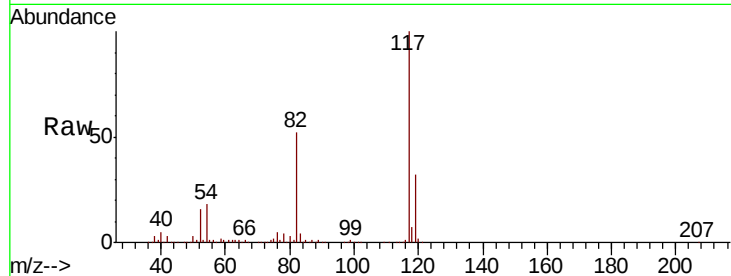

#67
Ethyl Benzene
Concen: 0.403 ug/l
RT: 10.23 min Scan# 1500
Delta R.T. 0.00 min
Lab File: VX019063.D
Acq: 23 Oct 2020 05:48

Tgt Ion: 91 Resp: 6858
Ion Ratio Lower Upper
91 100
106 31.1 25.3 37.9



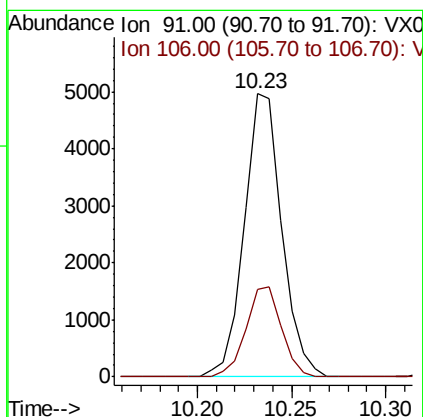
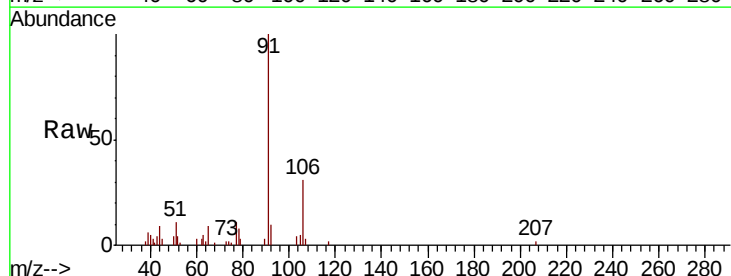


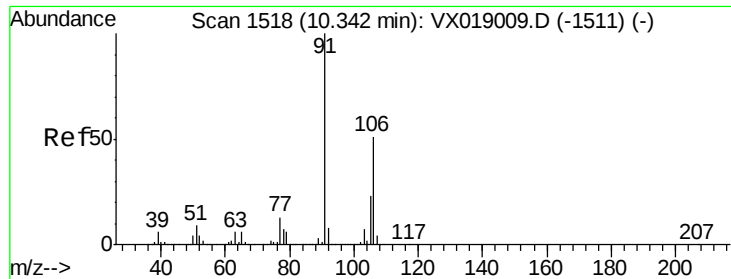

#68
m/p-Xvlenes
Concen: 0.361 ug/l
RT: 10.34 min Scan# 1518
Delta R.T. 0.00 min
Lab File: VX019063.D
Acq: 23 Oct 2020 05:48




Instrument :
MSVOA_X
ClientSampleId :
72-11998


Tot Ion:106 Resp: 2354
Ion Ratio Lower Upper
106 100
91 201.4 156.9 235.3

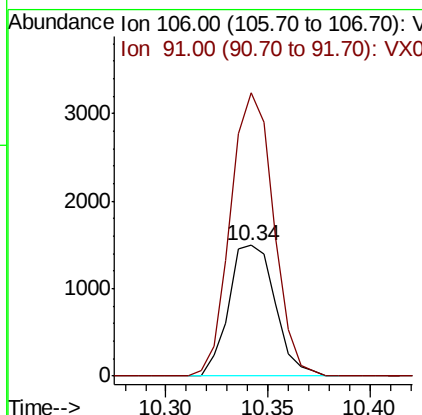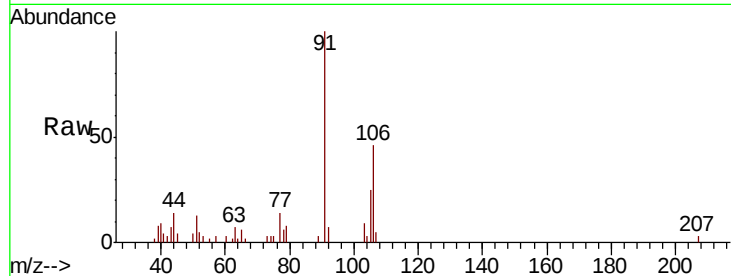

#72
1,4-Dichlorobenzene-d4
Concen: 50.000 ug/l
RT: 12.06 min Scan# 1800
Delta R.T. 0.00 min
Lab File: VX019063.D
Acq: 23 Oct 2020 05:48

Tgt Ion:152 Resp: 237290
Ion Ratio Lower Upper
152 100
115 57.2 40.8 122.5
150 154.6 0.0 345.6

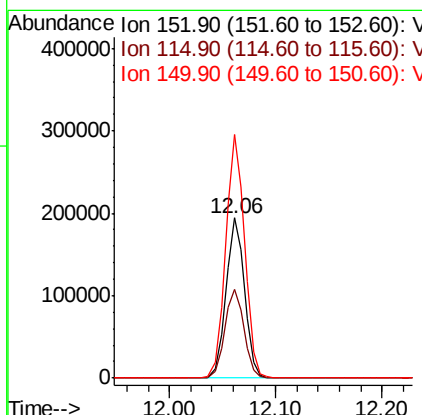



#74

N-amvl acetate

Concen: 0.518 ug/l

RT: 10.81 min Scan# 1594

Delta R.T. -0.07 min

Lab File: VX019063.D

Acq: 23 Oct 2020 05:48

Instrument :

MSVOA_X

ClientSampleId :

72-11998

Tot Ion: 43 Resp: 2832


Ion Ratio Lower Upper

43 100

70 0.0 44.5 66.7#

55 14.1 21.9 32.9#

61 0.0 23.9 35.9#



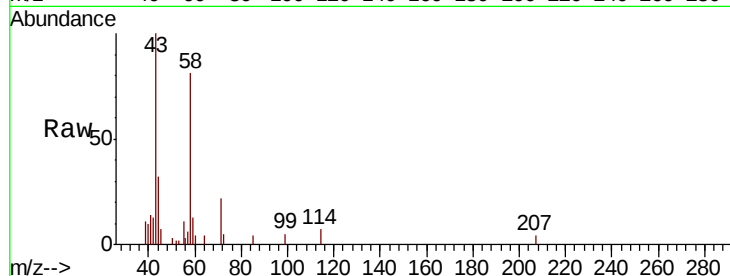


Abundance Ion 43.00 (42.70 to 43.70): VX0

Ion 70.00 (69.70 to 70.70): VX0

Ion 55.00 (54.70 to 55.70): VX0

Ion 61.00 (60.70 to 61.70): VX0

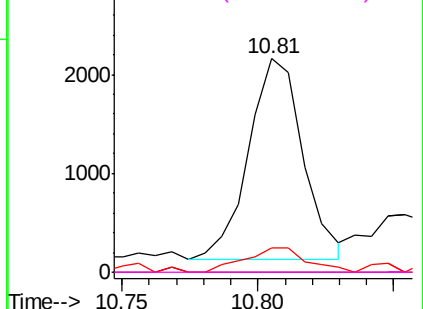

#76

1,2,3-Trichloropropane

Concen: 22.745 ug/l

RT: 11.12 min Scan# 1646

Delta R.T. -0.16 min

Lab File: VX019063.D


Acq: 23 Oct 2020 05:48

Tgt Ion: 75 Resp: 107872

Ion Ratio Lower Upper



75 100


77 1.2 20.7 62.1#



Abundance Ion 74.90 (74.60 to 75.60): VX0

Ion 77.00 (76.70 to 77.70): VX0



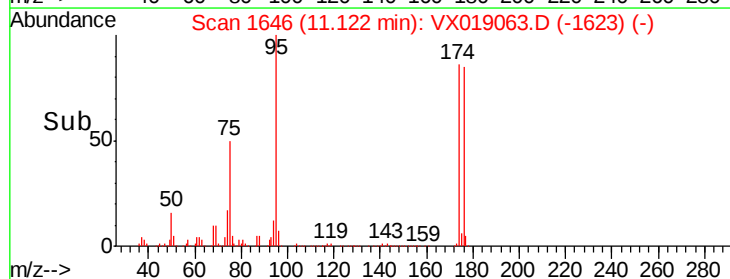
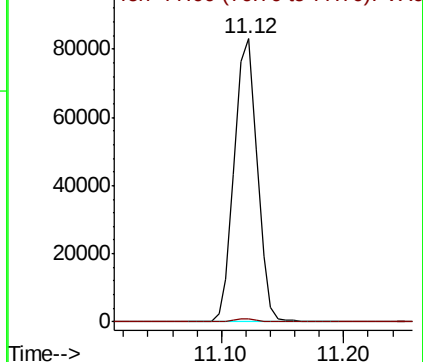




#81
trans-1,4-Dichloro-2-butene
Concen: 57.948 ug/l
RT: 11.12 min Scan# 1646
Delta R.T. 0.07 min
Lab File: VX019063.D
Acq: 23 Oct 2020 05:48

Instrument :
MSVOA_X
ClientSampled :
72-11998

Tot Ion: 75 Resp: 107872
Ion Ratio Lower Upper
75 100
53 0.0 67.4 101.2#
89 0.0 37.2 55.8#

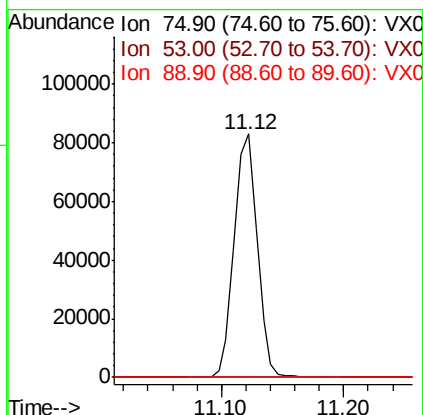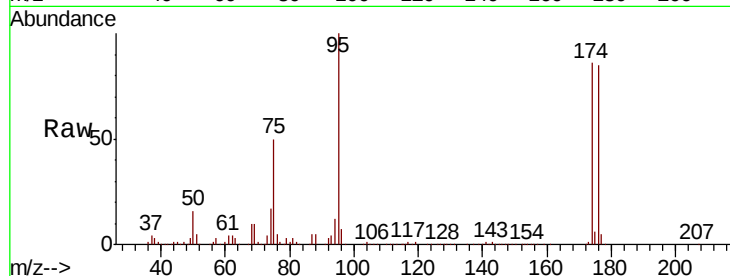

#84
1,2,4-Trimethylbenzene
Concen: 0.252 ug/l
RT: 11.79 min Scan# 1755
Delta R.T. -0.01 min
Lab File: VX019063.D
Acq: 23 Oct 2020 05:48

Tgt Ion: 105 Resp: 3560
Ion Ratio Lower Upper
105 100
120 47.1 22.9 68.8

