

Data Path : Z:\VOASRV\HPCHEM1\MSVOA X\DATA\VX102220\  
Data File : VX019015.D  
Acq On : 22 Oct 2020 10:35  
Operator : JC/SP  
Sample : VX1022WBL01  
Misc : 5.0mL/MSVOA X/WATER  
ALS Vial : 3 Sample Multiplier: 1

Instrument :  
MSVOA\_X  
ClientSampleId :  
VX1022WBL01

## Integration Parameters: RTEINT.P

Integrator: RTE  
Smoothing : ON Filtering: 5  
Sampling : 1 Min Area: 3 % of largest Peak  
Start Thrs: 0.2 Max Peaks: 100  
Stop Thrs : 0 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >  
Peak separation: 5

Method : Z:\VOASRV\HPCHEM1\MSVOA\_X\METHOD\82X102120W.M  
Title : SW846 8260

Signal : TIC

| peak<br># | R.T.<br>min | first<br>scan | max<br>scan | last<br>scan | PK<br>TY | peak<br>height | corr.<br>area | corr.<br>% max. | % of<br>total |
|-----------|-------------|---------------|-------------|--------------|----------|----------------|---------------|-----------------|---------------|
| 1         | 5.458       | 705           | 717         | 732          | rBV      | 192177         | 557497        | 32.83%          | 6.233%        |
| 2         | 5.623       | 732           | 744         | 760          | rVB2     | 314432         | 902755        | 53.17%          | 10.093%       |
| 3         | 6.025       | 799           | 810         | 828          | rBV      | 197169         | 524443        | 30.89%          | 5.863%        |
| 4         | 6.824       | 930           | 941         | 958          | rBV      | 509346         | 1196286       | 70.45%          | 13.375%       |
| 5         | 8.696       | 1240          | 1248        | 1265         | rBV      | 1064940        | 1697945       | 100.00%         | 18.983%       |
| 6         | 10.092      | 1471          | 1477        | 1491         | rBV      | 1078957        | 1466516       | 86.37%          | 16.396%       |
| 7         | 11.122      | 1640          | 1646        | 1658         | rBV      | 894554         | 1129327       | 66.51%          | 12.626%       |
| 8         | 12.061      | 1795          | 1800        | 1810         | rVB      | 1211318        | 1469717       | 86.56%          | 16.432%       |


Sum of corrected areas: 8944486

Data Path : Z:\V0ASRV\HPCHEM1\MSVOA X\DATA\VX102220\  
Data File : VX019015.D  
Acq On : 22 Oct 2020 10:35  
Operator : JC/SP  
Sample : VX1022WBL01  
Misc : 5.0mL/MSVOA X/WATER  
ALS Vial : 3 Sample Multiplier: 1

Instrument :  
MSVOA\_X  
ClientSampleId :  
VX1022WBL01

Quant Method : Z:\V0ASRV\HPCHEM1\MSVOA\_X\METHOD\82X102120W.M  
Quant Title : SW846 8260

TIC Library : C:\DATABASE\NIST11.L  
TIC Integration Parameters: LSCINT.P

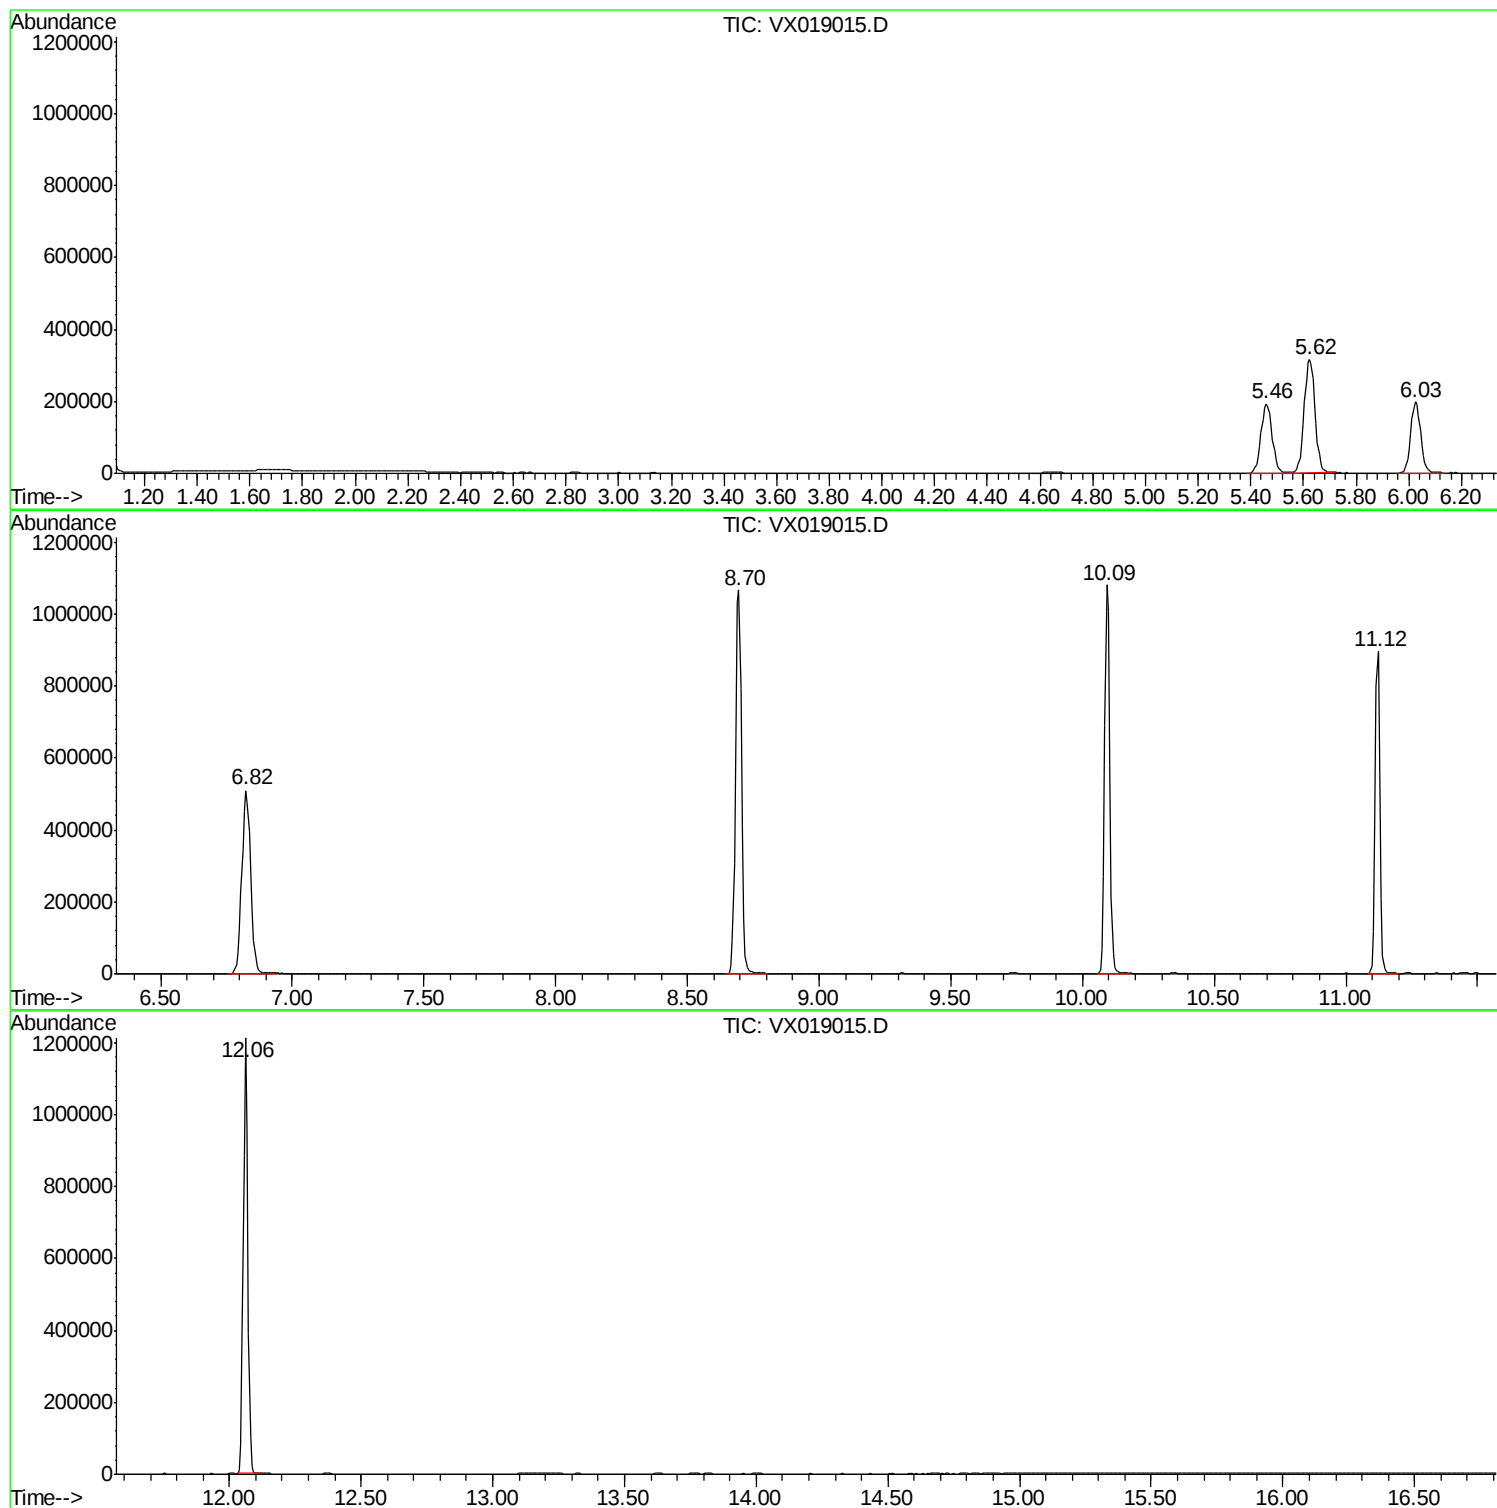

Data Path : Z:\V0ASRV\HPCHEM1\MSVOA\_X\DATA\VX102220\  
Data File : VX019015.D  
Acq On : 22 Oct 2020 10:35  
Operator : JC/SP  
Sample : VX1022WBL01  
Misc : 5.0mL/MSVOA\_X/WATER  
ALS Vial : 3 Sample Multiplier: 1

Instrument :  
MSVOA\_X  
ClientSampleId :  
VX1022WBL01

Quant Method : Z:\V0ASRV\HPCHEM1\MSVOA\_X\METHOD\82X102120W.M  
Quant Title : SW846 8260

TIC Library : C:\DATABASE\NIST11.L  
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

\*\*\*\*\*

Data Path : Z:\V0ASRV\HPCHEM1\MSVOA\_X\DATA\VX102220\  
Data File : VX019015.D  
Acq On : 22 Oct 2020 10:35  
Operator : JC/SP  
Sample : VX1022WBL01  
Misc : 5.0mL/MSVOA\_X/WATER  
ALS Vial : 3 Sample Multiplier: 1

Instrument :  
MSVOA\_X  
ClientSampleId :  
VX1022WBL01

Quant Method : Z:\V0ASRV\HPCHEM1\MSVOA\_X\METHOD\82X102120W.M  
Quant Title : SW846 8260

TIC Library : C:\DATABASE\NIST11.L  
TIC Integration Parameters: LSCINT.P

| TIC Top Hit name | RT | EstConc | Units | Response | --Internal Standard-- |
|------------------|----|---------|-------|----------|-----------------------|
|                  |    |         |       |          | # RT Resp Conc        |