

Data Path : Z:\VOASRV\HPCHEM1\MSVOA X\DATA\VX102220\  
Data File : VX019025.D  
Acq On : 22 Oct 2020 14:30  
Operator : JC/SP  
Sample : L4417-02  
Misc : 5.0mL/MSVOA X/WATER  
ALS Vial : 13 Sample Multiplier: 1

Instrument :  
MSVOA\_X  
ClientSampleId :  
MW-8

## Integration Parameters: RTEINT.P

Integrator: RTE  
Smoothing : ON Filtering: 5  
Sampling : 1 Min Area: 3 % of largest Peak  
Start Thrs: 0.2 Max Peaks: 100  
Stop Thrs : 0 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >  
Peak separation: 5

Method : Z:\VOASRV\HPCHEM1\MSVOA\_X\METHOD\82X102120W.M  
Title : SW846 8260

Signal : TIC

| peak<br># | R.T.<br>min | first<br>scan | max<br>scan | last<br>scan | PK<br>TY | peak<br>height | corr.<br>area | corr.<br>% max. | % of<br>total |
|-----------|-------------|---------------|-------------|--------------|----------|----------------|---------------|-----------------|---------------|
| 1         | 2.611       | 243           | 250         | 262          | rVB2     | 9969           | 28547         | 1.78%           | 0.331%        |
| 2         | 4.654       | 573           | 585         | 595          | rBV2     | 4934           | 18065         | 1.13%           | 0.210%        |
| 3         | 5.465       | 703           | 718         | 733          | rBV2     | 177450         | 516178        | 32.21%          | 5.987%        |
| 4         | 5.629       | 733           | 745         | 761          | rVB      | 302151         | 841442        | 52.51%          | 9.760%        |
| 5         | 6.031       | 800           | 811         | 827          | rBV      | 187681         | 493657        | 30.81%          | 5.726%        |
| 6         | 6.830       | 932           | 942         | 956          | rBV      | 466331         | 1114347       | 69.54%          | 12.925%       |
| 7         | 8.696       | 1241          | 1248        | 1266         | rBV      | 1042930        | 1602485       | 100.00%         | 18.587%       |
| 8         | 10.098      | 1472          | 1478        | 1492         | rBV      | 1065330        | 1437443       | 89.70%          | 16.672%       |
| 9         | 11.122      | 1640          | 1646        | 1659         | rBV      | 904067         | 1127315       | 70.35%          | 13.075%       |
| 10        | 12.061      | 1795          | 1800        | 1820         | rVB      | 1201656        | 1442232       | 90.00%          | 16.728%       |


Sum of corrected areas: 8621711

Data Path : Z:\V0ASRV\HPCHEM1\MSVOA X\DATA\VX102220\  
Data File : VX019025.D  
Acq On : 22 Oct 2020 14:30  
Operator : JC/SP  
Sample : L4417-02  
Misc : 5.0mL/MSVOA X/WATER  
ALS Vial : 13 Sample Multiplier: 1

Instrument :  
MSVOA\_X  
ClientSampleId :  
MW-8

Quant Method : Z:\V0ASRV\HPCHEM1\MSVOA\_X\METHOD\82X102120W.M  
Quant Title : SW846 8260

TIC Library : C:\DATABASE\NIST11.L  
TIC Integration Parameters: LSCINT.P

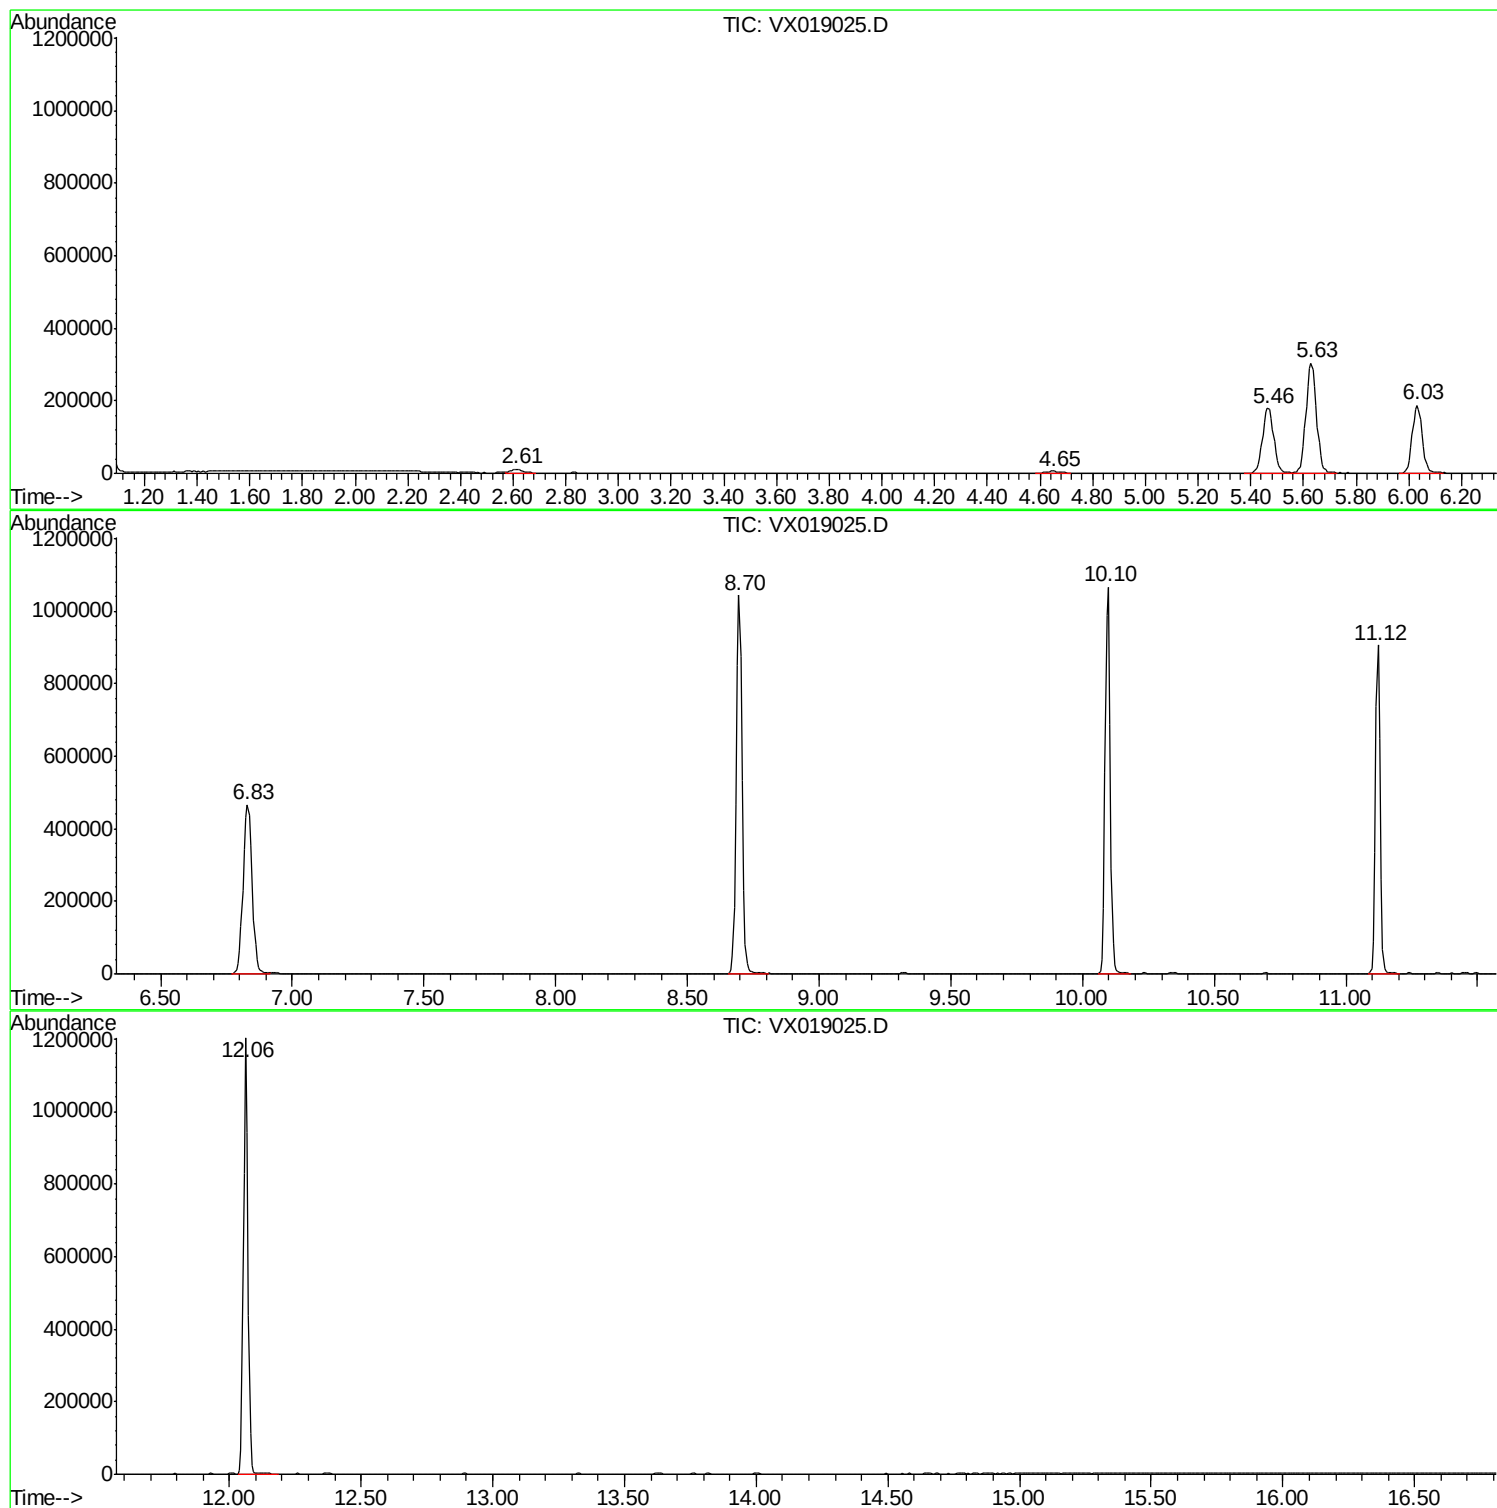

Data Path : Z:\V0ASRV\HPCHEM1\MSVOA\_X\DATA\VX102220\  
Data File : VX019025.D  
Acq On : 22 Oct 2020 14:30  
Operator : JC/SP  
Sample : L4417-02  
Misc : 5.0mL/MSVOA\_X/WATER  
ALS Vial : 13 Sample Multiplier: 1

Instrument :  
MSVOA\_X  
ClientSampleId :  
MW-8

Quant Method : Z:\V0ASRV\HPCHEM1\MSVOA\_X\METHOD\82X102120W.M  
Quant Title : SW846 8260

TIC Library : C:\DATABASE\NIST11.L  
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

\*\*\*\*\*

Data Path : Z:\V0ASRV\HPCHEM1\MSVOA\_X\DATA\VX102220\  
Data File : VX019025.D  
Acq On : 22 Oct 2020 14:30  
Operator : JC/SP  
Sample : L4417-02  
Misc : 5.0mL/MSVOA\_X/WATER  
ALS Vial : 13 Sample Multiplier: 1

Instrument :  
MSVOA\_X  
ClientSampleId :  
MW-8

Quant Method : Z:\V0ASRV\HPCHEM1\MSVOA\_X\METHOD\82X102120W.M  
Quant Title : SW846 8260

TIC Library : C:\DATABASE\NIST11.L  
TIC Integration Parameters: LSCINT.P

| TIC Top Hit name | RT | EstConc | Units | Response | --Internal Standard-- |
|------------------|----|---------|-------|----------|-----------------------|
|                  |    |         |       |          | # RT Resp Conc        |