

Data Path : Z:\VOASRV\HPCHEM1\MSVOA X\DATA\VX102220\
 Data File : VX019062.D
 Acq On : 23 Oct 2020 05:26
 Operator : JC/SP
 Sample : L4225-14
 Misc : 5.0mL/MSVOA X/WATER
 ALS Vial : 53 Sample Multiplier: 1

Instrument :
 MSVOA_X
 ClientSampleId :
 SU-02-102120

Integration Parameters: RTEINT.P

Integrator: RTE

Smoothing : ON

Sampling : 1

Start Thrs: 0.2

Stop Thrs : 0

Filtering: 5

Min Area: 3 % of largest Peak

Max Peaks: 100

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\VOASRV\HPCHEM1\MSVOA_X\METHOD\82X102120W.M

Title : SW846 8260

Signal : TIC

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	2.837	278	287	298	rVB2	12060	25001	1.18%	0.177%
2	4.641	572	583	592	rBV2	7341	24116	1.14%	0.171%
3	5.464	707	718	733	rBV2	174838	507003	23.87%	3.590%
4	5.629	733	745	764	rVB	289315	808155	38.04%	5.723%
5	6.031	799	811	832	rBV	184455	488032	22.97%	3.456%
6	6.409	863	873	885	rBV	48223	124688	5.87%	0.883%
7	6.830	929	942	955	rBV	459463	1119669	52.71%	7.929%
8	7.744	1088	1092	1098	rVB2	18940	33011	1.55%	0.234%
9	7.848	1101	1109	1124	rBV	1238687	2124244	100.00%	15.043%
10	8.592	1225	1231	1241	rBV	197199	307388	14.47%	2.177%
11	8.696	1241	1248	1257	rVV	996545	1577969	74.28%	11.174%
12	8.763	1257	1259	1267	rVB	17282	26594	1.25%	0.188%
13	8.994	1292	1297	1311	rVB	61326	90218	4.25%	0.639%
14	9.287	1336	1345	1351	rBV	373853	513848	24.19%	3.639%
15	9.348	1351	1355	1358	rVV	20066	27323	1.29%	0.193%
16	9.384	1358	1361	1363	rVV	46898	57383	2.70%	0.406%
17	9.421	1363	1367	1374	rVB	97831	138282	6.51%	0.979%
18	9.525	1378	1384	1389	rBV	648678	845783	39.82%	5.989%
19	9.616	1395	1399	1410	rVB	32536	46161	2.17%	0.327%
20	9.951	1448	1454	1466	rBV	892730	1112406	52.37%	7.877%
21	10.098	1469	1478	1484	rVV	979560	1396150	65.72%	9.887%
22	10.342	1509	1518	1524	rVB2	12116	22624	1.07%	0.160%
23	10.543	1546	1551	1558	rBV	23708	30135	1.42%	0.213%
24	10.677	1568	1573	1582	rBV	138480	162144	7.63%	1.148%
25	11.122	1640	1646	1658	rBV	848140	1071137	50.42%	7.585%
26	12.061	1795	1800	1807	rBV	1174742	1418083	66.76%	10.042%
27	13.884	2095	2099	2108	rBV	14022	23880	1.12%	0.169%


Sum of corrected areas: 14121427

Data Path : Z:\V0ASRV\HPCHEM1\MSVOA X\DATA\VX102220\
Data File : VX019062.D
Acq On : 23 Oct 2020 05:26
Operator : JC/SP
Sample : L4225-14
Misc : 5.0mL/MSVOA X/WATER
ALS Vial : 53 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
SU-02-102120

Quant Method : Z:\V0ASRV\HPCHEM1\MSVOA_X\METHOD\82X102120W.M
Quant Title : SW846 8260

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

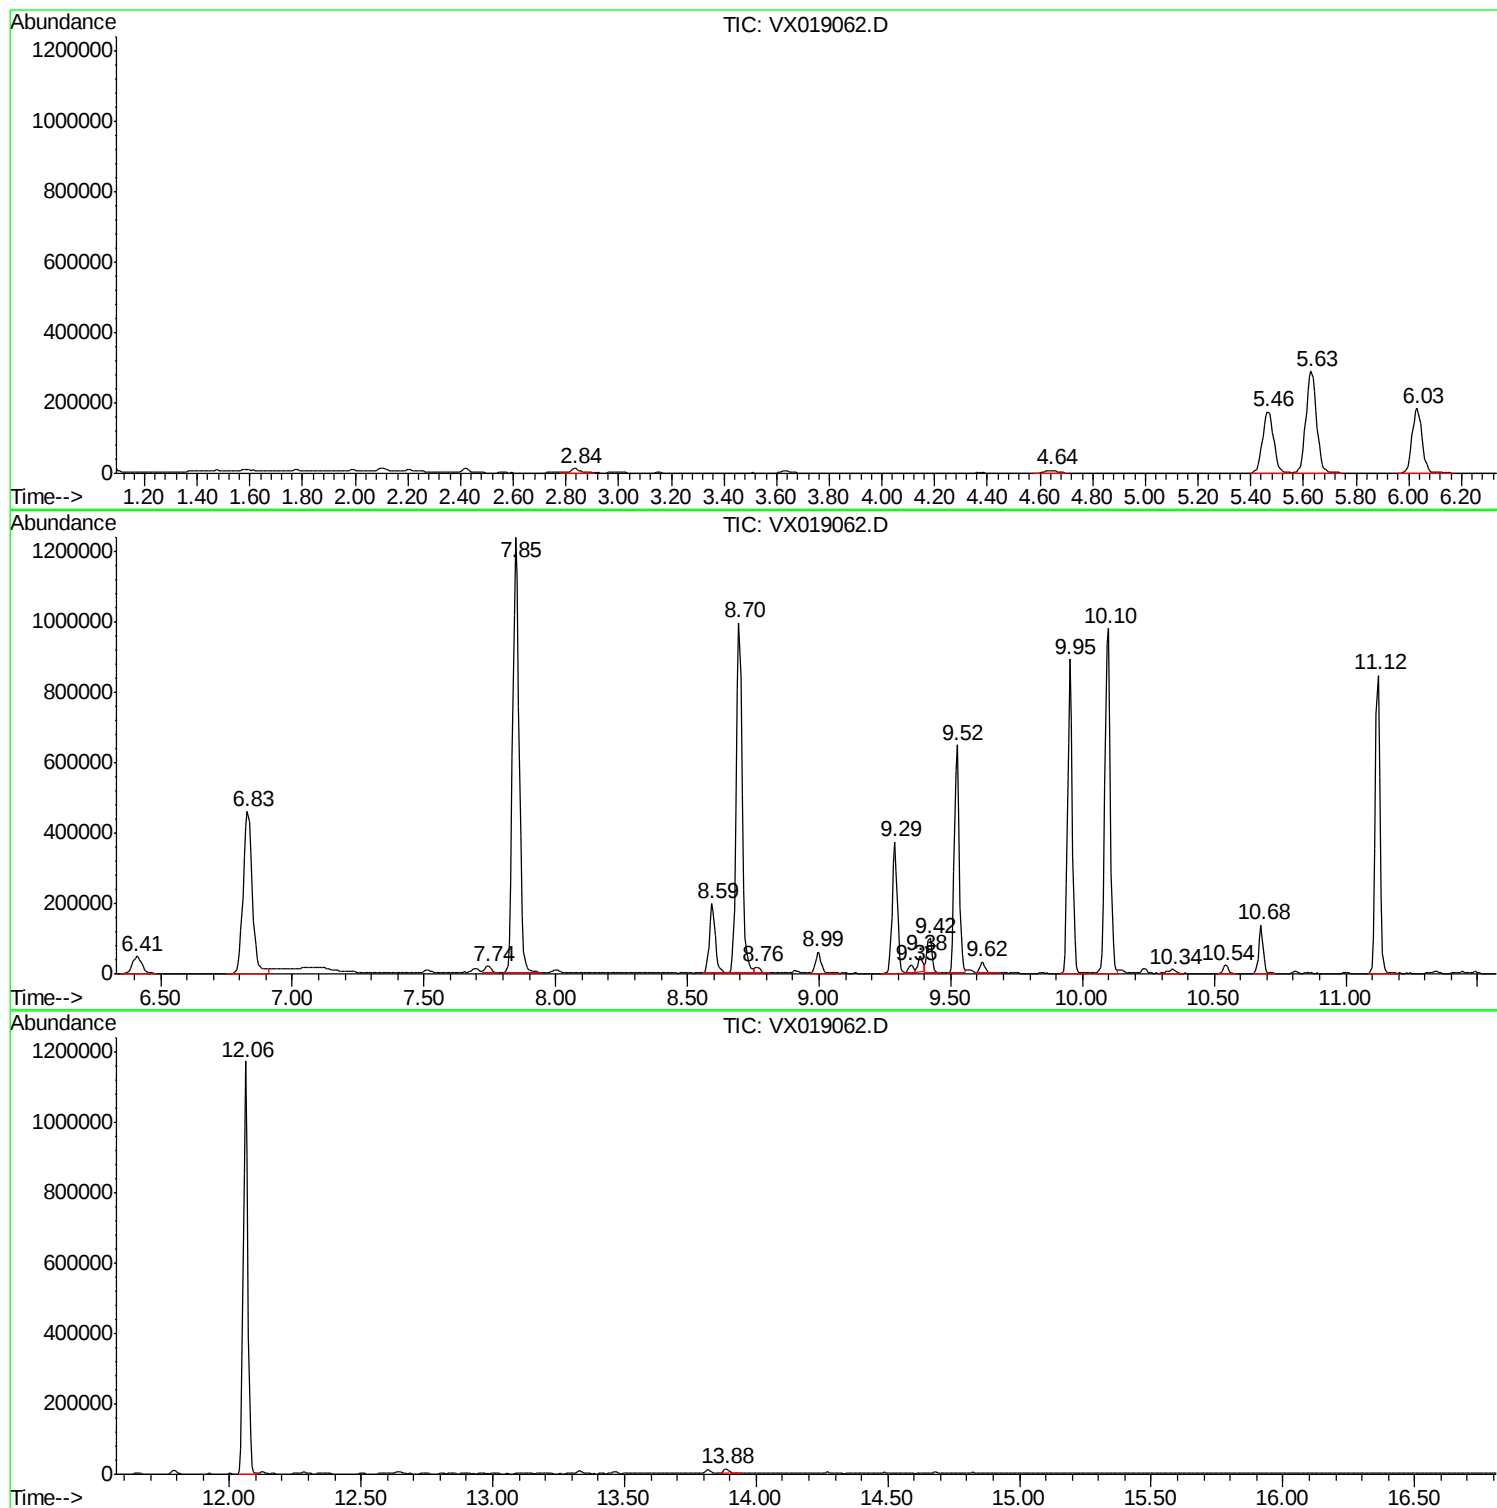

Data Path : Z:\V0ASRV\HPCHEM1\MSVOA_X\DATA\VX102220\
Data File : VX019062.D
Acq On : 23 Oct 2020 05:26
Operator : JC/SP
Sample : L4225-14
Misc : 5.0mL/MSVOA_X/WATER
ALS Vial : 53 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
SU-02-102120

Quant Method : Z:\V0ASRV\HPCHEM1\MSVOA_X\METHOD\82X102120W.M
Quant Title : SW846 8260

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\V0ASRV\HPCHEM1\MSVOA_X\DATA\VX102220\
Data File : VX019062.D
Acq On : 23 Oct 2020 05:26
Operator : JC/SP
Sample : L4225-14
Misc : 5.0mL/MSVOA_X/WATER
ALS Vial : 53 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
SU-02-102120

Quant Method : Z:\V0ASRV\HPCHEM1\MSVOA_X\METHOD\82X102120W.M
Quant Title : SW846 8260

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--
					# RT Resp Conc