


Data Path : Z:\voasrv\HPCHEM1\MSVOA X\Data\VX102220\
Data File : VX019042.D
Acq On : 22 Oct 2020 20:51
Operator : JC/SP
Sample : BFB
Misc : 5.0mL/MSVOA X/WATER
ALS Vial : 30 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
BFB

Integration File: RTEINT.P

Method : Z:\VOASRV\HPCHEM1\MSVOA_X\METHOD\82X102120W.M
Title : SW846 8260
Last Update : Thu Oct 22 17:51:42 2020

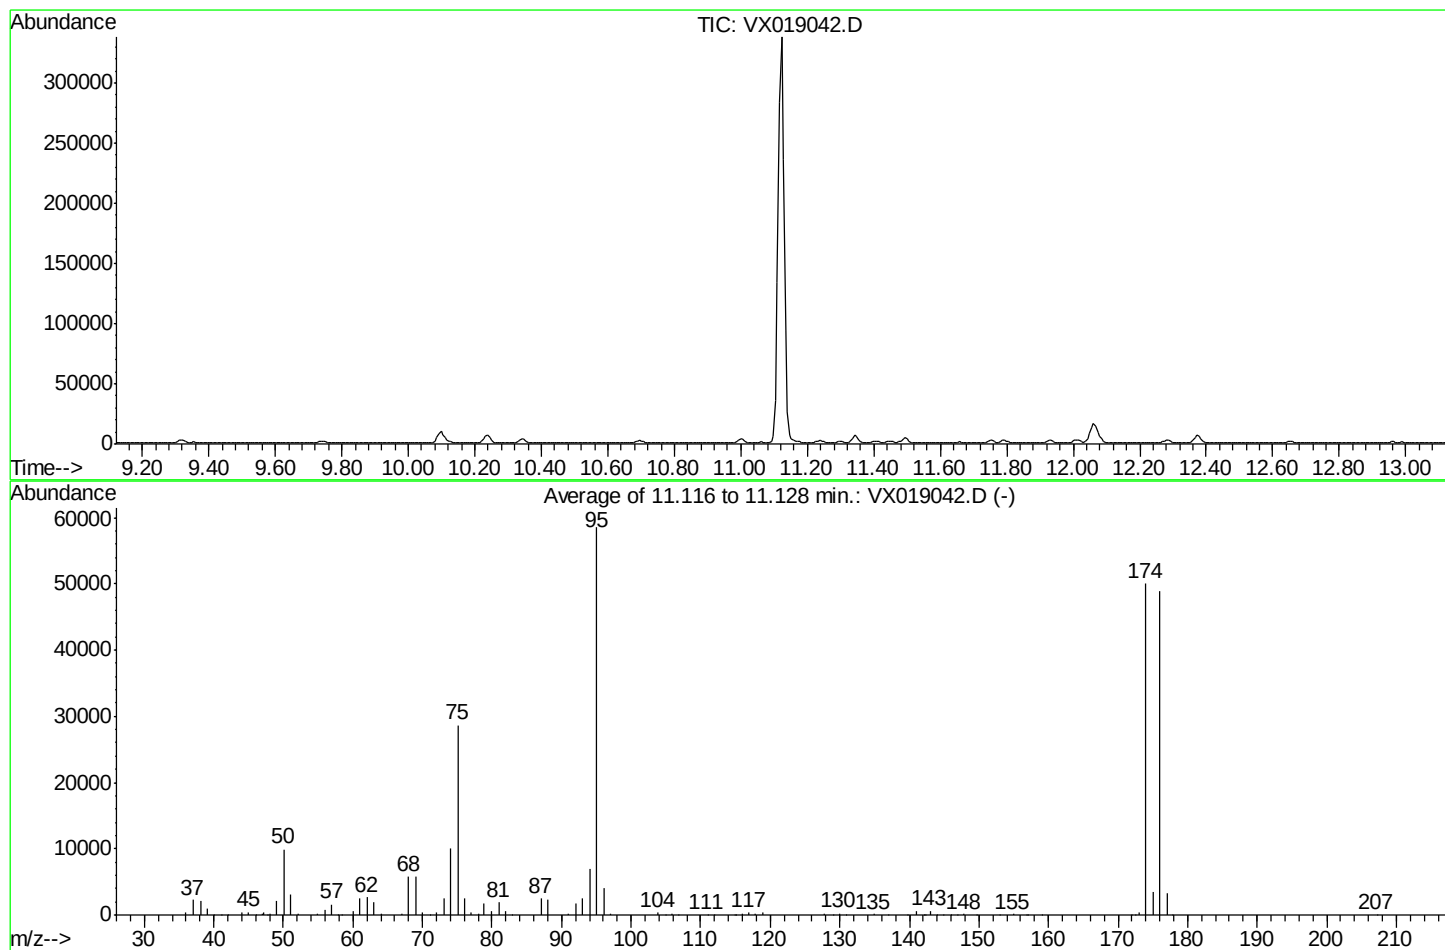

AutoFind: Scans 1645, 1646, 1647; Background Corrected with Scan 1638

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	15	40	16.9	9879	PASS
75	95	30	60	49.0	28656	PASS
95	95	100	100	100.0	58530	PASS
96	95	5	9	6.8	3988	PASS
173	174	0.00	2	0.9	457	PASS
174	95	50	100	85.4	49970	PASS
175	174	5	9	7.0	3479	PASS
176	174	95	101	98.0	48949	PASS
177	176	5	9	6.5	3197	PASS