

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX102221\
 Data File : VX024871.D
 Acq On : 22 Oct 2021 15:02
 Operator : JC/MD
 Sample : M4291-04
 Misc : 25.0mL/MSVOA_X/WATER
 ALS Vial : 14 Sample Multiplier: 1

Instrument :
 MSVOA_X
 ClientSampleId :
 P001-TW001-06

Quant Time: Oct 23 03:54:50 2021
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXTR102221WMA.M
 Quant Title : TRACE VOA SFAM1.0
 QLast Update : Sat Oct 23 03:44:55 2021
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) 1,4-Difluorobenzene	6.769	114	69068	5.000	ug/L	0.00
28) Chlorobenzene-d5	10.055	117	64858	5.000	ug/L	0.00
58) 1,4-Dichlorobenzene-d4	12.024	152	30590	5.000	ug/L	0.00
System Monitoring Compounds						
4) Vinyl Chloride-d3	1.368	65	10274	5.067	ug/L	0.00
Spiked Amount	5.000	Range	40 - 130	Recovery	=	101.400%
7) Chloroethane-d5	1.672	69	9521	5.211	ug/L	0.00
Spiked Amount	5.000	Range	65 - 130	Recovery	=	104.200%
11) 1,1-Dichloroethene-d2	2.306	63	27969	3.700	ug/L	0.00
Spiked Amount	5.000	Range	60 - 125	Recovery	=	74.000%
20) 2-Butanone-d5	4.477	46	34595	46.665	ug/L	0.00
Spiked Amount	50.000	Range	40 - 130	Recovery	=	93.340%
24) Chloroform-d	5.068	84	48323	4.950	ug/L	0.00
Spiked Amount	5.000	Range	70 - 125	Recovery	=	99.000%
26) 1,2-Dichloroethane-d4	5.964	65	25095	4.704	ug/L	0.00
Spiked Amount	5.000	Range	70 - 130	Recovery	=	94.000%
32) Benzene-d6	5.983	84	78989	5.227	ug/L	0.00
Spiked Amount	5.000	Range	70 - 125	Recovery	=	104.600%
36) 1,2-Dichloropropane-d6	7.318	67	22952	4.761	ug/L	0.00
Spiked Amount	5.000	Range	60 - 140	Recovery	=	95.200%
41) Toluene-d8	8.653	98	75782	5.002	ug/L	0.00
Spiked Amount	5.000	Range	70 - 130	Recovery	=	100.000%
43) trans-1,3-Dichloroprop...	8.958	79	9116	4.119	ug/L	0.00
Spiked Amount	5.000	Range	55 - 130	Recovery	=	82.400%
46) 2-Hexanone-d5	9.391	63	36482	45.806	ug/L	0.00
Spiked Amount	50.000	Range	45 - 130	Recovery	=	91.620%
56) 1,1,2,2-Tetrachloroeth...	11.195	84	17587	4.773	ug/L	0.00
Spiked Amount	5.000	Range	65 - 120	Recovery	=	95.400%
66) 1,2-Dichlorobenzene-d4	12.323	152	26973	5.232	ug/L	0.00
Spiked Amount	5.000	Range	80 - 120	Recovery	=	104.600%
Target Compounds					Qvalue	
13) Acetone	2.392	43	1214	2.183	ug/L	95


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX102221\
Data File : VX024871.D
Acq On : 22 Oct 2021 15:02
Operator : JC/MD
Sample : M4291-04
Misc : 25.0mL/MSVOA_X/WATER
ALS Vial : 14 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
P001-TW001-06

Quant Time: Oct 23 03:54:50 2021
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXTR102221WMA.M
Quant Title : TRACE VOA SFAM1.0
QLast Update : Sat Oct 23 03:44:55 2021
Response via : Initial Calibration

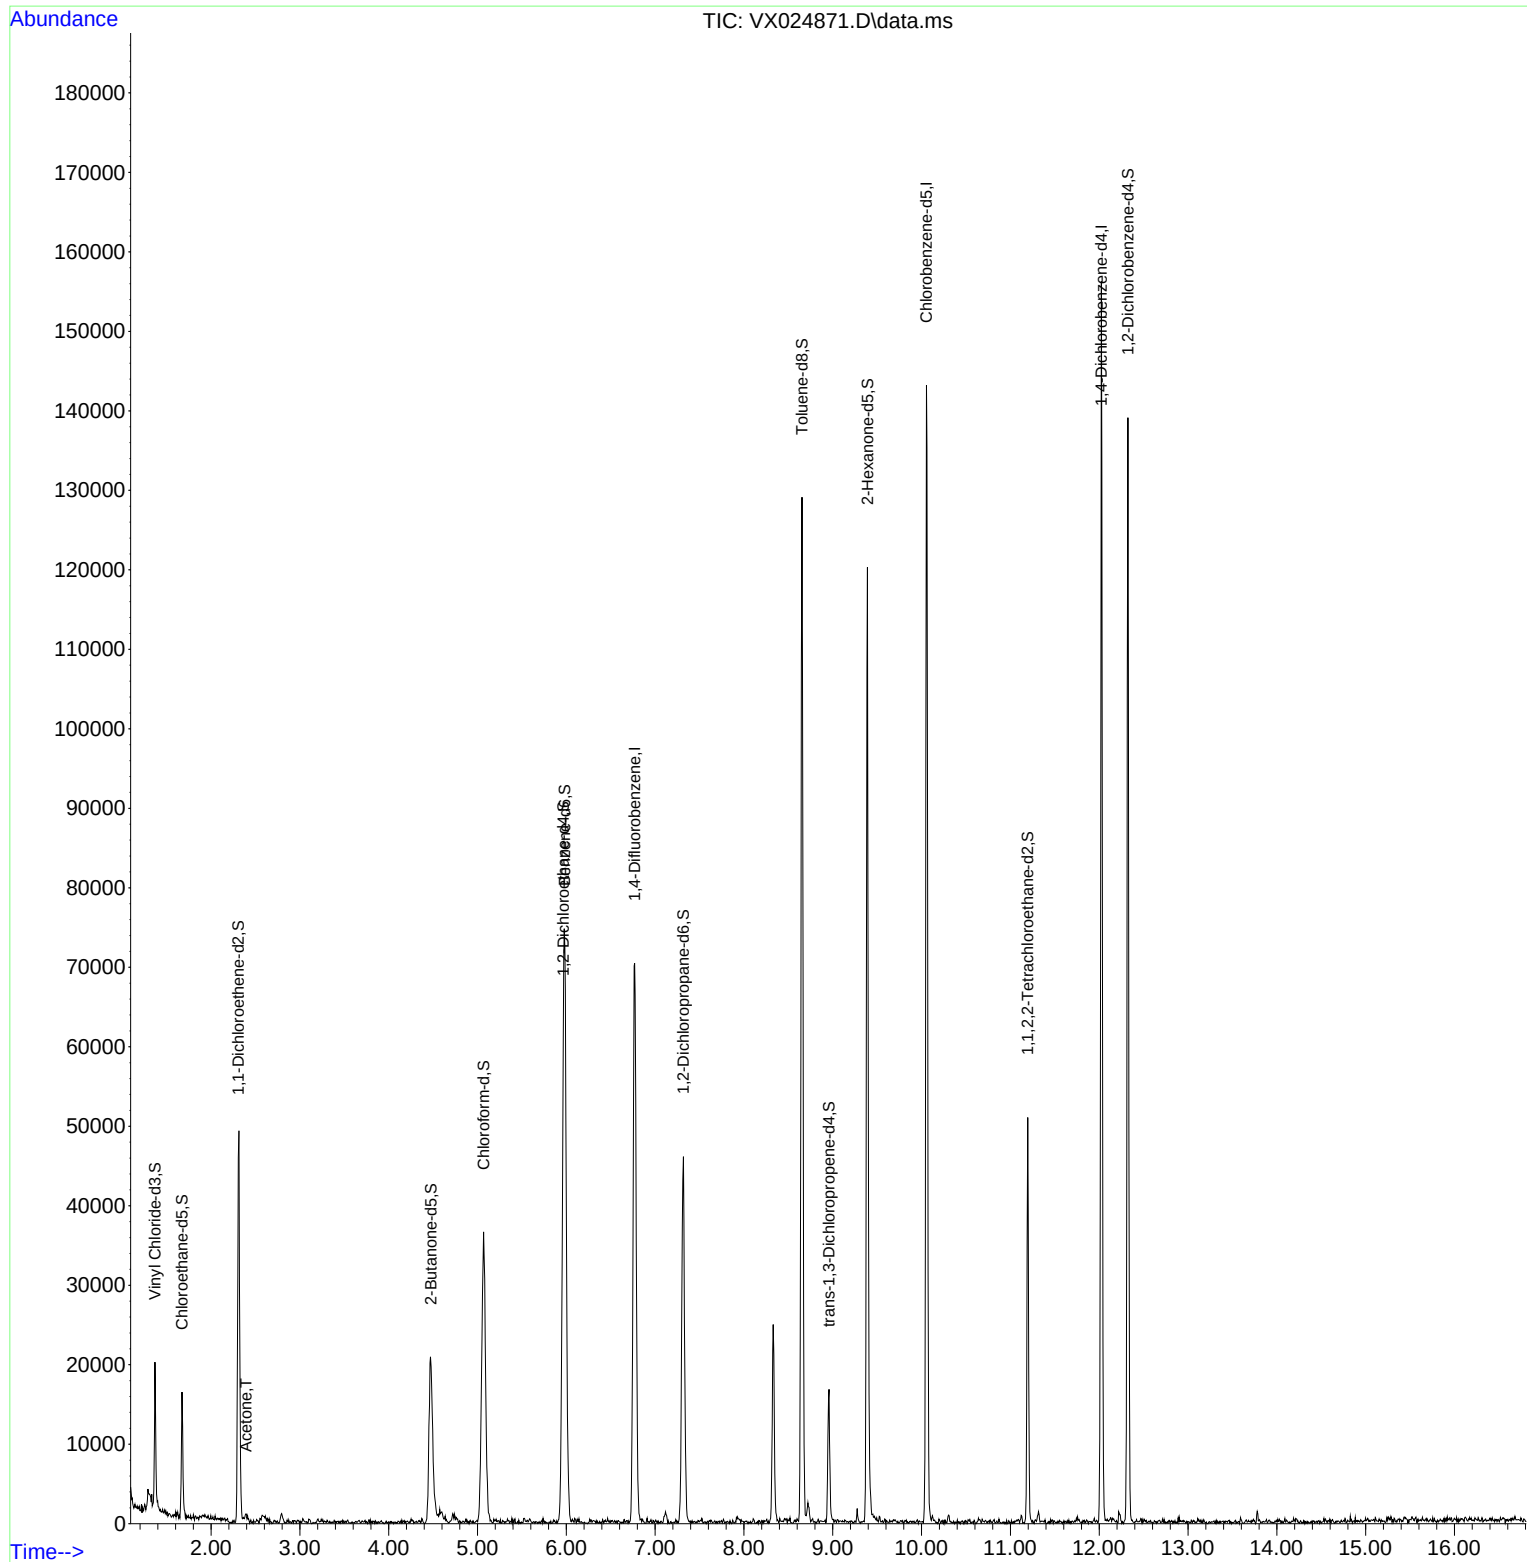

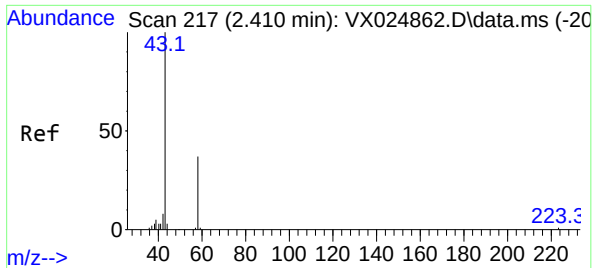

#13
Acetone
Concen: 2.183 ug/L
RT: 2.392 min Scan# 214
Delta R.T. -0.018 min
Lab File: VX024871.D
Acq: 22 Oct 2021 15:02

Instrument :
MSVOA_X
ClientSampleId :
P001-TW001-06

Tgt Ion: 43 Resp: 1214
Ion Ratio Lower Upper
43 100
58 34.9 0.0 64.2

