

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX102221\
 Data File : VX024876.D
 Acq On : 22 Oct 2021 17:00
 Operator : JC/MD
 Sample : M4291-07
 Misc : 25.0mL/MSVOA_X/WATER
 ALS Vial : 19 Sample Multiplier: 1

Instrument :
 MSVOA_X
 ClientSampleId :
 P007-TW001-02

Quant Time: Oct 23 03:55:45 2021
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXTR102221WMA.M
 Quant Title : TRACE VOA SFAM1.0
 QLast Update : Sat Oct 23 03:44:55 2021
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) 1,4-Difluorobenzene	6.769	114	70843	5.000	ug/L	0.00
28) Chlorobenzene-d5	10.055	117	67242	5.000	ug/L	0.00
58) 1,4-Dichlorobenzene-d4	12.024	152	32253	5.000	ug/L	0.00
System Monitoring Compounds						
4) Vinyl Chloride-d3	1.368	65	11611	5.583	ug/L	0.00
Spiked Amount	5.000	Range	40 - 130	Recovery	=	111.600%
7) Chloroethane-d5	1.672	69	10514	5.611	ug/L	0.00
Spiked Amount	5.000	Range	65 - 130	Recovery	=	112.200%
11) 1,1-Dichloroethene-d2	2.306	63	29889	3.855	ug/L	0.00
Spiked Amount	5.000	Range	60 - 125	Recovery	=	77.200%
20) 2-Butanone-d5	4.483	46	38802	51.029	ug/L	0.00
Spiked Amount	50.000	Range	40 - 130	Recovery	=	102.060%
24) Chloroform-d	5.074	84	54028	5.396	ug/L	0.00
Spiked Amount	5.000	Range	70 - 125	Recovery	=	108.000%
26) 1,2-Dichloroethane-d4	5.964	65	27124	4.957	ug/L	0.00
Spiked Amount	5.000	Range	70 - 130	Recovery	=	99.200%
32) Benzene-d6	5.983	84	85286	5.443	ug/L	0.00
Spiked Amount	5.000	Range	70 - 125	Recovery	=	108.800%
36) 1,2-Dichloropropane-d6	7.318	67	24652	4.932	ug/L	0.00
Spiked Amount	5.000	Range	60 - 140	Recovery	=	98.600%
41) Toluene-d8	8.653	98	81871	5.212	ug/L	0.00
Spiked Amount	5.000	Range	70 - 130	Recovery	=	104.200%
43) trans-1,3-Dichloroprop...	8.952	79	9917	4.322	ug/L	0.00
Spiked Amount	5.000	Range	55 - 130	Recovery	=	86.400%
46) 2-Hexanone-d5	9.391	63	39744	48.133	ug/L	0.00
Spiked Amount	50.000	Range	45 - 130	Recovery	=	96.260%
56) 1,1,2,2-Tetrachloroeth...	11.195	84	19048	4.986	ug/L	0.00
Spiked Amount	5.000	Range	65 - 120	Recovery	=	99.800%
66) 1,2-Dichlorobenzene-d4	12.323	152	30298	5.574	ug/L	0.00
Spiked Amount	5.000	Range	80 - 120	Recovery	=	111.400%
Target Compounds					Qvalue	
13) Acetone	2.410	43	1442	2.528	ug/L	51


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX102221\
Data File : VX024876.D
Acq On : 22 Oct 2021 17:00
Operator : JC/MD
Sample : M4291-07
Misc : 25.0mL/MSVOA_X/WATER
ALS Vial : 19 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
P007-TW001-02

Quant Time: Oct 23 03:55:45 2021
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXTR102221WMA.M
Quant Title : TRACE VOA SFAM1.0
QLast Update : Sat Oct 23 03:44:55 2021
Response via : Initial Calibration

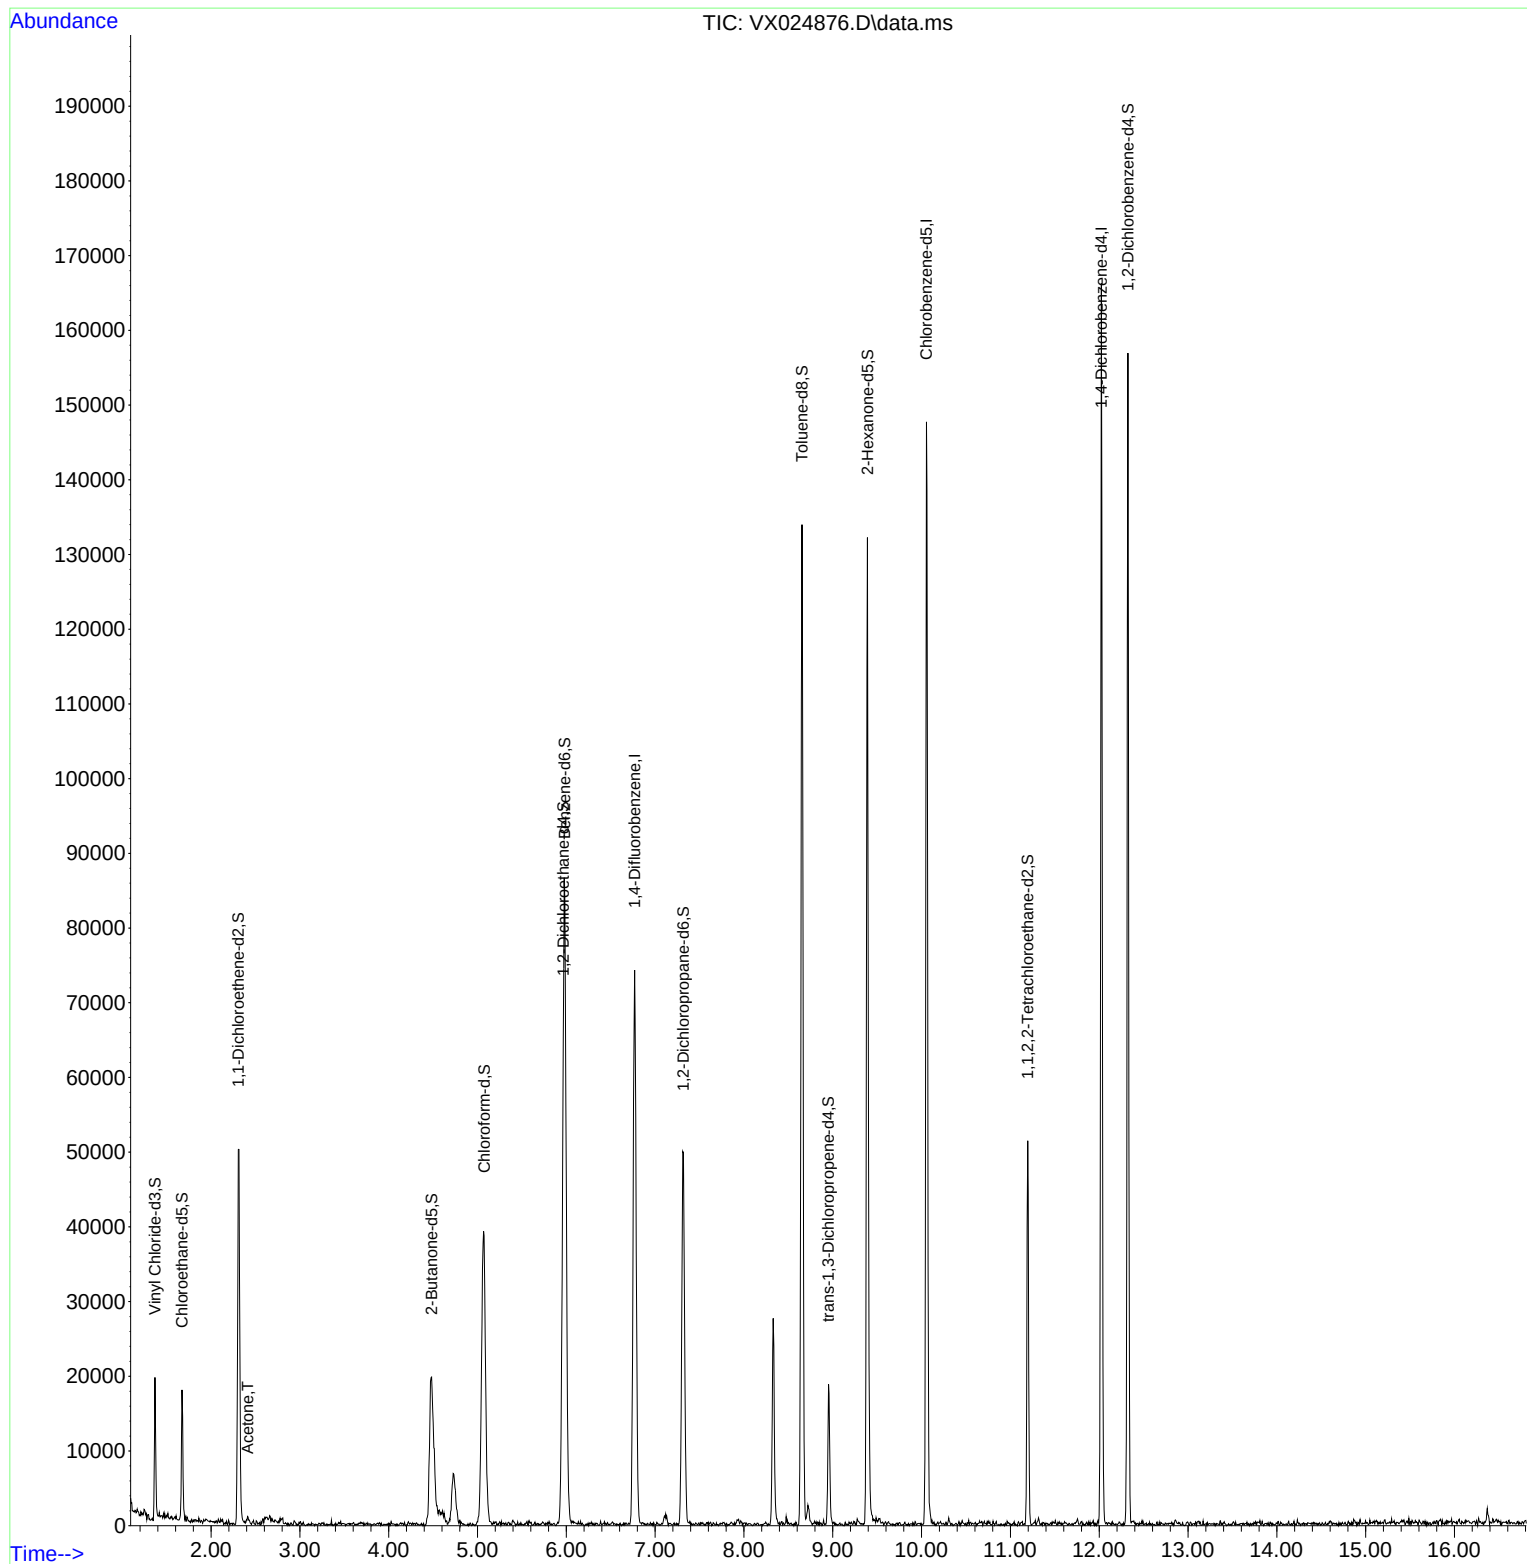

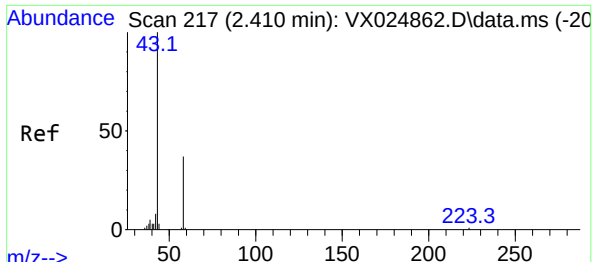

#13
 Acetone
 Concen: 2.528 ug/L
 RT: 2.410 min Scan# 217
 Delta R.T. -0.000 min
 Lab File: VX024876.D
 Acq: 22 Oct 2021 17:00

Instrument :
 MSVOA_X
 ClientSampleId :
 P007-TW001-02

Tgt Ion: 43 Resp: 1442
 Ion Ratio Lower Upper
 43 100
 58 4.9 0.0 64.2

