

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX102221\
 Data File : VX024879.D
 Acq On : 22 Oct 2021 18:11
 Operator : JC/MD
 Sample : M4291-10
 Misc : 25.0mL/MSVOA_X/WATER
 ALS Vial : 22 Sample Multiplier: 1

Instrument :
 MSVOA_X
 ClientSampleId :
 P022-TW001-02

Quant Time: Oct 23 03:56:20 2021
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXTR102221WMA.M
 Quant Title : TRACE VOA SFAM1.0
 QLast Update : Sat Oct 23 03:44:55 2021
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) 1,4-Difluorobenzene	6.769	114	70951	5.000	ug/L	0.00
28) Chlorobenzene-d5	10.061	117	65646	5.000	ug/L	0.00
58) 1,4-Dichlorobenzene-d4	12.024	152	31217	5.000	ug/L	0.00
System Monitoring Compounds						
4) Vinyl Chloride-d3	1.368	65	12324	5.917	ug/L	0.00
Spiked Amount	5.000	Range 40 - 130	Recovery	=	118.400%	
7) Chloroethane-d5	1.672	69	10489	5.589	ug/L	0.00
Spiked Amount	5.000	Range 65 - 130	Recovery	=	111.800%	
11) 1,1-Dichloroethene-d2	2.313	63	30961	3.987	ug/L	0.00
Spiked Amount	5.000	Range 60 - 125	Recovery	=	79.800%	
20) 2-Butanone-d5	4.483	46	40210	52.800	ug/L	0.00
Spiked Amount	50.000	Range 40 - 130	Recovery	=	105.600%	
24) Chloroform-d	5.062	84	53744	5.360	ug/L	-0.01
Spiked Amount	5.000	Range 70 - 125	Recovery	=	107.200%	
26) 1,2-Dichloroethane-d4	5.964	65	28884	5.270	ug/L	0.00
Spiked Amount	5.000	Range 70 - 130	Recovery	=	105.400%	
32) Benzene-d6	5.983	84	87376	5.712	ug/L	0.00
Spiked Amount	5.000	Range 70 - 125	Recovery	=	114.200%	
36) 1,2-Dichloropropane-d6	7.318	67	25055	5.134	ug/L	0.00
Spiked Amount	5.000	Range 60 - 140	Recovery	=	102.600%	
41) Toluene-d8	8.653	98	84213	5.491	ug/L	0.00
Spiked Amount	5.000	Range 70 - 130	Recovery	=	109.800%	
43) trans-1,3-Dichloroprop...	8.958	79	10352	4.622	ug/L	0.00
Spiked Amount	5.000	Range 55 - 130	Recovery	=	92.400%	
46) 2-Hexanone-d5	9.391	63	42645	52.902	ug/L	0.00
Spiked Amount	50.000	Range 45 - 130	Recovery	=	105.800%	
56) 1,1,2,2-Tetrachloroeth...	11.195	84	19574	5.248	ug/L	0.00
Spiked Amount	5.000	Range 65 - 120	Recovery	=	105.000%	
66) 1,2-Dichlorobenzene-d4	12.323	152	30008	5.704	ug/L	0.00
Spiked Amount	5.000	Range 80 - 120	Recovery	=	114.000%	
Target Compounds						Qvalue
34) Trichloroethene	7.135	95	3791	0.607	ug/L	94

(#) = qualifier out of range (m) = manual integration (+) = signals summed


Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX102221\
Data File : VX024879.D
Acq On : 22 Oct 2021 18:11
Operator : JC/MD
Sample : M4291-10
Misc : 25.0mL/MSVOA_X/WATER
ALS Vial : 22 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
P022-TW001-02

Quant Time: Oct 23 03:56:20 2021
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXTR102221WMA.M
Quant Title : TRACE VOA SFAM1.0
QLast Update : Sat Oct 23 03:44:55 2021
Response via : Initial Calibration

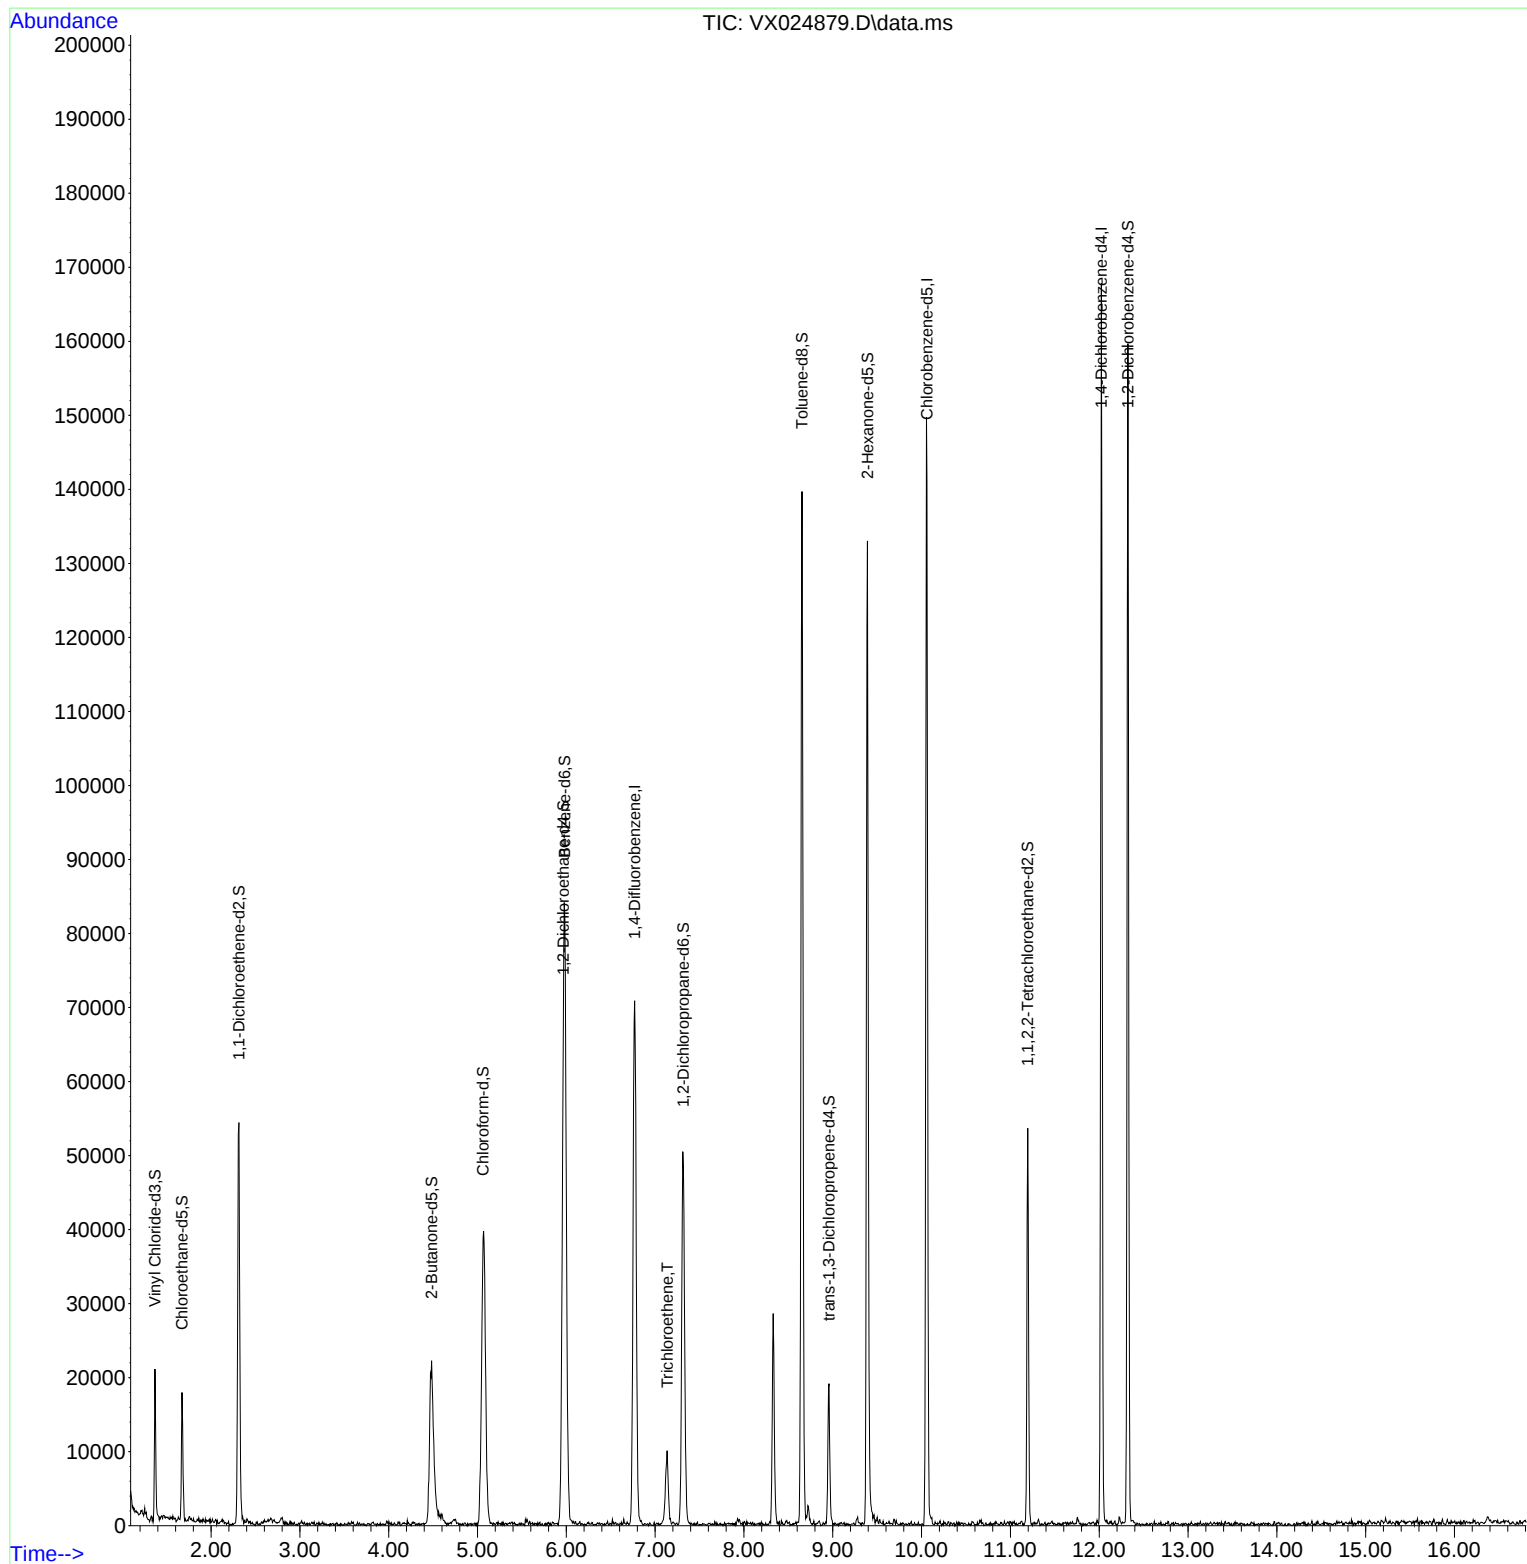


Abundance Scan 992 (7.135 min): VX024862.D\data.ms (-98

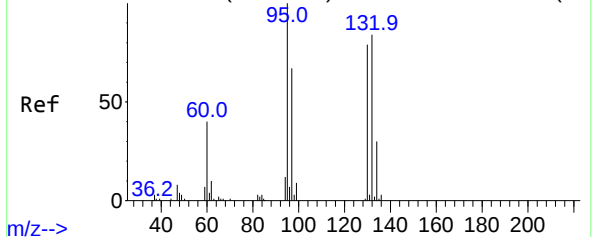

#34
Trichloroethene
Concen: 0.607 ug/L
RT: 7.135 min Scan# 992
Delta R.T. 0.000 min
Lab File: VX024879.D
Acq: 22 Oct 2021 18:11

Tgt Ion: 95	Resp:	3791
Ion	Ratio	Lower Upper
95	100	
97	70.2	46.6 86.6
132	92.4	58.4 108.6
130	81.5	55.4 103.0

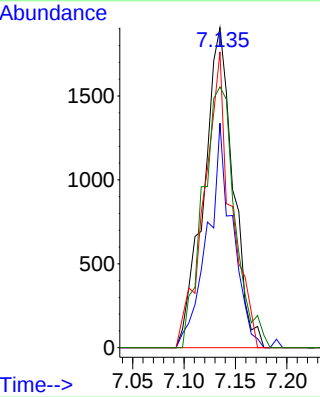

Instrument :
MSVOA_X
ClientSampleId :
P022-TW001-02