

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX102221\
 Data File : VX024880.D
 Acq On : 22 Oct 2021 18:35
 Operator : JC/MD
 Sample : M4291-11
 Misc : 25.0mL/MSVOA_X/WATER
 ALS Vial : 23 Sample Multiplier: 1

Instrument :
 MSVOA_X
 ClientSampleId :
 P028-TW001-01

Quant Time: Oct 23 03:56:31 2021
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXTR102221WMA.M
 Quant Title : TRACE VOA SFAM1.0
 QLast Update : Sat Oct 23 03:44:55 2021
 Response via : Initial Calibration

Compound	R.T. QIon		Response	Conc	Units	Dev(Min)


Internal Standards						
1) 1,4-Difluorobenzene	6.769	114	74689	5.000	ug/L	0.00
28) Chlorobenzene-d5	10.055	117	66875	5.000	ug/L	0.00
58) 1,4-Dichlorobenzene-d4	12.024	152	32047	5.000	ug/L	0.00
System Monitoring Compounds						
4) Vinyl Chloride-d3	1.367	65	11980	5.464	ug/L	0.00
Spiked Amount	5.000	Range 40 - 130	Recovery	= 109.200%		
7) Chloroethane-d5	1.672	69	11005	5.570	ug/L	0.00
Spiked Amount	5.000	Range 65 - 130	Recovery	= 111.400%		
11) 1,1-Dichloroethene-d2	2.306	63	31461	3.849	ug/L	0.00
Spiked Amount	5.000	Range 60 - 125	Recovery	= 77.000%		
20) 2-Butanone-d5	4.483	46	42459	52.963	ug/L	0.00
Spiked Amount	50.000	Range 40 - 130	Recovery	= 105.920%		
24) Chloroform-d	5.068	84	55010	5.211	ug/L	0.00
Spiked Amount	5.000	Range 70 - 125	Recovery	= 104.200%		
26) 1,2-Dichloroethane-d4	5.964	65	29694	5.147	ug/L	0.00
Spiked Amount	5.000	Range 70 - 130	Recovery	= 103.000%		
32) Benzene-d6	5.976	84	90451	5.805	ug/L	0.00
Spiked Amount	5.000	Range 70 - 125	Recovery	= 116.000%		
36) 1,2-Dichloropropane-d6	7.317	67	25894	5.209	ug/L	0.00
Spiked Amount	5.000	Range 60 - 140	Recovery	= 104.200%		
41) Toluene-d8	8.653	98	85707	5.486	ug/L	0.00
Spiked Amount	5.000	Range 70 - 130	Recovery	= 109.800%		
43) trans-1,3-Dichloroprop...	8.951	79	10528	4.614	ug/L	0.00
Spiked Amount	5.000	Range 55 - 130	Recovery	= 92.200%		
46) 2-Hexanone-d5	9.390	63	43070	52.447	ug/L	0.00
Spiked Amount	50.000	Range 45 - 130	Recovery	= 104.900%		
56) 1,1,2,2-Tetrachloroeth...	11.195	84	20986	5.523	ug/L	0.00
Spiked Amount	5.000	Range 65 - 120	Recovery	= 110.400%		
66) 1,2-Dichlorobenzene-d4	12.323	152	28974	5.365	ug/L	0.00
Spiked Amount	5.000	Range 80 - 120	Recovery	= 107.200%		
Target Compounds						Qvalue
13) Acetone	2.404	43	1571	2.613	ug/L	92


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX102221\
Data File : VX024880.D
Acq On : 22 Oct 2021 18:35
Operator : JC/MD
Sample : M4291-11
Misc : 25.0mL/MSVOA_X/WATER
ALS Vial : 23 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
P028-TW001-01

Quant Time: Oct 23 03:56:31 2021
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXTR102221WMA.M
Quant Title : TRACE VOA SFAM1.0
QLast Update : Sat Oct 23 03:44:55 2021
Response via : Initial Calibration

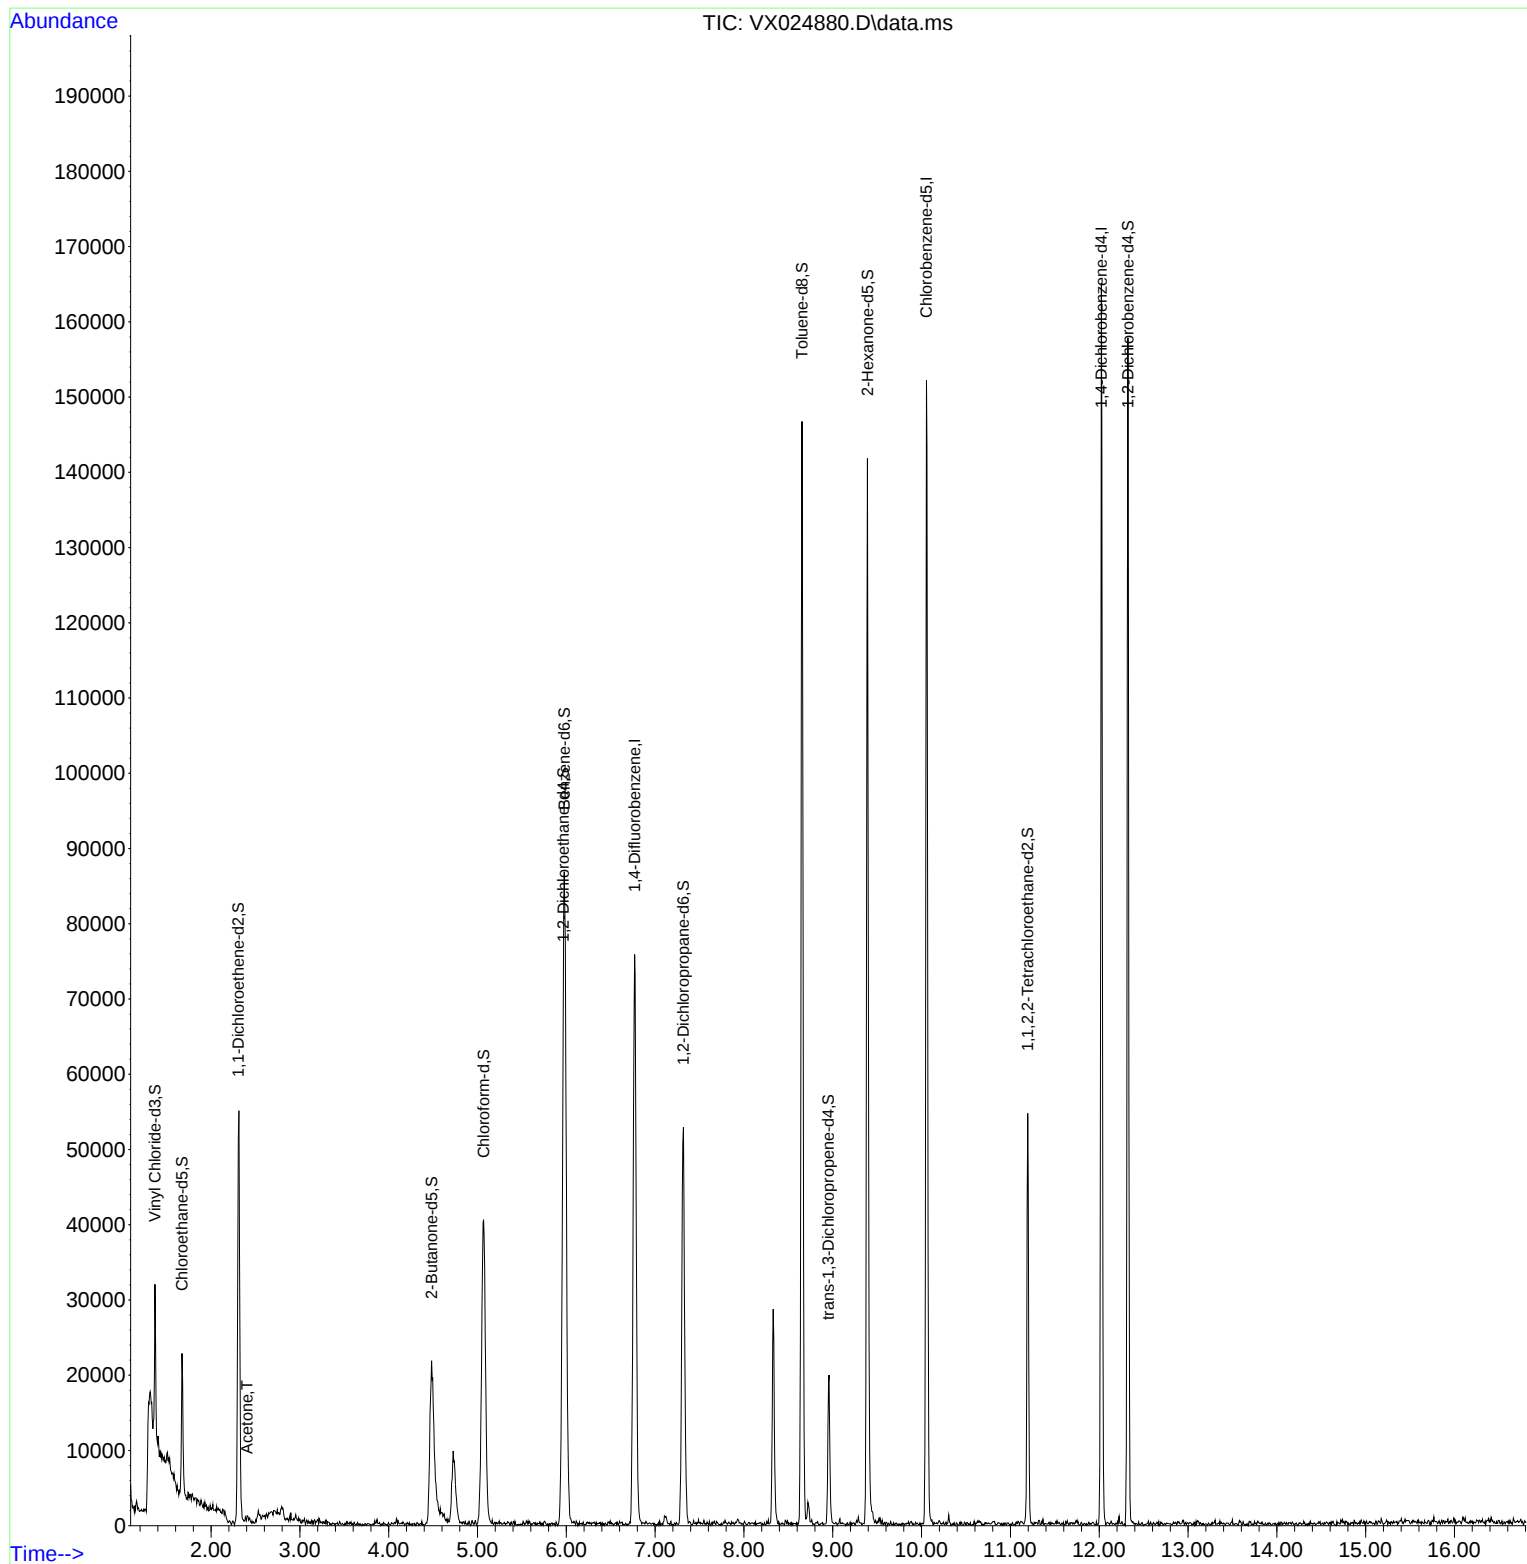

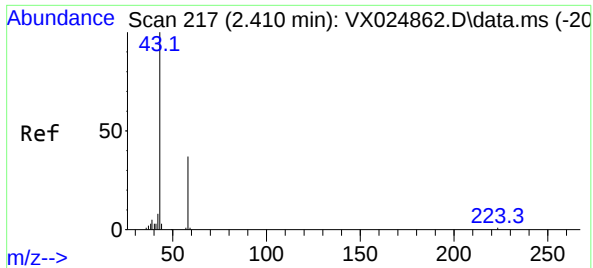

#13
Acetone
Concen: 2.613 ug/L
RT: 2.404 min Scan# 216
Delta R.T. -0.006 min
Lab File: VX024880.D
Acq: 22 Oct 2021 18:35

Instrument :
MSVOA_X
ClientSampleId :
P028-TW001-01

Tgt Ion: 43 Resp: 1571
Ion Ratio Lower Upper
43 100
58 36.3 0.0 64.2

