

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX102221\
 Data File : VX024882.D
 Acq On : 22 Oct 2021 19:23
 Operator : JC/MD
 Sample : M4291-13
 Misc : 25.0mL/MSVOA_X/WATER
 ALS Vial : 25 Sample Multiplier: 1

Instrument :
 MSVOA_X
 ClientSampleId :
 P030-TW001-01

Quant Time: Oct 23 03:56:54 2021
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXTR102221WMA.M
 Quant Title : TRACE VOA SFAM1.0
 QLast Update : Sat Oct 23 03:44:55 2021
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) 1,4-Difluorobenzene	6.769	114	76526	5.000	ug/L	0.00
28) Chlorobenzene-d5	10.055	117	70002	5.000	ug/L	0.00
58) 1,4-Dichlorobenzene-d4	12.024	152	32578	5.000	ug/L	0.00
System Monitoring Compounds						
4) Vinyl Chloride-d3	1.368	65	13258	5.901	ug/L	0.00
Spiked Amount	5.000	Range	40 - 130	Recovery	=	118.000%
7) Chloroethane-d5	1.672	69	11817	5.838	ug/L	0.00
Spiked Amount	5.000	Range	65 - 130	Recovery	=	116.800%
11) 1,1-Dichloroethene-d2	2.313	63	34617	4.134	ug/L	0.00
Spiked Amount	5.000	Range	60 - 125	Recovery	=	82.600%
20) 2-Butanone-d5	4.483	46	46772	56.942	ug/L	0.00
Spiked Amount	50.000	Range	40 - 130	Recovery	=	113.880%
24) Chloroform-d	5.068	84	58285	5.389	ug/L	0.00
Spiked Amount	5.000	Range	70 - 125	Recovery	=	107.800%
26) 1,2-Dichloroethane-d4	5.964	65	30752	5.202	ug/L	0.00
Spiked Amount	5.000	Range	70 - 130	Recovery	=	104.000%
32) Benzene-d6	5.983	84	95050	5.827	ug/L	0.00
Spiked Amount	5.000	Range	70 - 125	Recovery	=	116.600%
36) 1,2-Dichloropropane-d6	7.312	67	29373	5.645	ug/L	0.00
Spiked Amount	5.000	Range	60 - 140	Recovery	=	112.800%
41) Toluene-d8	8.653	98	93900	5.742	ug/L	0.00
Spiked Amount	5.000	Range	70 - 130	Recovery	=	114.800%
43) trans-1,3-Dichloroprop...	8.958	79	11117	4.654	ug/L	0.00
Spiked Amount	5.000	Range	55 - 130	Recovery	=	93.000%
46) 2-Hexanone-d5	9.391	63	47700	55.491	ug/L	0.00
Spiked Amount	50.000	Range	45 - 130	Recovery	=	110.980%
56) 1,1,2,2-Tetrachloroeth...	11.195	84	21676	5.450	ug/L	0.00
Spiked Amount	5.000	Range	65 - 120	Recovery	=	109.000%
66) 1,2-Dichlorobenzene-d4	12.323	152	31677	5.770	ug/L	0.00
Spiked Amount	5.000	Range	80 - 120	Recovery	=	115.400%
Target Compounds						
13) Acetone	2.410	43	947	1.537	ug/L	90


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX102221\
Data File : VX024882.D
Acq On : 22 Oct 2021 19:23
Operator : JC/MD
Sample : M4291-13
Misc : 25.0mL/MSVOA_X/WATER
ALS Vial : 25 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
P030-TW001-01

Quant Time: Oct 23 03:56:54 2021
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXTR102221WMA.M
Quant Title : TRACE VOA SFAM1.0
QLast Update : Sat Oct 23 03:44:55 2021
Response via : Initial Calibration

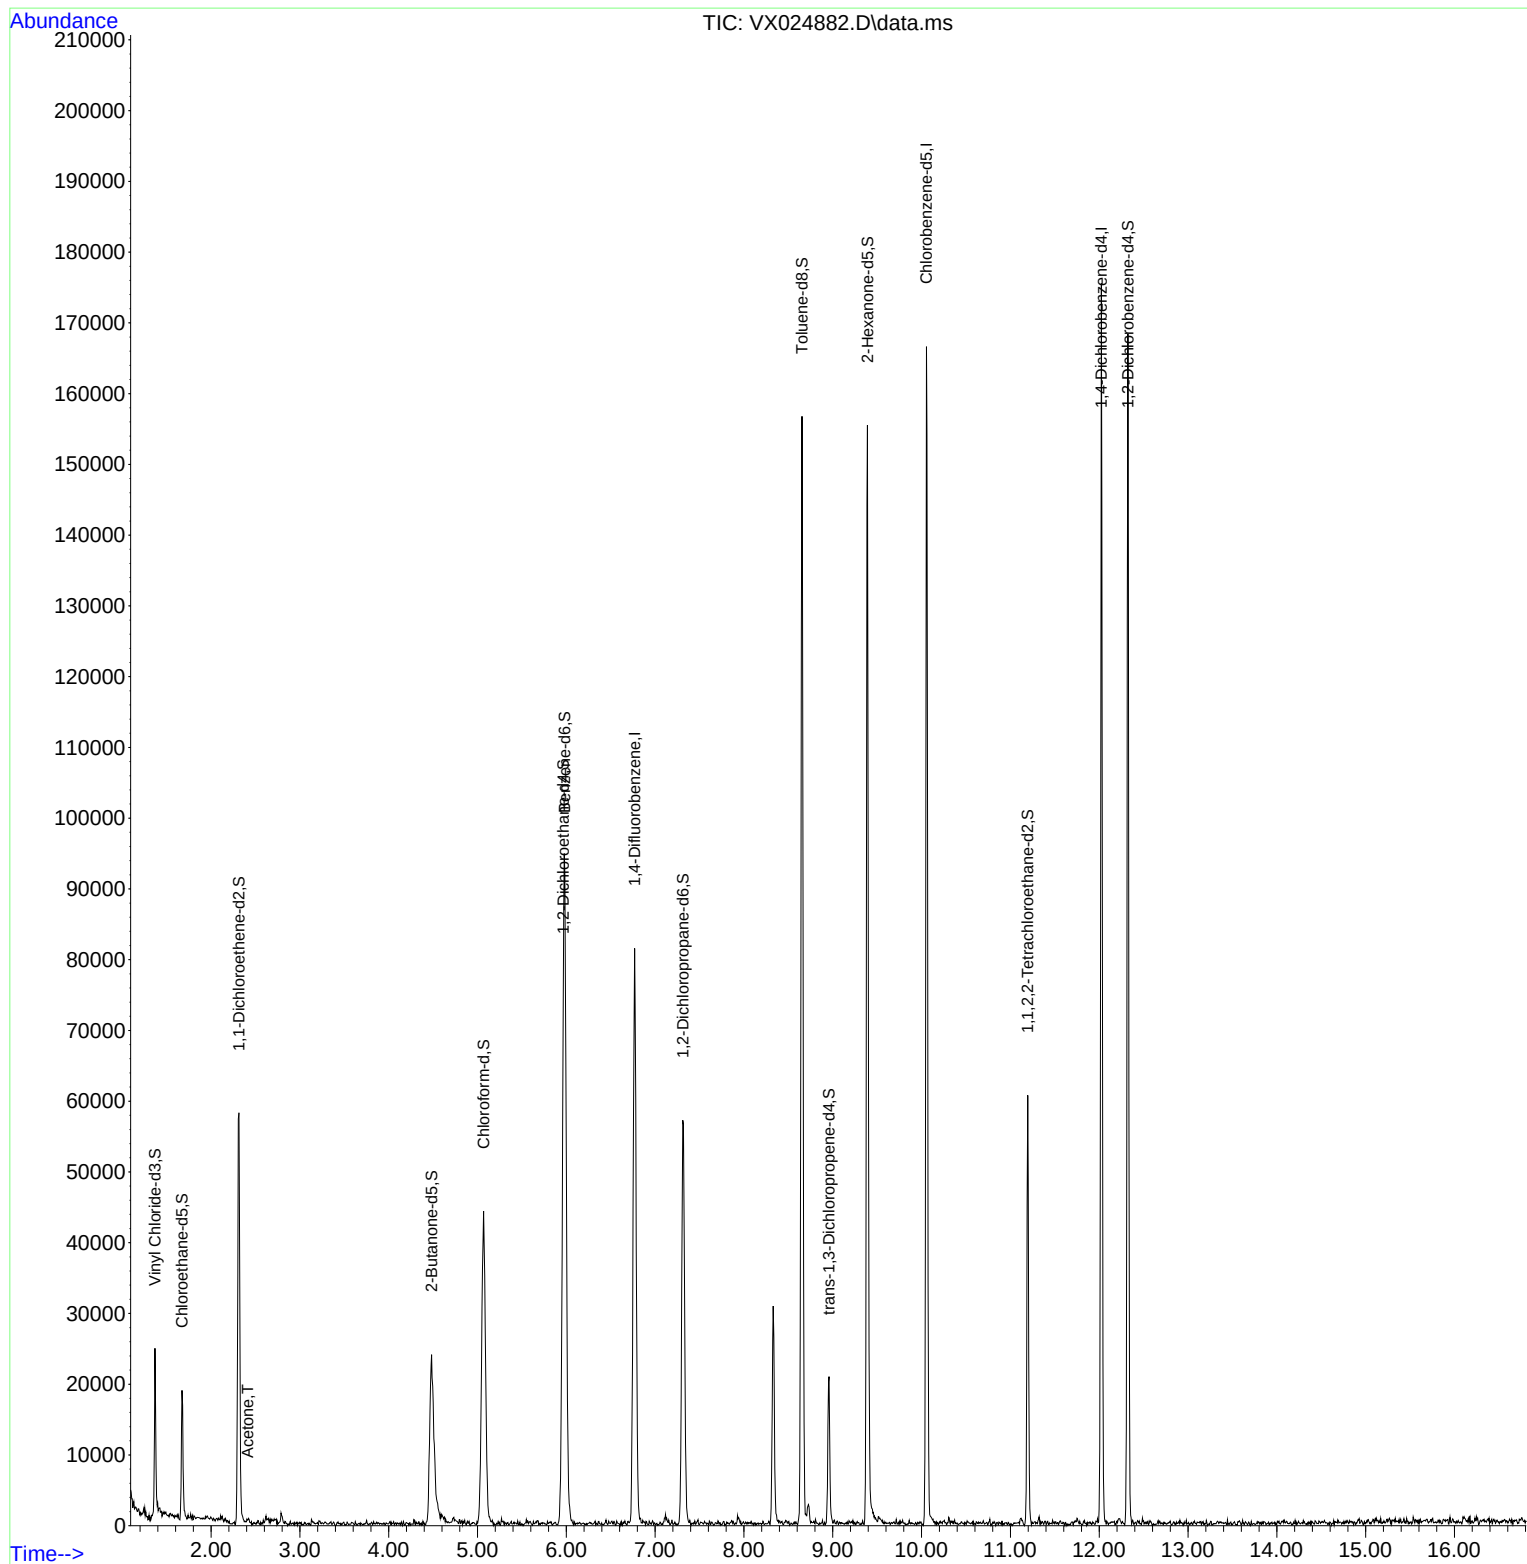

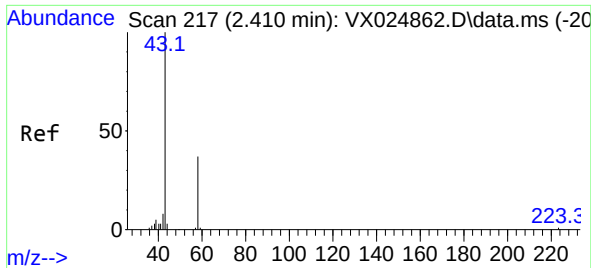

#13
Acetone
Concen: 1.537 ug/L
RT: 2.410 min Scan# 217
Delta R.T. 0.000 min
Lab File: VX024882.D
Acq: 22 Oct 2021 19:23

Instrument :
MSVOA_X
ClientSampleId :
P030-TW001-01

Tgt Ion: 43 Resp: 947
Ion Ratio Lower Upper
43 100
58 37.9 0.0 64.2

