

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX102221\
 Data File : VX024866.D
 Acq On : 22 Oct 2021 13:03
 Operator : JC/MD
 Sample : VX1022WBL01
 Misc : 25.0mL/MSVOA_X/WATER
 ALS Vial : 9 Sample Multiplier: 1

Instrument :
 MSVOA_X
 ClientSampleId :
 VBLK604

Integration Parameters: rteint.p

Integrator: RTE

Smoothing : ON

Filtering: 5

Sampling : 1

Min Area: 3 % of largest Peak

Start Thrs: 0.1

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXTR102221WMA.M

Title : TRACE VOA SFAM1.0

Signal : TIC: VX024866.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.367	43	46	52	rVB	18762	19500	7.91%	0.909%
2	1.672	92	96	104	rVB	15896	19424	7.88%	0.906%
3	2.312	194	201	213	rVB	47890	79019	32.07%	3.684%
4	2.794	274	280	290	rBV2	6261	11172	4.53%	0.521%
5	4.483	546	557	573	rBV2	20883	75426	30.61%	3.517%
6	5.068	642	653	666	rVB2	40589	123771	50.23%	5.771%
7	5.976	789	802	814	rBV4	84361	246401	100.00%	11.488%
8	6.769	922	932	946	rBV	82858	192541	78.14%	8.977%
9	7.129	984	991	995	rVB5	2214	4539	1.84%	0.212%
10	7.318	1010	1022	1031	rBV	50185	112173	45.52%	5.230%
11	8.330	1182	1188	1194	rBV2	32289	52737	21.40%	2.459%
12	8.653	1235	1241	1248	rBV	144613	216951	88.05%	10.115%
13	8.726	1248	1253	1258	rVB3	3258	5493	2.23%	0.256%
14	8.957	1285	1291	1301	rVB	20377	32137	13.04%	1.498%
15	9.390	1355	1362	1373	rBV	140789	204939	83.17%	9.555%
16	10.055	1463	1471	1484	rBV	160176	227987	92.53%	10.630%
17	10.305	1509	1512	1517	rVB3	1675	2679	1.09%	0.125%
18	10.646	1564	1568	1574	rBV4	1773	3504	1.42%	0.163%
19	11.195	1653	1658	1665	rBV2	58816	74425	30.20%	3.470%
20	12.024	1789	1794	1800	rBV	177822	234591	95.21%	10.938%
21	12.323	1838	1843	1849	rBV	159177	205359	83.34%	9.575%




Sum of corrected areas: 2144768

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX102221\
Data File : VX024866.D
Acq On : 22 Oct 2021 13:03
Operator : JC/MD
Sample : VX1022WBL01
Misc : 25.0mL/MSVOA_X/WATER
ALS Vial : 9 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
VBLK604

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXTR102221WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

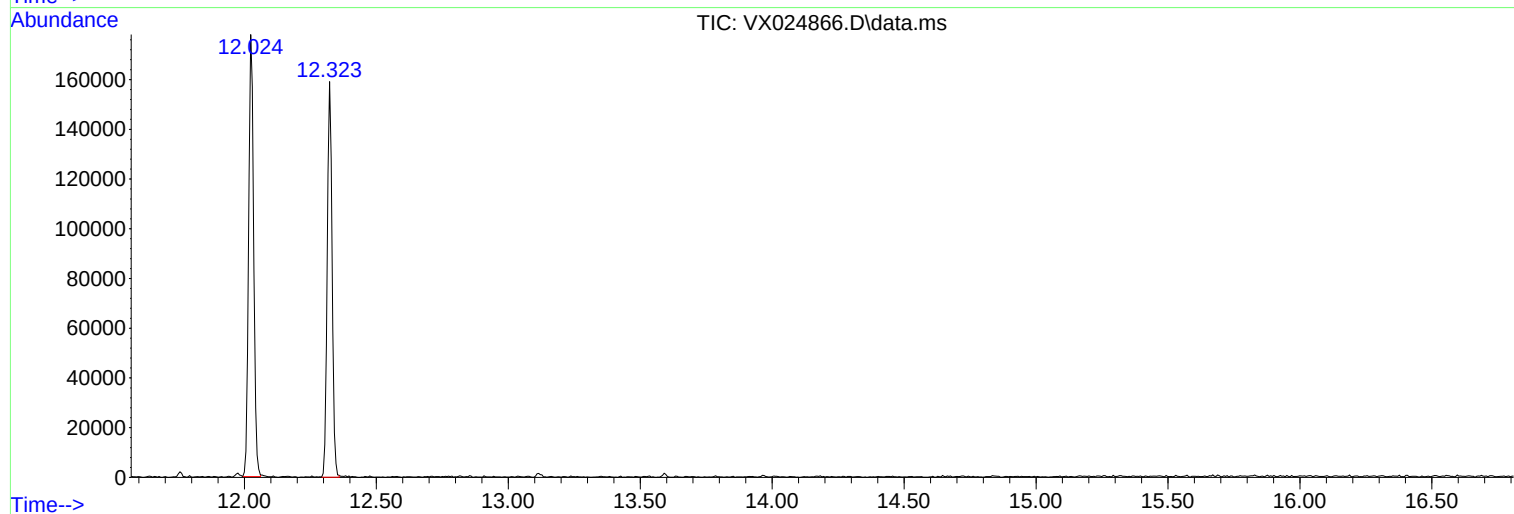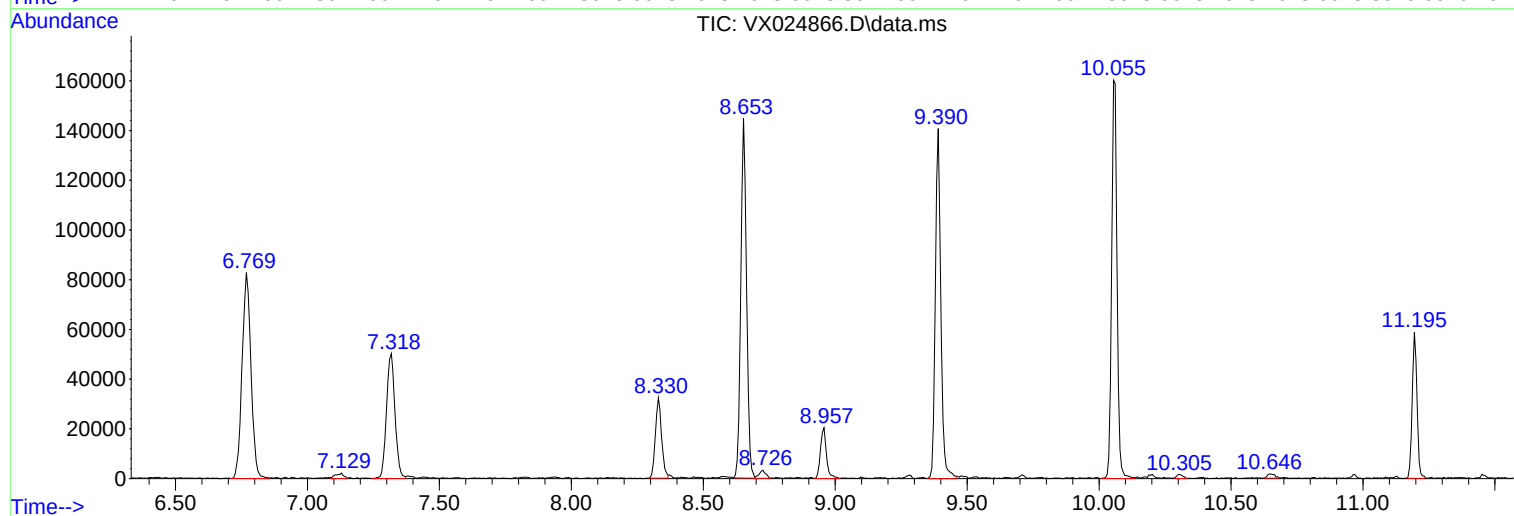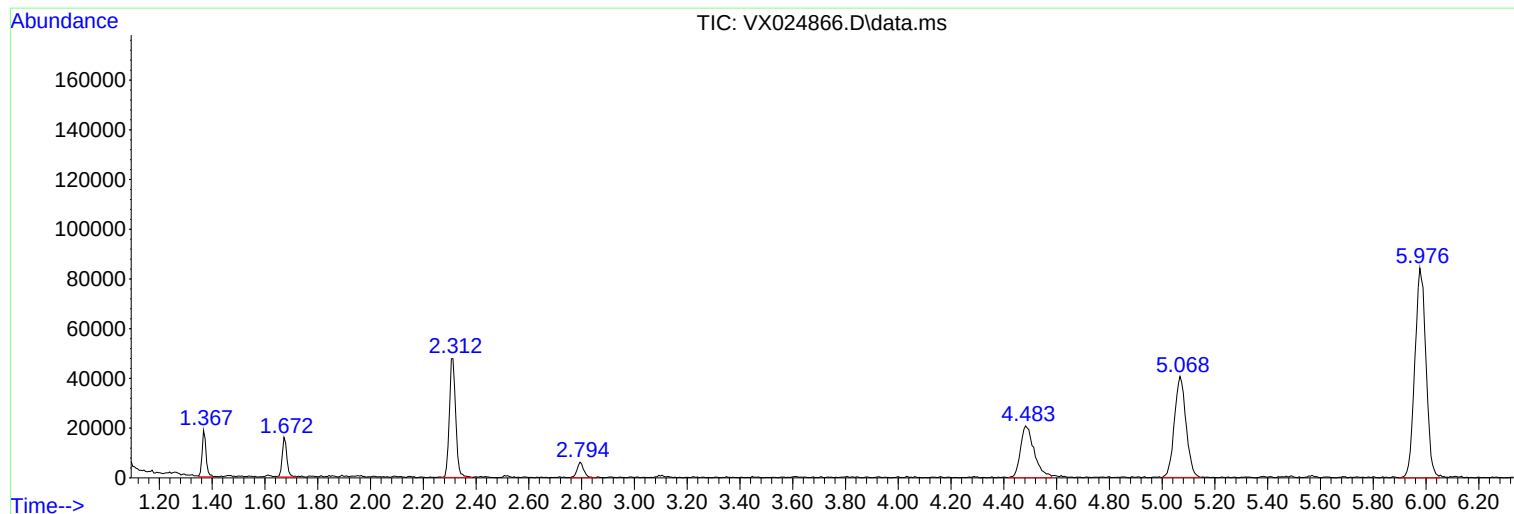

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX102221\
Data File : VX024866.D
Acq On : 22 Oct 2021 13:03
Operator : JC/MD
Sample : VX1022WBL01
Misc : 25.0mL/MSVOA_X/WATER
ALS Vial : 9 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
VBLK604

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXTR102221WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX102221\
Data File : VX024866.D
Acq On : 22 Oct 2021 13:03
Operator : JC/MD
Sample : VX1022WBL01
Misc : 25.0mL/MSVOA_X/WATER
ALS Vial : 9 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
VBLK604

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXTR102221WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST0.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc
