

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX102221\
 Data File : VX024870.D
 Acq On : 22 Oct 2021 14:38
 Operator : JC/MD
 Sample : M4291-01
 Misc : 25.0mL/MSVOA_X/WATER
 ALS Vial : 13 Sample Multiplier: 1

Instrument :
 MSVOA_X
 ClientSampleId :
 P001-TW001-05

Integration Parameters: rteint.p

Integrator: RTE

Smoothing : ON

Filtering: 5

Sampling : 1

Min Area: 3 % of largest Peak

Start Thrs: 0.1

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXTR102221WMA.M

Title : TRACE VOA SFAM1.0

Signal : TIC: VX024870.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.368	42	46	52	rBV	21068	21156	8.49%	1.049%
2	1.672	92	96	101	rVB	16332	19559	7.85%	0.970%
3	2.306	194	200	210	rBV	53778	86355	34.67%	4.283%
4	4.477	546	556	570	rBV2	22019	69508	27.91%	3.448%
5	5.068	641	653	667	rBV3	41440	125855	50.53%	6.243%
6	5.977	791	802	813	rBV4	85666	249077	100.00%	12.355%
7	6.769	922	932	940	rBV	69097	164239	65.94%	8.147%
8	7.129	988	991	996	rVB4	1852	3028	1.22%	0.150%
9	7.312	1013	1021	1030	rBV2	50788	112938	45.34%	5.602%
10	8.330	1181	1188	1199	rBV	29717	48289	19.39%	2.395%
11	8.653	1233	1241	1248	rBV	144084	224971	90.32%	11.159%
12	8.726	1248	1253	1257	rVB2	3161	5436	2.18%	0.270%
13	8.952	1285	1290	1296	rBV	19650	29192	11.72%	1.448%
14	9.391	1356	1362	1374	rBV	128371	188843	75.82%	9.367%
15	10.055	1466	1471	1479	rBV	133817	190765	76.59%	9.462%
16	10.305	1505	1512	1515	rBV2	2275	3312	1.33%	0.164%
17	10.659	1563	1570	1575	rBV6	2103	4373	1.76%	0.217%
18	11.195	1653	1658	1664	rBV	55477	69089	27.74%	3.427%
19	11.750	1745	1749	1756	rVB	2153	3222	1.29%	0.160%
20	12.024	1789	1794	1801	rVV	154034	194149	77.95%	9.630%
21	12.323	1837	1843	1851	rVB	160419	198971	79.88%	9.869%
22	13.780	2077	2082	2088	rVB2	2738	3725	1.50%	0.185%


Sum of corrected areas: 2016052

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX102221\
Data File : VX024870.D
Acq On : 22 Oct 2021 14:38
Operator : JC/MD
Sample : M4291-01
Misc : 25.0mL/MSVOA_X/WATER
ALS Vial : 13 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
P001-TW001-05

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXTR102221WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

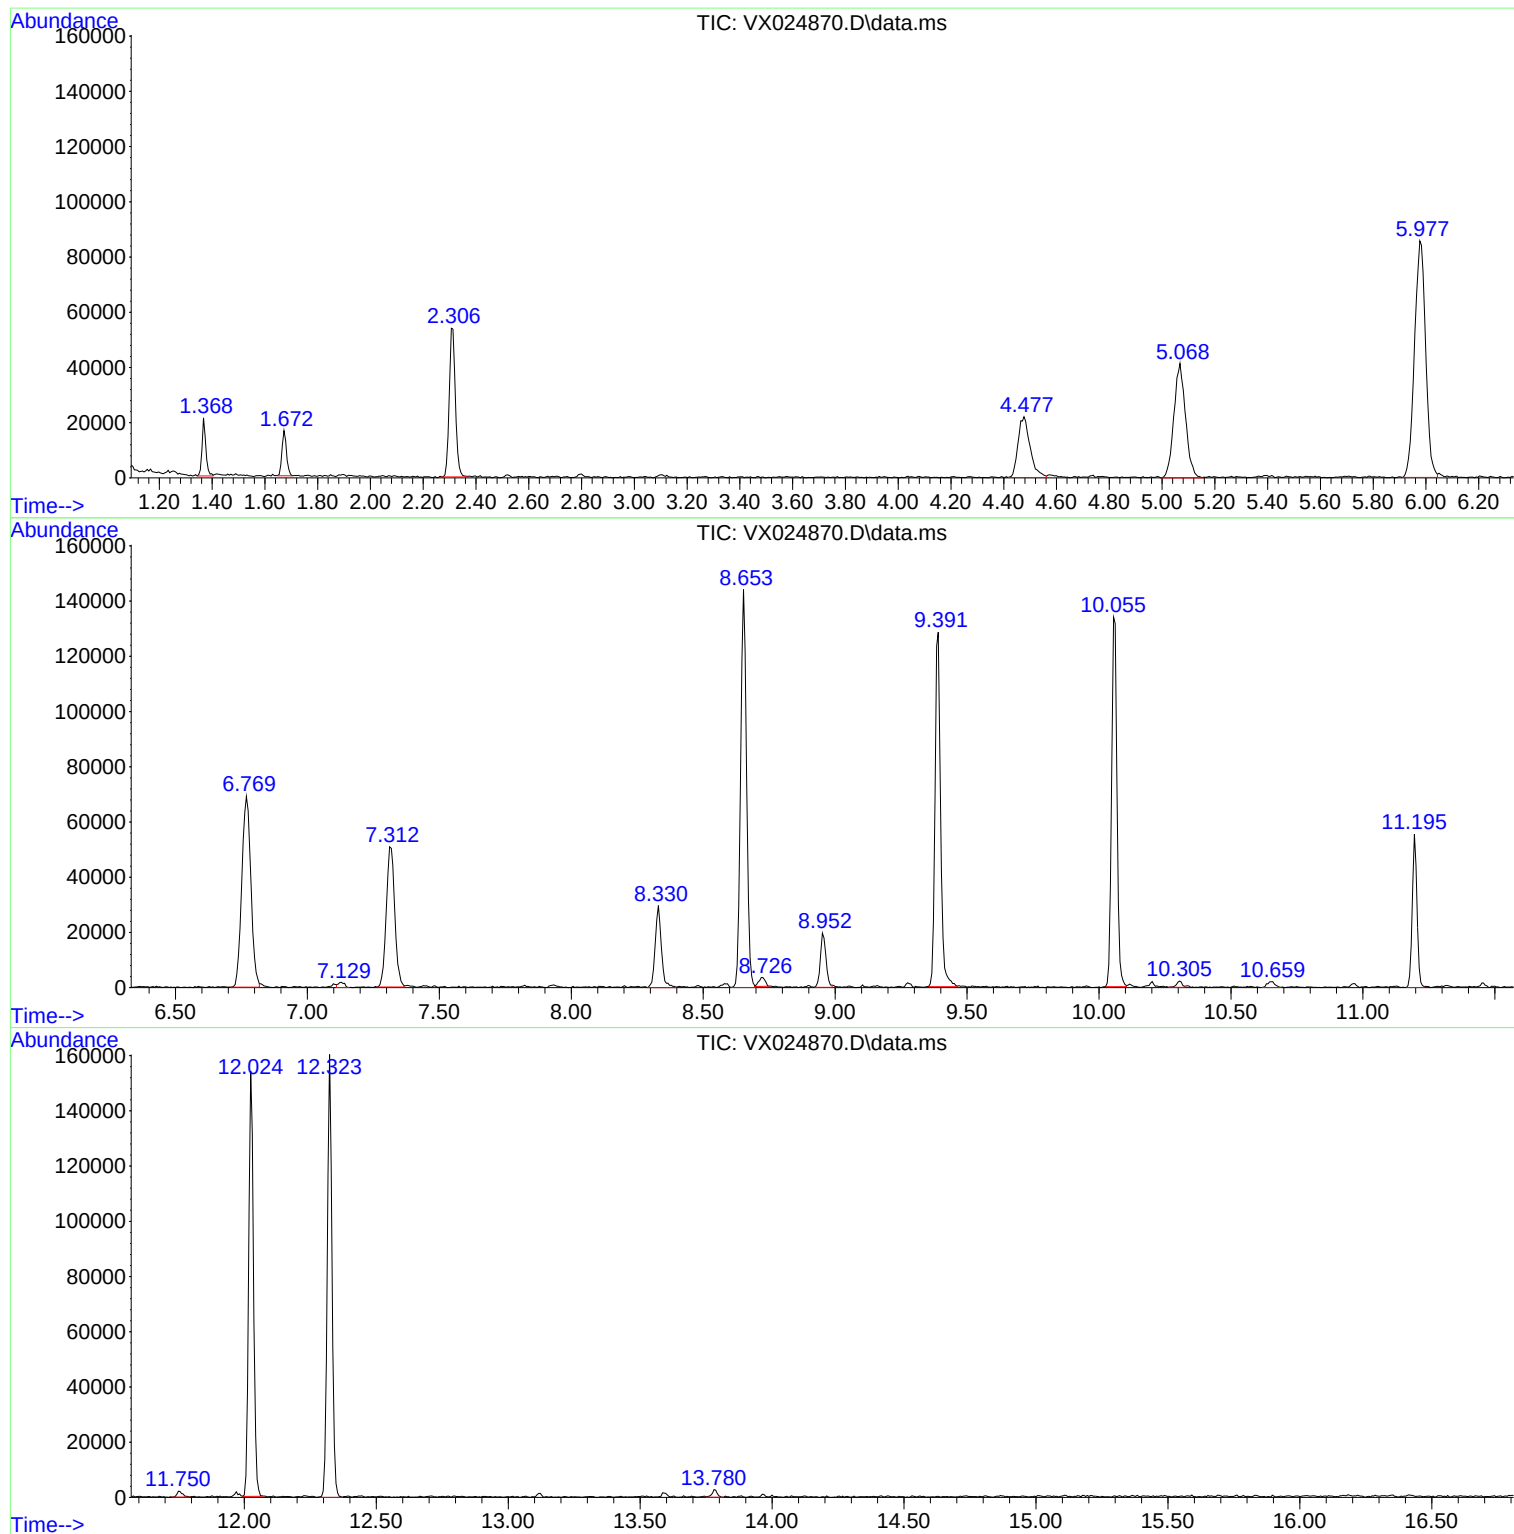

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX102221\
Data File : VX024870.D
Acq On : 22 Oct 2021 14:38
Operator : JC/MD
Sample : M4291-01
Misc : 25.0mL/MSVOA_X/WATER
ALS Vial : 13 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
P001-TW001-05

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXTR102221WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX102221\
Data File : VX024870.D
Acq On : 22 Oct 2021 14:38
Operator : JC/MD
Sample : M4291-01
Misc : 25.0mL/MSVOA_X/WATER
ALS Vial : 13 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
P001-TW001-05

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXTR102221WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc
