

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX102221\
 Data File : VX024871.D
 Acq On : 22 Oct 2021 15:02
 Operator : JC/MD
 Sample : M4291-04
 Misc : 25.0mL/MSVOA_X/WATER
 ALS Vial : 14 Sample Multiplier: 1

Instrument :
 MSVOA_X
 ClientSampleId :
 P001-TW001-06

Integration Parameters: rteint.p

Integrator: RTE

Smoothing : ON

Filtering: 5

Sampling : 1

Min Area: 3 % of largest Peak

Start Thrs: 0.1

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXTR102221WMA.M

Title : TRACE VOA SFAM1.0

Signal : TIC: VX024871.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.288	29	33	35	rBV3	2635	3243	1.45%	0.173%
2	1.368	42	46	55	rVB	18704	20799	9.32%	1.110%
3	1.672	92	96	104	rVB	15920	19419	8.70%	1.036%
4	2.313	194	201	208	rBV	49299	76061	34.08%	4.059%
5	2.794	274	280	285	rBV4	1218	2277	1.02%	0.122%
6	4.471	544	555	567	rBV2	20995	63194	28.31%	3.372%
7	5.068	642	653	665	rBV2	36452	108805	48.75%	5.806%
8	5.977	789	802	815	rBV3	74782	223186	100.00%	11.911%
9	6.769	922	932	942	rBV2	70360	170708	76.49%	9.110%
10	7.117	983	989	993	rVB3	1386	2486	1.11%	0.133%
11	7.318	1013	1022	1034	rBV	46032	100978	45.24%	5.389%
12	8.330	1180	1188	1195	rBV2	24999	41803	18.73%	2.231%
13	8.653	1235	1241	1248	rBV	128857	198138	88.78%	10.574%
14	8.720	1249	1252	1257	rVB4	2407	3938	1.76%	0.210%
15	8.958	1285	1291	1298	rBV	16781	25902	11.61%	1.382%
16	9.391	1356	1362	1370	rBV	120064	170124	76.23%	9.079%
17	10.055	1465	1471	1480	rBV	143104	201537	90.30%	10.755%
18	11.195	1652	1658	1666	rBV	51062	63285	28.36%	3.377%
19	12.024	1788	1794	1801	rBV	156163	200597	89.88%	10.705%
20	12.323	1837	1843	1855	rVB	139034	177369	79.47%	9.465%




Sum of corrected areas: 1873849

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX102221\
Data File : VX024871.D
Acq On : 22 Oct 2021 15:02
Operator : JC/MD
Sample : M4291-04
Misc : 25.0mL/MSVOA_X/WATER
ALS Vial : 14 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
P001-TW001-06

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXTR102221WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

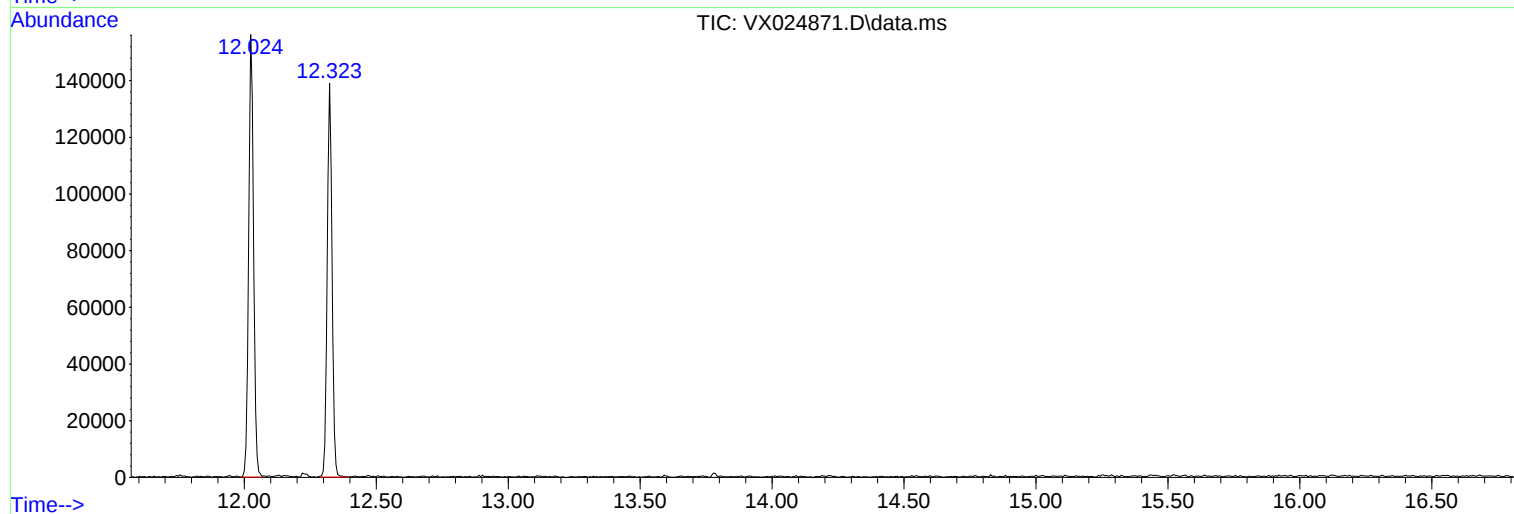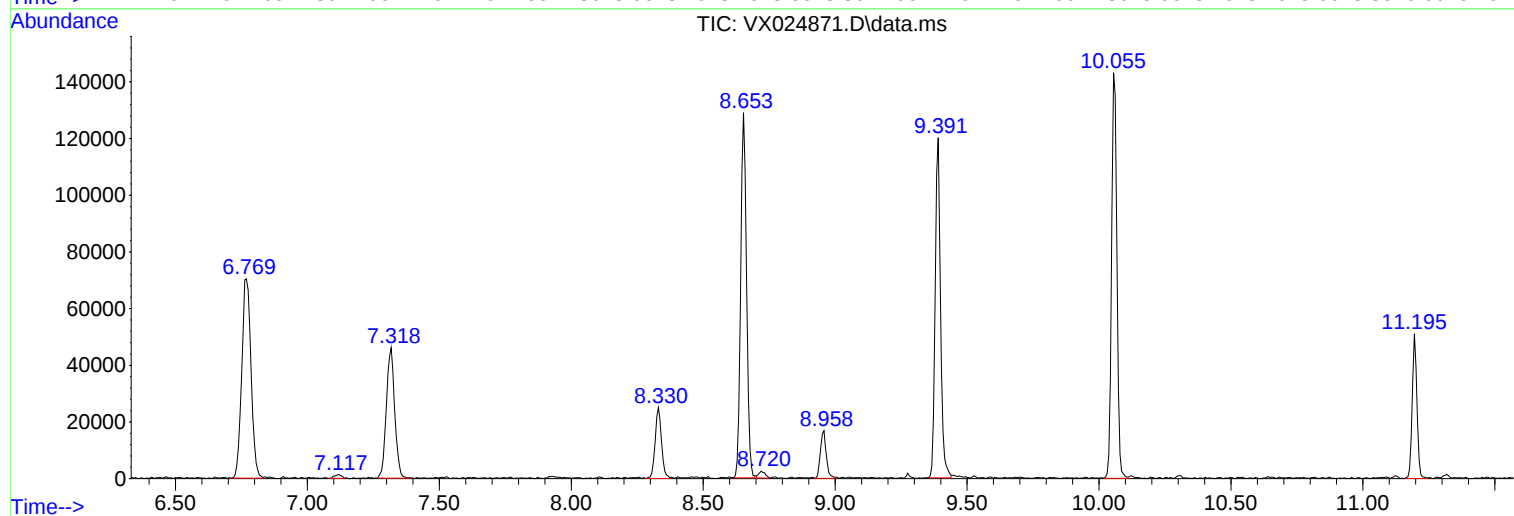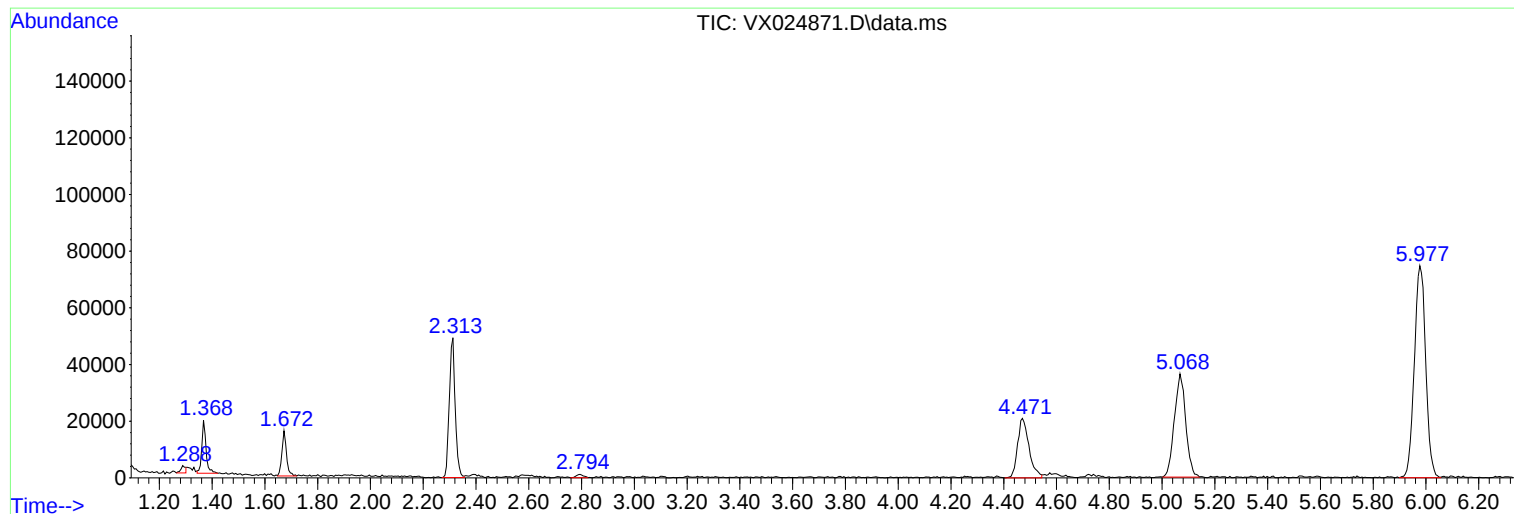

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX102221\
Data File : VX024871.D
Acq On : 22 Oct 2021 15:02
Operator : JC/MD
Sample : M4291-04
Misc : 25.0mL/MSVOA_X/WATER
ALS Vial : 14 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
P001-TW001-06

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXTR102221WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX102221\
Data File : VX024871.D
Acq On : 22 Oct 2021 15:02
Operator : JC/MD
Sample : M4291-04
Misc : 25.0mL/MSVOA_X/WATER
ALS Vial : 14 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
P001-TW001-06

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXTR102221WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc
