

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX102221\
 Data File : VX024875.D
 Acq On : 22 Oct 2021 16:36
 Operator : JC/MD
 Sample : M4291-06
 Misc : 25.0mL/MSVOA_X/WATER
 ALS Vial : 18 Sample Multiplier: 1

Instrument :
 MSVOA_X
 ClientSampleId :
 P002-TW001-03

Integration Parameters: rteint.p

Integrator: RTE

Smoothing : ON

Filtering: 5

Sampling : 1

Min Area: 3 % of largest Peak

Start Thrs: 0.1

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXTR102221WMA.M

Title : TRACE VOA SFAM1.0

Signal : TIC: VX024875.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.368	43	46	51	rBV	18166	18978	7.66%	0.931%
2	1.672	92	96	102	rBV	16172	19799	7.99%	0.971%
3	2.312	195	201	215	rVB	52352	82700	33.37%	4.055%
4	2.794	274	280	285	rVB4	1161	2669	1.08%	0.131%
5	4.483	547	557	569	rBV3	20238	69358	27.99%	3.401%
6	4.739	592	599	609	rVB3	1049	3317	1.34%	0.163%
7	5.068	642	653	663	rBV3	38595	122765	49.54%	6.020%
8	5.983	791	803	817	rBV5	84095	247824	100.00%	12.152%
9	6.769	922	932	943	rBV	75093	179267	72.34%	8.790%
10	7.123	984	990	994	rBV4	1489	3203	1.29%	0.157%
11	7.318	1012	1022	1031	rBV2	49418	110673	44.66%	5.427%
12	8.330	1179	1188	1196	rBV	28701	46739	18.86%	2.292%
13	8.653	1234	1241	1249	rBV	142665	220150	88.83%	10.795%
14	8.952	1286	1290	1297	rBV2	17667	27406	11.06%	1.344%
15	9.390	1356	1362	1374	rBV	131425	194382	78.44%	9.531%
16	10.055	1466	1471	1487	rVB	145254	208869	84.28%	10.242%
17	11.195	1653	1658	1664	rBV	54772	69877	28.20%	3.426%
18	12.024	1789	1794	1801	rBV	164526	208533	84.15%	10.225%
19	12.323	1836	1843	1850	rBV	155508	198968	80.29%	9.756%
20	16.371	2503	2507	2513	rVB4	2588	3918	1.58%	0.192%


Sum of corrected areas: 2039395

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX102221\
Data File : VX024875.D
Acq On : 22 Oct 2021 16:36
Operator : JC/MD
Sample : M4291-06
Misc : 25.0mL/MSVOA_X/WATER
ALS Vial : 18 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
P002-TW001-03

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXTR102221WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

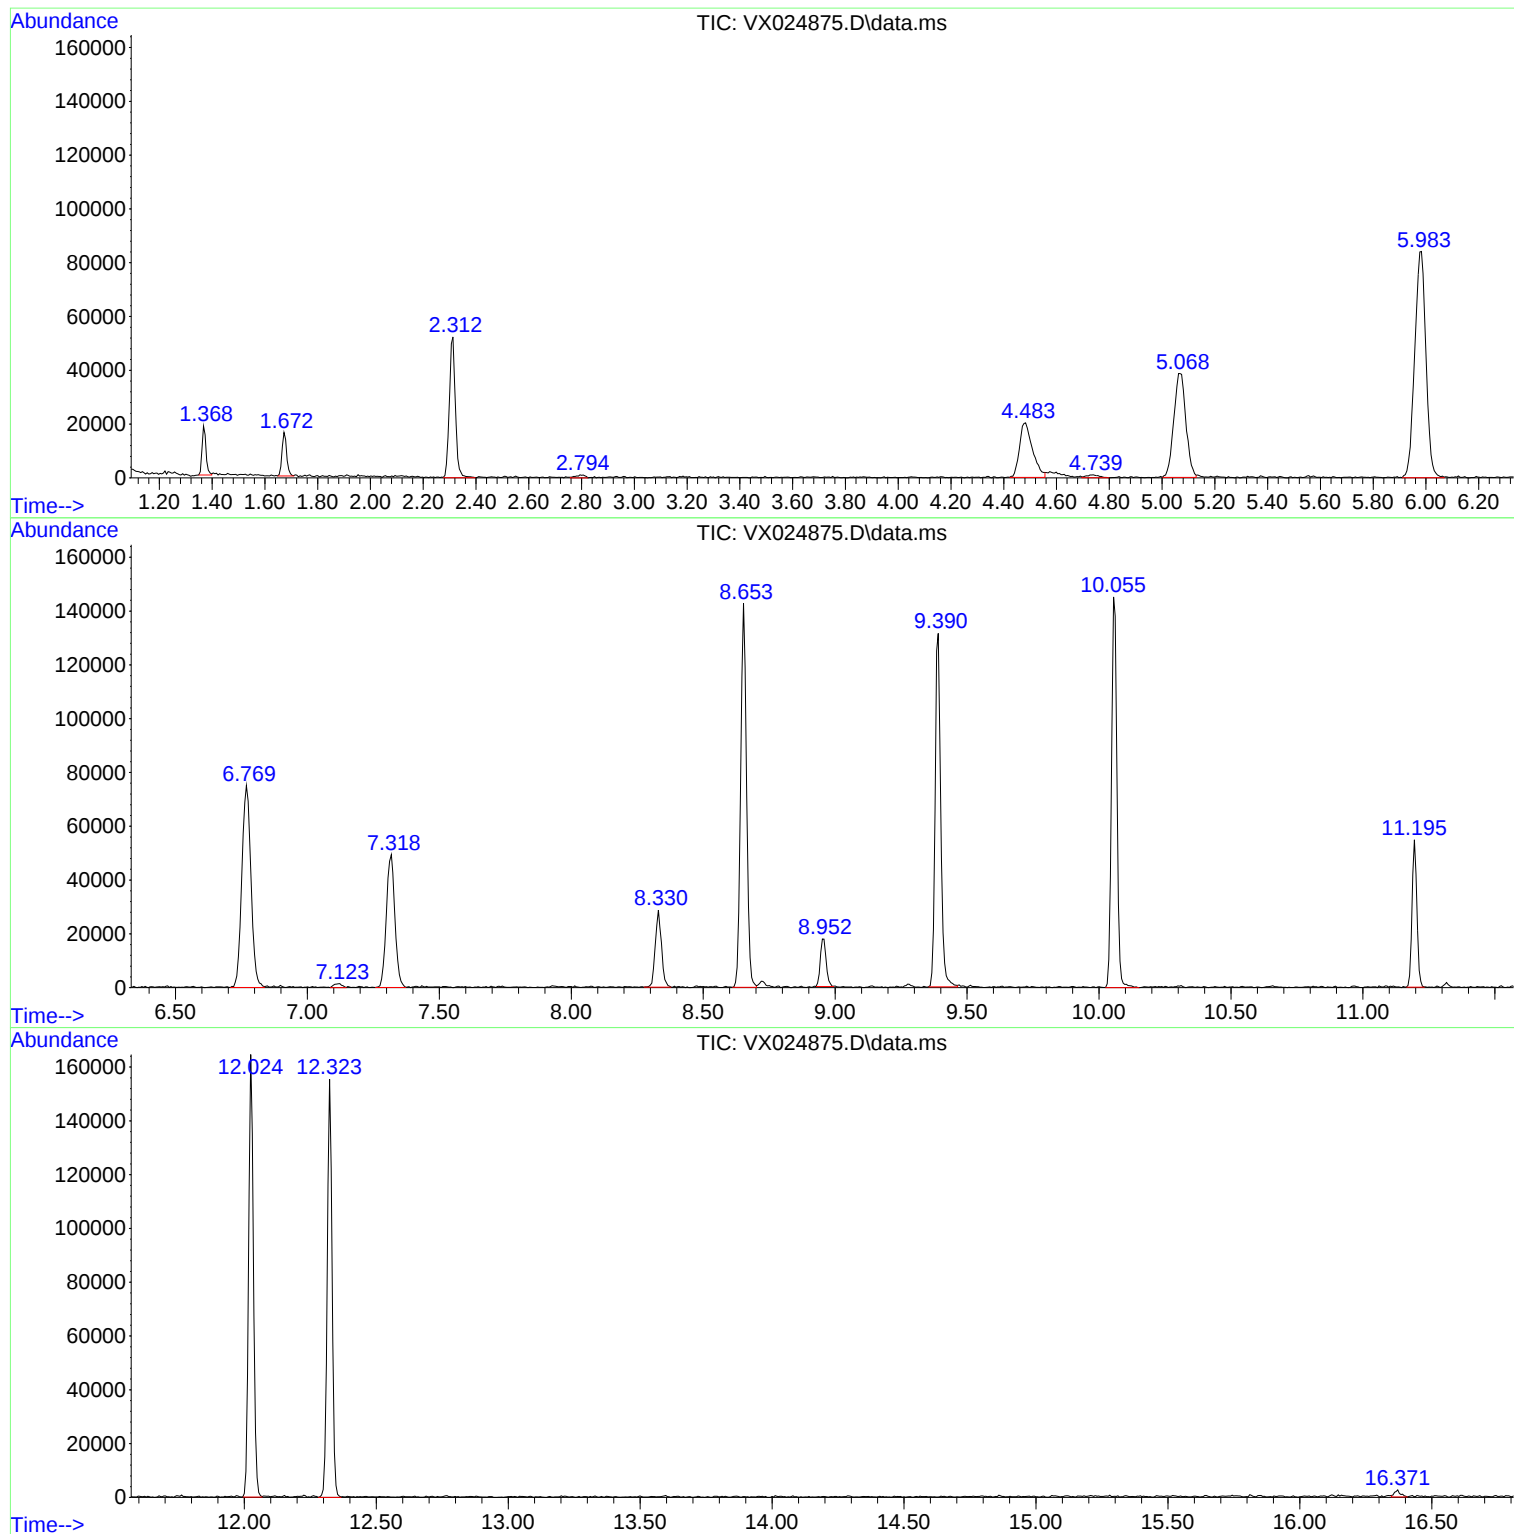

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX102221\
Data File : VX024875.D
Acq On : 22 Oct 2021 16:36
Operator : JC/MD
Sample : M4291-06
Misc : 25.0mL/MSVOA_X/WATER
ALS Vial : 18 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
P002-TW001-03

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXTR102221WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX102221\
Data File : VX024875.D
Acq On : 22 Oct 2021 16:36
Operator : JC/MD
Sample : M4291-06
Misc : 25.0mL/MSVOA_X/WATER
ALS Vial : 18 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
P002-TW001-03

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXTR102221WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc
