

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX102221\
 Data File : VX024876.D
 Acq On : 22 Oct 2021 17:00
 Operator : JC/MD
 Sample : M4291-07
 Misc : 25.0mL/MSVOA_X/WATER
 ALS Vial : 19 Sample Multiplier: 1

Instrument :
 MSVOA_X
 ClientSampleId :
 P007-TW001-02

Integration Parameters: rteint.p

Integrator: RTE

Smoothing : ON

Filtering: 5

Sampling : 1

Min Area: 3 % of largest Peak

Start Thrs: 0.1

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXTR102221WMA.M
 Title : TRACE VOA SFAM1.0

Signal : TIC: VX024876.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.368	43	46	52	rBV	19184	20253	8.37%	0.997%
2	1.672	91	96	104	rVB	17594	21037	8.69%	1.036%
3	2.313	194	201	211	rBV	50246	81897	33.84%	4.033%
4	4.483	545	557	569	rBV	19904	70374	29.08%	3.465%
5	4.727	586	597	607	rBV2	6801	21298	8.80%	1.049%
6	5.068	637	653	665	rBV3	39400	124258	51.35%	6.119%
7	5.977	791	802	815	rVB4	86391	241995	100.00%	11.916%
8	6.769	923	932	943	rBV2	74192	176066	72.76%	8.670%
9	7.312	1013	1021	1033	rBV	50027	111851	46.22%	5.508%
10	8.330	1181	1188	1199	rBV2	27626	45775	18.92%	2.254%
11	8.653	1234	1241	1248	rBV	133908	214209	88.52%	10.548%
12	8.720	1248	1252	1260	rVB4	2646	5126	2.12%	0.252%
13	8.952	1285	1290	1298	rBV2	18718	27598	11.40%	1.359%
14	9.391	1356	1362	1372	rBV	132012	190055	78.54%	9.359%
15	10.055	1465	1471	1480	rBV	147559	207237	85.64%	10.205%
16	11.195	1653	1658	1665	rVB	51486	68211	28.19%	3.359%
17	12.024	1789	1794	1802	rVB	165989	208490	86.15%	10.267%
18	12.323	1836	1843	1849	rBV	156849	191764	79.24%	9.443%
19	16.371	2500	2507	2511	rBV2	2139	3283	1.36%	0.162%




Sum of corrected areas: 2030777

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX102221\
Data File : VX024876.D
Acq On : 22 Oct 2021 17:00
Operator : JC/MD
Sample : M4291-07
Misc : 25.0mL/MSVOA_X/WATER
ALS Vial : 19 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
P007-TW001-02

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXTR102221WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

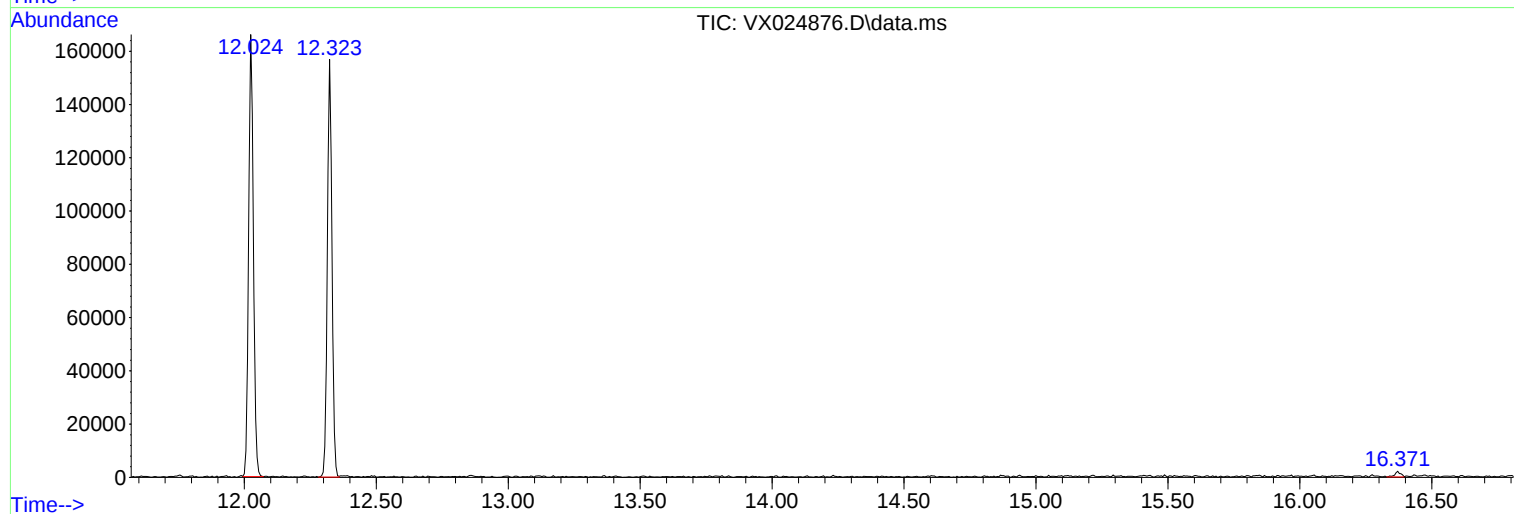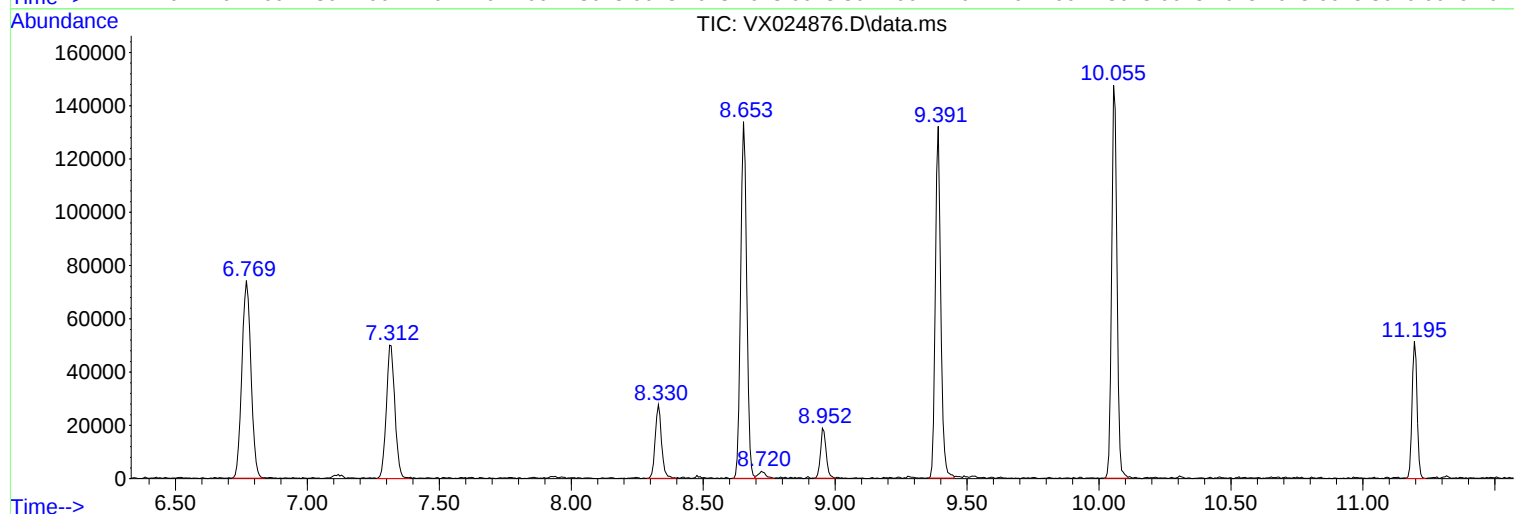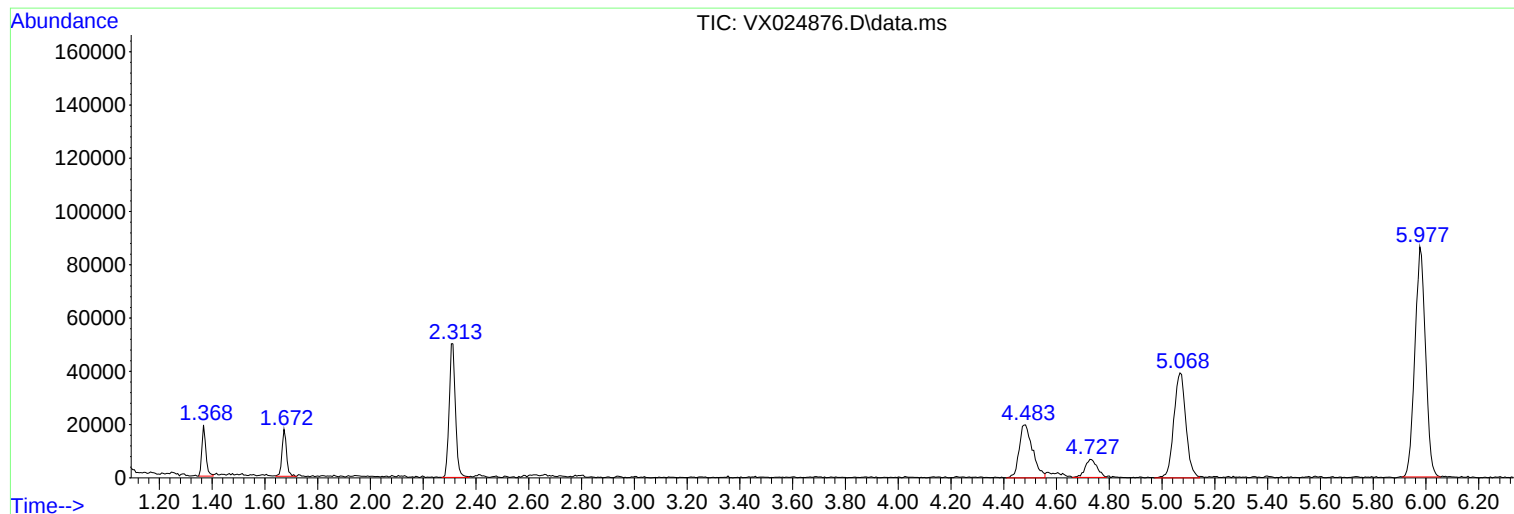

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX102221\
Data File : VX024876.D
Acq On : 22 Oct 2021 17:00
Operator : JC/MD
Sample : M4291-07
Misc : 25.0mL/MSVOA_X/WATER
ALS Vial : 19 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
P007-TW001-02









Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXTR102221WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

Peak Number 1 CH3C(O)CH2CH2OH Concentration Rank 2

R.T.	EstConc	Area	Relative to ISTD	R.T.
4.727	0.60 ug/L	21298	1,4-Difluorobenzene	6.769

Hit#	of	5	Tentative ID	MW	MolForm	CAS#	Qual
1			CH3C(O)CH2CH2OH	88	C4H8O2	000590-90-9	72
2			Ethyl Acetate	88	C4H8O2	000141-78-6	64
3			Ethyl Acetate	88	C4H8O2	000141-78-6	64
4			CH3C(O)CH2CH2OH	88	C4H8O2	000590-90-9	59
5			beta-Alanine amide	88	C3H8N2O	004726-85-6	28

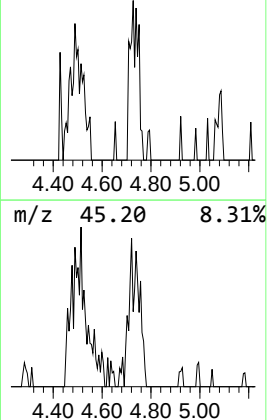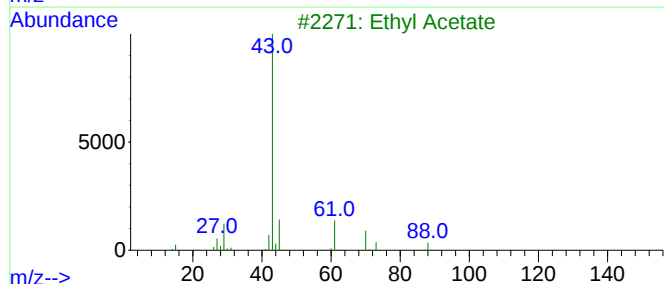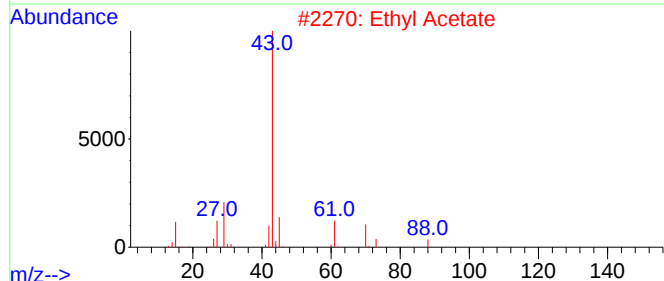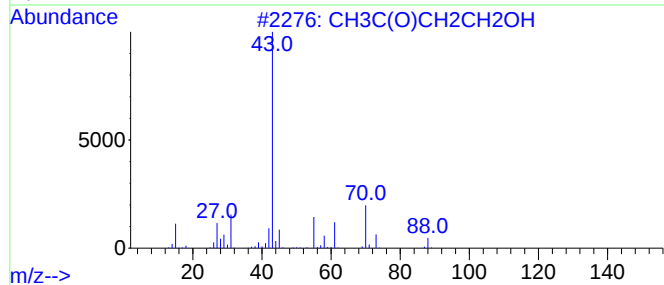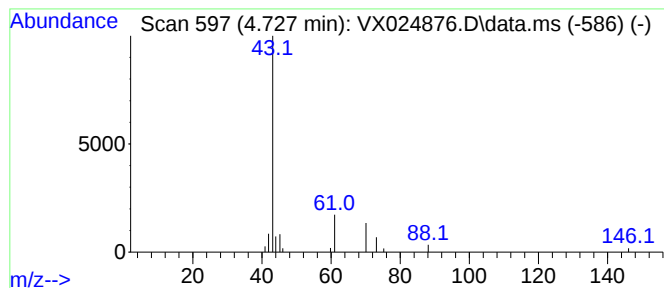

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX102221\
Data File : VX024876.D
Acq On : 22 Oct 2021 17:00
Operator : JC/MD
Sample : M4291-07
Misc : 25.0mL/MSVOA_X/WATER
ALS Vial : 19 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
P007-TW001-02

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXTR102221WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc
CH3C(O)CH2CH2OH	4.727	0.6	ug/L	21298	1	6.769	176066	5.0