


Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX102221\
 Data File : VX024859.D
 Acq On : 22 Oct 2021 09:02
 Operator : JC/MD
 Sample : BFB607
 Misc : 25.0mL/MSVOA_X/WATER
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_X
 ClientSampleId :
 BFB607

Integration File: rteint.p

Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXTR102221WMA.M
 Title : TRACE VOA SFAM1.0
 Last Update : Wed Oct 27 02:59:04 2021

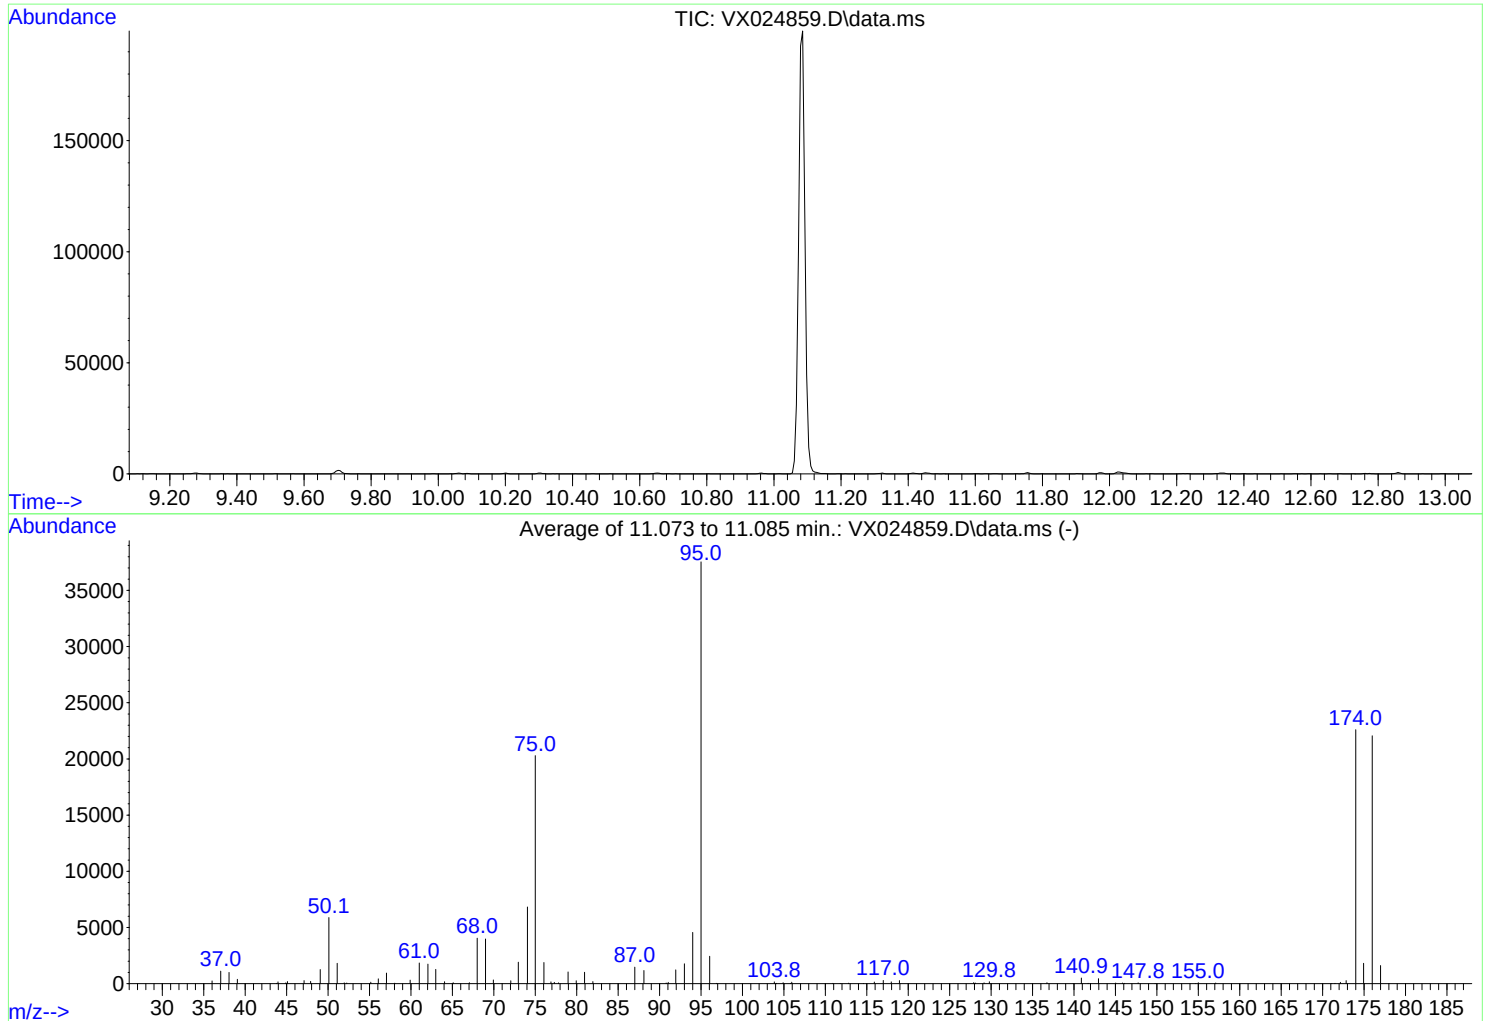

AutoFind: Scans 1638, 1639, 1640; Background Corrected with Scan 1632

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	15	40	15.7	5881	PASS
75	95	30	80	54.1	20293	PASS
95	95	100	100	100.0	37541	PASS
96	95	5	9	6.5	2439	PASS
173	174	0.00	2	1.2	274	PASS
174	95	50	120	60.2	22594	PASS
175	174	5	9	8.0	1808	PASS
176	174	95	105	97.7	22065	PASS
177	176	5	10	7.3	1612	PASS

Instrument :
MSVOA_X
ClientSampleId :
BFB607

m/z	Abundance
36.00	158.0
37.00	784.0
38.00	606.0
39.10	287.0
43.80	103.0
44.90	206.0
47.10	199.0
47.90	177.0
49.10	849.0
50.10	4115.0
51.10	1118.0
51.90	93.0
55.10	108.0
56.10	244.0
57.10	696.0
58.00	55.0
60.00	157.0
61.00	1269.0
62.00	1175.0
63.00	736.0
64.00	183.0
65.10	72.0
67.10	57.0
68.00	2756.0
69.00	2475.0
70.00	199.0
72.00	138.0
72.90	1303.0
74.10	4652.0
75.00	14063.0
76.10	1272.0
77.00	90.0
77.80	112.0
78.90	579.0
80.00	241.0
80.90	752.0
82.00	129.0
87.00	1172.0
88.20	649.0
91.10	93.0
92.00	900.0
93.00	1122.0
94.00	2982.0
95.00	24144.0
96.10	1507.0
96.90	66.0
104.10	74.0
104.90	75.0
105.80	89.0
114.60	53.0
115.90	86.0
117.00	328.0
119.00	183.0
127.90	78.0
129.20	58.0
129.80	132.0
141.00	216.0
142.90	254.0
146.10	65.0
154.70	60.0
172.80	224.0
174.00	11847.0
174.90	867.0
176.00	10467.0
177.00	1034.0

Instrument :
MSVOA_X
ClientSampleId :
BFB607

m/z	Abundance
36.00	281.0
37.10	1335.0
38.10	1254.0
39.00	515.0
44.00	295.0
45.10	325.0
47.10	295.0
47.90	238.0
49.00	1474.0
50.10	7325.0
51.10	2279.0
51.90	57.0
52.30	118.0
55.10	171.0
56.00	535.0
57.10	1037.0
59.90	509.0
61.00	2348.0
62.10	2012.0
63.00	1479.0
64.10	209.0
65.10	167.0
67.10	136.0
68.00	4631.0
69.00	4761.0
70.00	510.0
71.00	53.0
72.00	278.0
73.00	2154.0
74.00	7805.0
75.00	23256.0
76.00	2397.0
76.90	144.0
77.30	131.0
77.80	122.0
79.00	1170.0
80.00	300.0
80.90	1086.0
81.90	257.0
87.00	1809.0
88.10	1360.0
90.80	180.0
91.90	1520.0
93.00	2029.0
94.00	5257.0
95.00	44672.0
96.00	2846.0
103.80	306.0
104.90	91.0
106.00	154.0
111.80	51.0
112.80	66.0
115.80	112.0
117.10	236.0
117.90	216.0
118.90	324.0
128.10	163.0
129.20	62.0
129.90	205.0
136.80	105.0
140.90	649.0
141.70	102.0
143.00	510.0
145.10	123.0
145.80	88.0
147.70	91.0
149.80	57.0
155.00	109.0
157.10	67.0
171.10	51.0
171.50	69.0
172.10	169.0
172.90	361.0
174.00	24888.0
175.00	2182.0
176.00	25960.0
177.00	1854.0
178.00	52.0

Instrument :
MSVOA_X
ClientSampleId :
BFB607

m/z	Abundance
36.00	302.0
37.10	1218.0
38.10	1120.0
39.10	371.0
43.90	169.0
45.10	252.0
47.10	343.0
47.90	191.0
49.10	1430.0
50.10	6202.0
51.10	2041.0
52.00	68.0
52.20	71.0
55.20	117.0
56.00	492.0
57.00	1100.0
58.10	92.0
59.90	291.0
61.00	1903.0
62.00	2015.0
63.00	1588.0
64.00	124.0
67.00	82.0
68.00	4746.0
69.00	4671.0
69.90	269.0
72.10	342.0
73.00	2260.0
74.00	8013.0
75.00	23560.0
76.00	1967.0
76.80	231.0
77.30	229.0
79.00	1385.0
79.90	237.0
81.00	1190.0
82.00	187.0
87.00	1444.0
88.00	1487.0
91.00	231.0
92.00	1245.0
93.00	2166.0
94.00	5430.0
95.00	43808.0
96.10	2963.0
103.90	188.0
104.90	87.0
105.90	218.0
110.90	66.0
112.80	58.0
115.90	248.0
116.90	304.0
118.00	239.0
118.90	306.0
127.90	172.0
129.10	93.0
129.70	173.0
136.70	150.0
139.90	54.0
140.90	617.0
142.00	59.0
142.90	546.0
145.00	53.0
145.90	97.0
147.80	123.0
155.00	166.0
157.10	117.0
172.20	184.0
172.90	237.0
174.00	31048.0
175.00	2374.0
176.00	29768.0
177.00	1949.0

Instrument :
MSVOA_X
ClientSampleId :
BFB607