
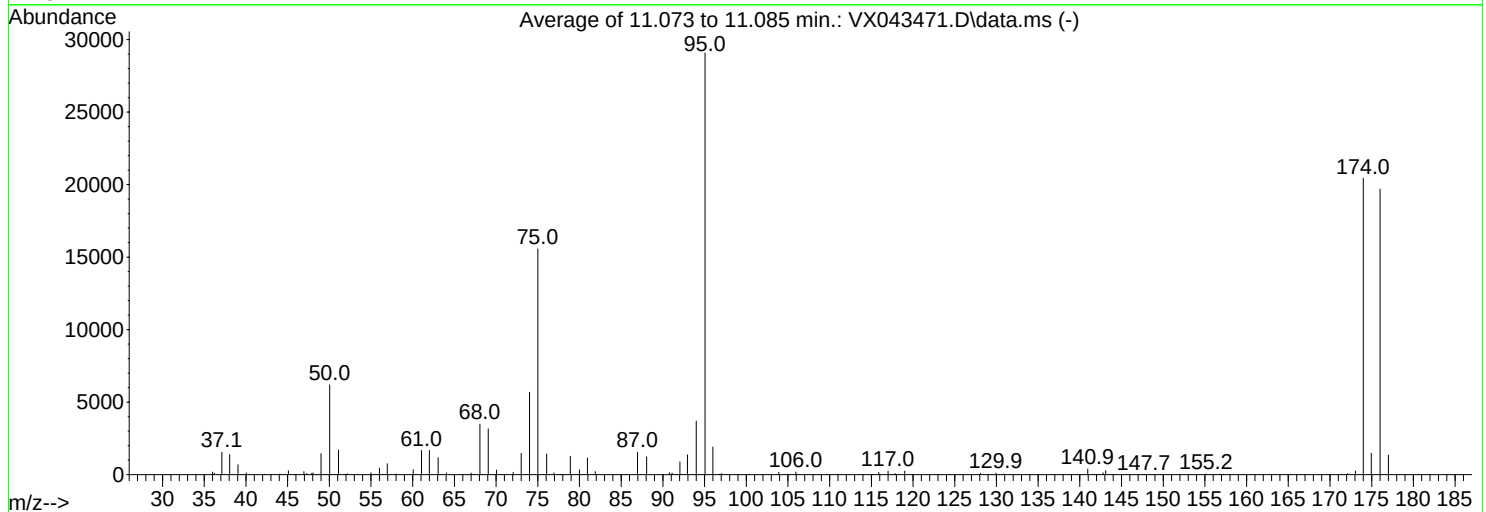


Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX102224\
Data File : VX043471.D
Acq On : 22 Oct 2024 08:13
Operator : JC/MD
Sample : BFB690
Misc : 5.0mL/MSVOA_X/WATER
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
BFB690

Integration File: LSCINT.P

Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXLM102224WMA.M
Title : VOC Analysis
Last Update : Wed Oct 23 02:04:35 2024

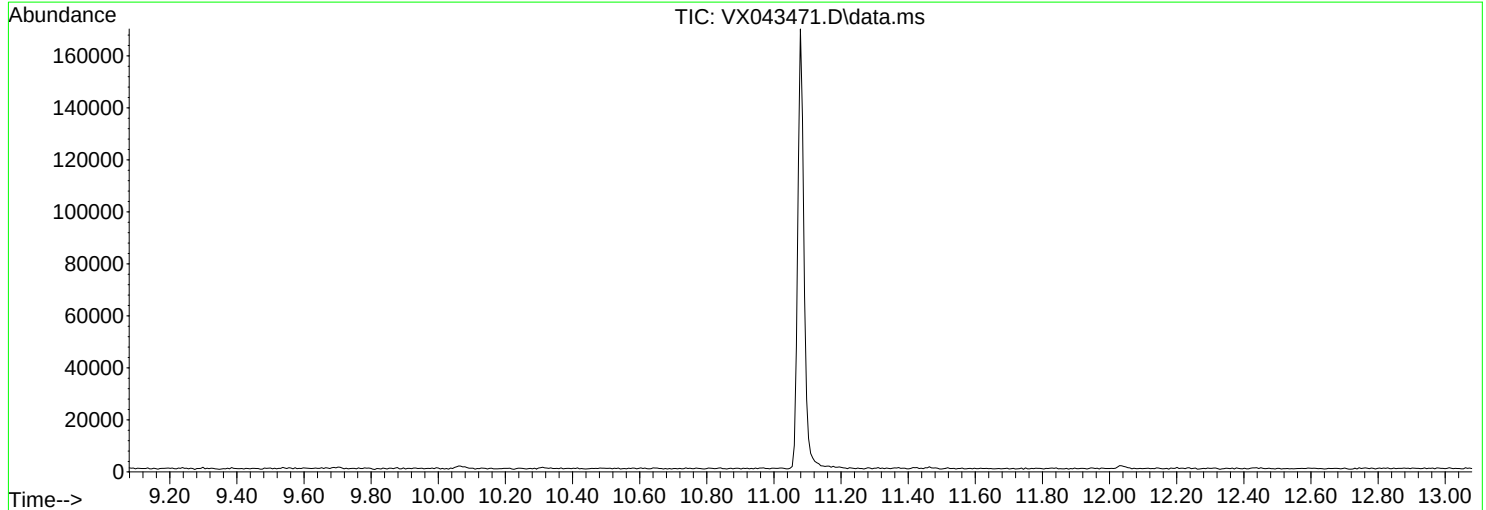

AutoFind: Scans 1638, 1639, 1640; Background Corrected with Scan 1633

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	15	40	21.3	6187	PASS
75	95	30	80	53.5	15564	PASS
95	95	100	100	100.0	29088	PASS
96	95	5	9	6.6	1912	PASS
173	174	0.00	2	1.3	258	PASS
174	95	50	120	70.2	20432	PASS
175	174	5	9	7.2	1474	PASS
176	174	95	101	96.4	19698	PASS
177	176	5	9	6.8	1346	PASS

m/z	Abundance
40.10	628.0
44.00	566.0

Instrument :
MSVOA_X
ClientSampleId :
BFB690

m/z	Abundance
36.00	252.0
37.10	1703.0
38.00	1363.0
39.10	714.0
40.00	783.0
44.10	633.0
45.20	244.0
46.90	273.0
47.90	272.0
49.00	1265.0
50.00	6191.0
51.10	1534.0
52.10	88.0
55.00	85.0
56.00	442.0
57.00	511.0
60.10	310.0
61.00	1604.0
62.00	1391.0
63.10	1199.0
64.00	103.0
67.00	110.0
68.10	2933.0
69.10	3067.0
70.00	188.0
72.00	125.0
73.00	1254.0
74.00	5116.0
75.00	13456.0
76.00	1208.0
77.00	119.0
77.80	80.0
78.90	1168.0
80.00	293.0
81.00	1144.0
82.00	164.0
87.00	838.0
88.10	1003.0
91.10	333.0
92.00	789.0
92.90	1158.0
94.00	3012.0
95.10	25208.0
96.00	1701.0
97.10	82.0
103.90	163.0
106.00	108.0
109.70	61.0
116.00	166.0
116.90	140.0
119.00	166.0
128.10	107.0
129.90	106.0
141.00	215.0
142.80	371.0
172.10	62.0
173.10	222.0
174.00	15247.0
174.90	1257.0
176.00	14910.0
177.00	921.0

Instrument :
MSVOA_X
ClientSampleId :
BFB690

m/z	Abundance
36.20	345.0
37.10	1824.0
38.10	1783.0
39.10	818.0
40.10	611.0
42.20	75.0
44.10	509.0
45.00	362.0
45.80	74.0
47.30	228.0
48.10	205.0
49.00	1980.0
50.00	7137.0
51.10	2035.0
52.20	128.0
55.00	195.0
56.10	560.0
56.90	816.0
58.00	68.0
59.90	294.0
61.00	1960.0
62.00	2012.0
63.00	1500.0
64.10	155.0
67.00	166.0
68.00	4489.0
69.10	3836.0
70.10	425.0
72.10	206.0
73.00	1891.0
74.00	6351.0
75.00	18224.0
76.10	1710.0
76.90	144.0
78.90	1585.0
80.00	438.0
80.90	1218.0
81.90	252.0
86.90	1349.0
87.00	1348.0
88.00	1532.0
90.80	259.0
92.10	1137.0
93.00	1753.0
94.00	4733.0
95.10	35088.0
96.00	2422.0
97.00	144.0
103.90	222.0
105.00	68.0
106.00	205.0
115.90	151.0
117.00	341.0
117.90	132.0
119.00	331.0
128.00	140.0
129.90	144.0
130.90	67.0
140.90	460.0
141.70	64.0
143.10	394.0
155.20	79.0
156.90	52.0
172.10	87.0
173.10	273.0
174.00	24456.0
175.00	1685.0
176.00	22896.0
177.00	1688.0

Instrument :
MSVOA_X
ClientSampleId :
BFB690

m/z	Abundance
36.00	288.0
37.00	1096.0
38.10	1034.0
39.00	516.0
40.00	859.0
44.10	704.0
45.00	194.0
47.00	344.0
48.00	173.0
49.00	1124.0
50.10	5232.0
51.10	1520.0
51.90	91.0
55.00	116.0
55.90	346.0
57.00	920.0
58.00	92.0
60.10	431.0
61.10	1419.0
62.00	1604.0
63.00	813.0
64.00	100.0
67.00	62.0
68.00	3032.0
69.00	2551.0
70.10	362.0
72.10	120.0
73.00	1273.0
74.00	5539.0
75.00	15011.0
76.00	1356.0
77.00	118.0
78.90	1017.0
80.00	254.0
80.90	1095.0
81.80	199.0
87.00	1092.0
88.10	1143.0
90.80	140.0
92.00	721.0
93.00	1180.0
94.00	3330.0
95.00	26968.0
96.00	1614.0
96.80	104.0
104.00	114.0
105.00	68.0
105.90	212.0
111.00	58.0
115.10	62.0
115.80	160.0
117.10	253.0
117.80	100.0
119.00	227.0
128.20	54.0
130.00	88.0
130.90	68.0
141.00	471.0
143.10	430.0
147.70	67.0
155.10	92.0
156.80	59.0
157.20	61.0
172.10	84.0
173.00	278.0
174.00	21592.0
175.00	1480.0
176.00	21288.0
177.00	1428.0

Instrument :
MSVOA_X
ClientSampleId :
BFB690