

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX102225\
 Data File : VX048304.D
 Acq On : 22 Oct 2025 17:13
 Operator : JC/MD
 Sample : Q3426-01 50X
 Misc : 5.0mL/MSVOA_X/WATER
 ALS Vial : 26 Sample Multiplier: 1

Instrument :
 MSVOA_X
 ClientSampleId :
 TWP2

Integration Parameters: RTEINT.P

Integrator: RTE

Smoothing : ON

Filtering: 5

Sampling : 1

Min Area: 3 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\82X102025W.M
 Title : SW846 8260

Signal : TIC: VX048304.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.459	59	61	70	rVB	9051	14037	1.91%	0.264%
2	1.971	140	145	155	rVB3	7347	20964	2.85%	0.394%
3	2.221	181	186	196	rVB	10801	18992	2.58%	0.357%
4	2.380	202	212	216	rBV	12282	26281	3.57%	0.493%
5	2.459	217	225	226	rBV2	7499	14972	2.04%	0.281%
6	4.294	517	526	540	rVB6	7213	21929	2.98%	0.412%
7	4.538	557	566	581	rBV4	2644	10373	1.41%	0.195%
8	5.184	660	672	681	rBV5	4930	16120	2.19%	0.303%
9	5.373	692	703	715	rBV2	78395	256353	34.85%	4.813%
10	5.538	721	730	748	rVB	127388	397310	54.02%	7.460%
11	5.940	785	796	805	rBV	90130	260397	35.40%	4.889%
12	6.025	805	810	824	rVB2	20663	61357	8.34%	1.152%
13	6.745	919	928	951	rBV	230133	608750	82.77%	11.430%
14	7.367	1021	1030	1040	rBV4	14209	35587	4.84%	0.668%
15	8.635	1231	1238	1246	rBV	451990	735498	100.00%	13.810%
16	8.702	1246	1249	1254	rVB2	8875	14159	1.93%	0.266%
17	8.946	1285	1289	1297	rVB6	3334	8463	1.15%	0.159%
18	10.037	1462	1468	1482	rVB	434284	606196	82.42%	11.382%
19	10.177	1486	1491	1497	rBV	28562	38420	5.22%	0.721%
20	10.287	1502	1509	1516	rBV	105982	153873	20.92%	2.889%
21	10.622	1560	1564	1572	rVB	18988	27007	3.67%	0.507%
22	11.061	1631	1636	1647	rBV	354044	480872	65.38%	9.029%
23	11.360	1681	1685	1687	rBV	17096	23161	3.15%	0.435%
24	11.433	1693	1697	1707	rVB	25744	37093	5.04%	0.696%
25	11.598	1717	1724	1731	rBV	18651	27395	3.72%	0.514%
26	11.732	1742	1746	1755	rVB	50567	66473	9.04%	1.248%
27	12.000	1785	1790	1797	rBV	521542	673684	91.60%	12.650%
28	12.067	1797	1801	1809	rVB	23285	34710	4.72%	0.652%
29	12.225	1820	1827	1834	rBV2	21207	35092	4.77%	0.659%
30	12.299	1834	1839	1845	rVB2	18377	28922	3.93%	0.543%
31	12.445	1859	1863	1870	rVB2	7044	11393	1.55%	0.214%
32	12.518	1870	1875	1876	rBV2	5922	8648	1.18%	0.162%
33	12.591	1884	1887	1891	rVB	9988	11094	1.51%	0.208%
34	12.677	1896	1901	1910	rBV4	10947	23166	3.15%	0.435%
35	12.799	1916	1921	1924	rBV4	6499	9269	1.26%	0.174%
36	12.902	1933	1938	1941	rBV2	8674	11801	1.60%	0.222%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX102225\
 Data File : VX048304.D
 Acq On : 22 Oct 2025 17:13
 Operator : JC/MD
 Sample : Q3426-01 50X
 Misc : 5.0mL/MSVOA_X/WATER
 ALS Vial : 26 Sample Multiplier: 1

Instrument :
 MSVOA_X
 ClientSampleId :
 TWP2

Integration Parameters: RTEINT.P

Integrator: RTE

Smoothing : ON

Filtering: 5

Sampling : 1

Min Area: 3 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\82X102025W.M
 Title : SW846 8260

37	12.945	1941	1945	1952	rVB2	14310	25732	3.50%	0.483%
38	13.024	1952	1958	1961	rBV5	8050	12365	1.68%	0.232%
39	13.146	1975	1978	1982	rVB3	8647	11264	1.53%	0.212%
40	13.237	1987	1993	1994	rBV5	5907	9330	1.27%	0.175%
41	13.274	1994	1999	2004	rVB2	36419	53231	7.24%	1.000%
42	13.365	2009	2014	2016	rVV3	8038	9807	1.33%	0.184%
43	13.402	2016	2020	2029	rVB5	18760	37486	5.10%	0.704%
44	13.481	2029	2033	2036	rBV6	6676	9385	1.28%	0.176%
45	13.524	2036	2040	2042	rBV	7942	9847	1.34%	0.185%
46	13.567	2042	2047	2052	rBV3	12529	21206	2.88%	0.398%
47	13.646	2057	2060	2064	rVB3	9130	12145	1.65%	0.228%
48	13.756	2075	2078	2080	rBV	9471	10936	1.49%	0.205%
49	13.829	2085	2090	2096	rVB7	15873	28160	3.83%	0.529%
50	13.902	2096	2102	2107	rBV5	11624	22487	3.06%	0.422%
51	14.054	2124	2127	2130	rBV4	11342	15001	2.04%	0.282%
52	14.207	2144	2152	2157	rVB5	22997	47320	6.43%	0.889%
53	14.298	2164	2167	2172	rBV6	6408	9657	1.31%	0.181%
54	14.353	2172	2176	2179	rVV2	11291	13795	1.88%	0.259%
55	14.457	2189	2193	2203	rVB7	16198	28369	3.86%	0.533%
56	14.591	2211	2215	2222	rBV4	24476	46713	6.35%	0.877%
57	14.652	2222	2225	2230	rVB3	10115	14055	1.91%	0.264%
58	14.707	2230	2234	2236	rBV5	5815	7742	1.05%	0.145%
59	14.823	2251	2253	2257	rVB5	8488	10574	1.44%	0.199%
60	15.158	2303	2308	2311	rBV3	12752	19800	2.69%	0.372%
61	15.664	2388	2391	2398	rBV7	5499	9534	1.30%	0.179%


Sum of corrected areas: 5325752

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX102225\
Data File : VX048304.D
Acq On : 22 Oct 2025 17:13
Operator : JC/MD
Sample : Q3426-01 50X
Misc : 5.0mL/MSVOA_X/WATER
ALS Vial : 26 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
TWP2

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\82X102025W.M
Quant Title : SW846 8260

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

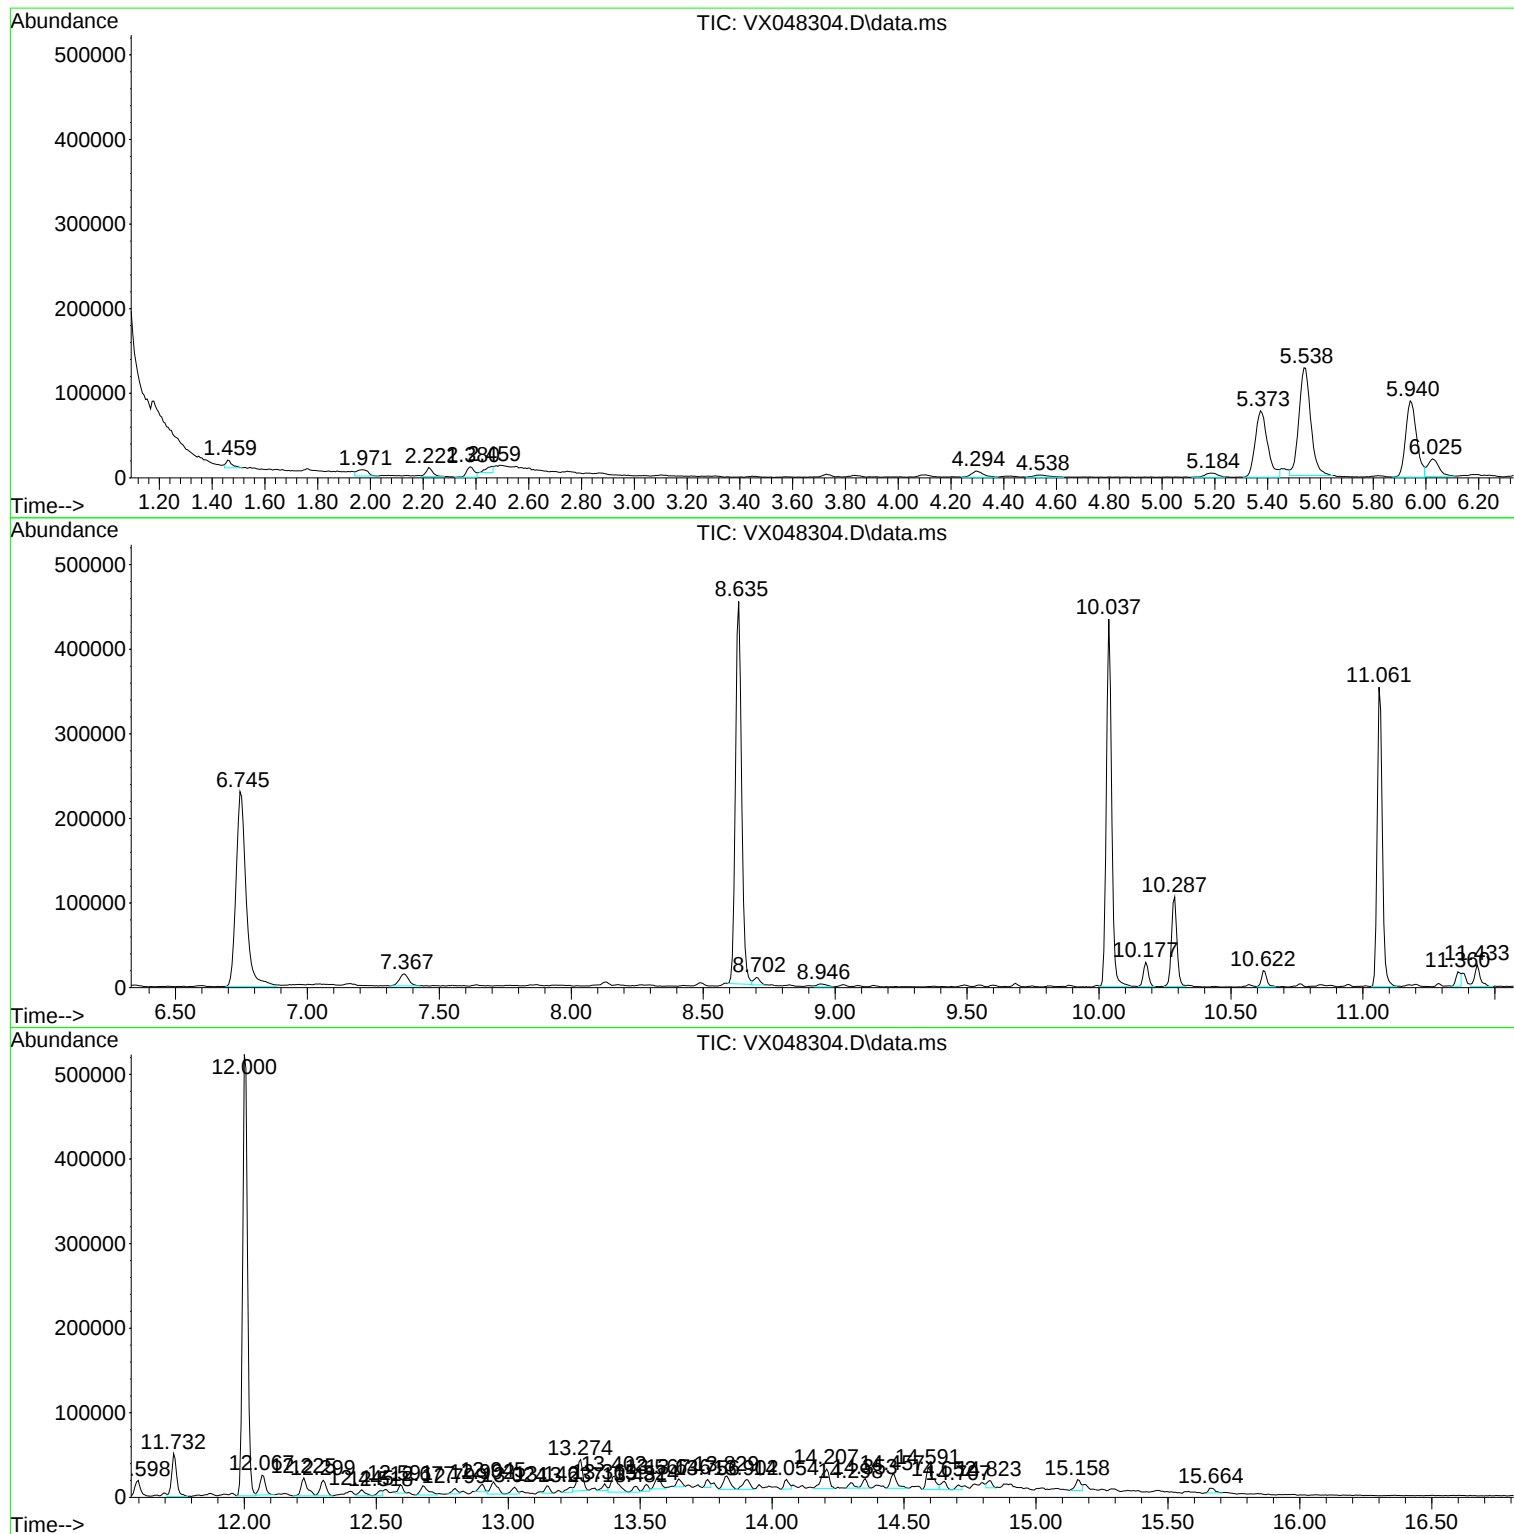

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX102225\
Data File : VX048304.D
Acq On : 22 Oct 2025 17:13
Operator : JC/MD
Sample : Q3426-01 50X
Misc : 5.0mL/MSVOA_X/WATER
ALS Vial : 26 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
TWP2

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\82X102025W.M
Quant Title : SW846 8260

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX102225\
Data File : VX048304.D
Acq On : 22 Oct 2025 17:13
Operator : JC/MD
Sample : Q3426-01 50X
Misc : 5.0mL/MSVOA_X/WATER
ALS Vial : 26 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
TWP2

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\82X102025W.M
Quant Title : SW846 8260

TIC Library : C:\Database\NIST0.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	#	RT	Resp	Conc
------------------	----	---------	-------	----------	---	----	------	------