


Data Path : Z:\voasrv\HPCHEM1\MSVOA X\Data\VX102320\
 Data File : VX019067.D
 Acq On : 23 Oct 2020 09:20
 Operator : JC/SP
 Sample : BFB
 Misc : 5.0mL/MSVOA X/WATER
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_X
 ClientSampleId :
 BFB

Integration File: RTEINT3.P

Method : Z:\VOASRV\HPCHEM1\MSVOA_X\METHOD\624X102320W.M
 Title : METHOD 624 VOLATILE ORGANIC ANALYSIS
 Last Update : Mon Oct 26 11:58:08 2020

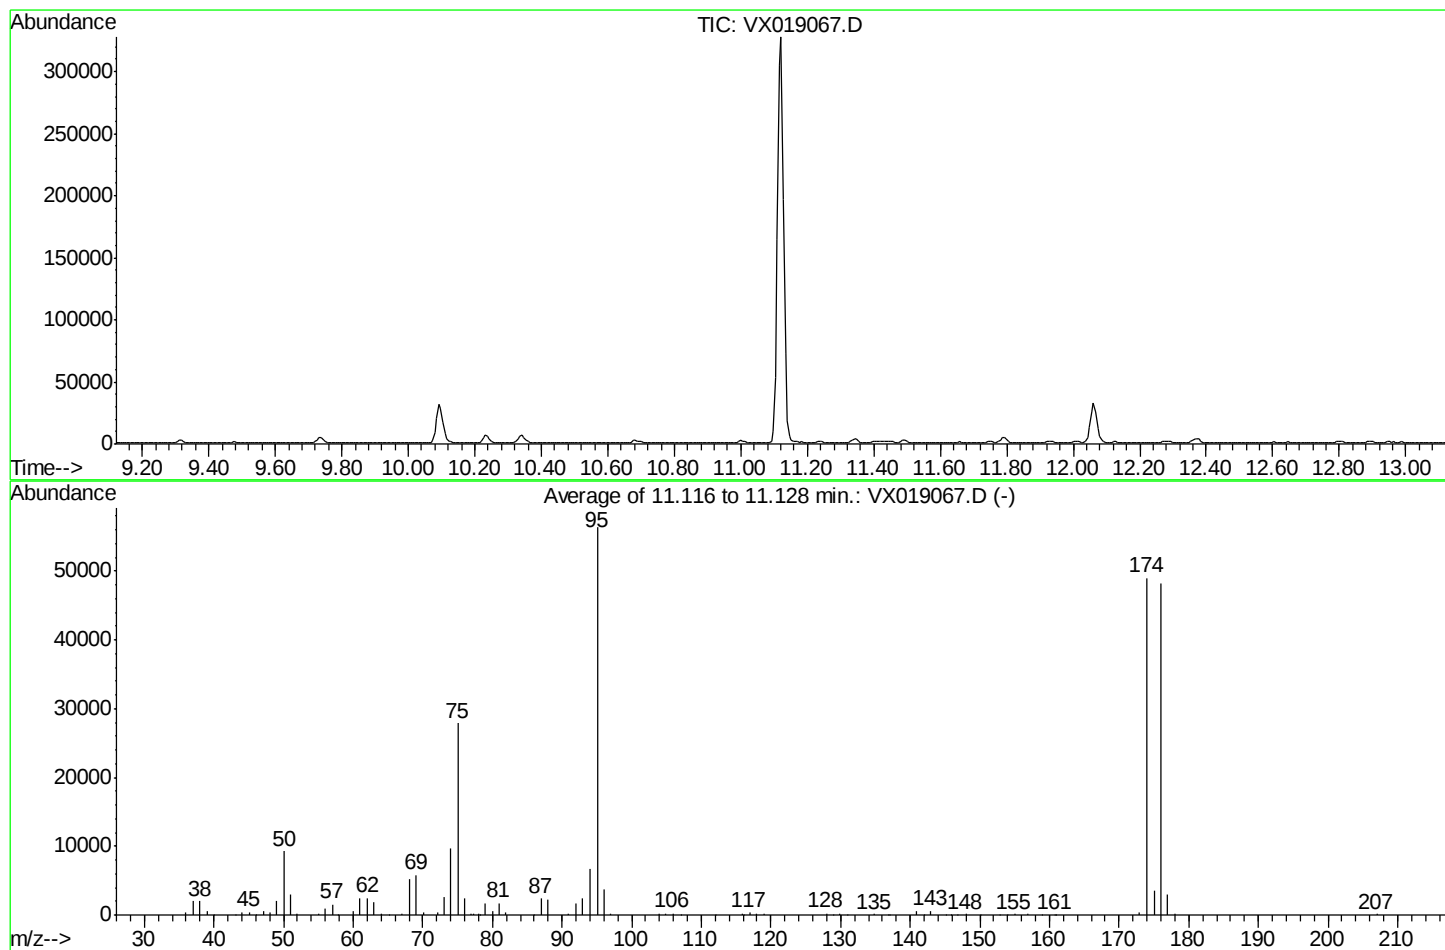

AutoFind: Scans 1645, 1646, 1647; Background Corrected with Scan 1639

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	15	40	16.4	9222	PASS
75	95	30	60	49.5	27888	PASS
95	95	100	100	100.0	56384	PASS
96	95	5	9	6.5	3663	PASS
173	174	0.00	2	0.9	418	PASS
174	95	50	100	86.9	49010	PASS
175	174	5	9	7.1	3493	PASS
176	174	95	101	98.5	48274	PASS
177	176	5	9	6.3	3047	PASS