


Data Path : Z:\VOASRV\HPCHEM1\MSVOA X\DATA\VX102320\
Data File : VX019091.D
Acq On : 23 Oct 2020 21:22
Operator : JC/SP
Sample : BFB
Misc : 5.0mL/MSVOA X/WATER
ALS Vial : 27 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
BFB

Integration File: RTEINT.P

Method : Z:\VOASRV\HPCHEM1\MSVOA_X\METHOD\82X102120W.M
Title : SW846 8260
Last Update : Thu Oct 22 17:51:42 2020

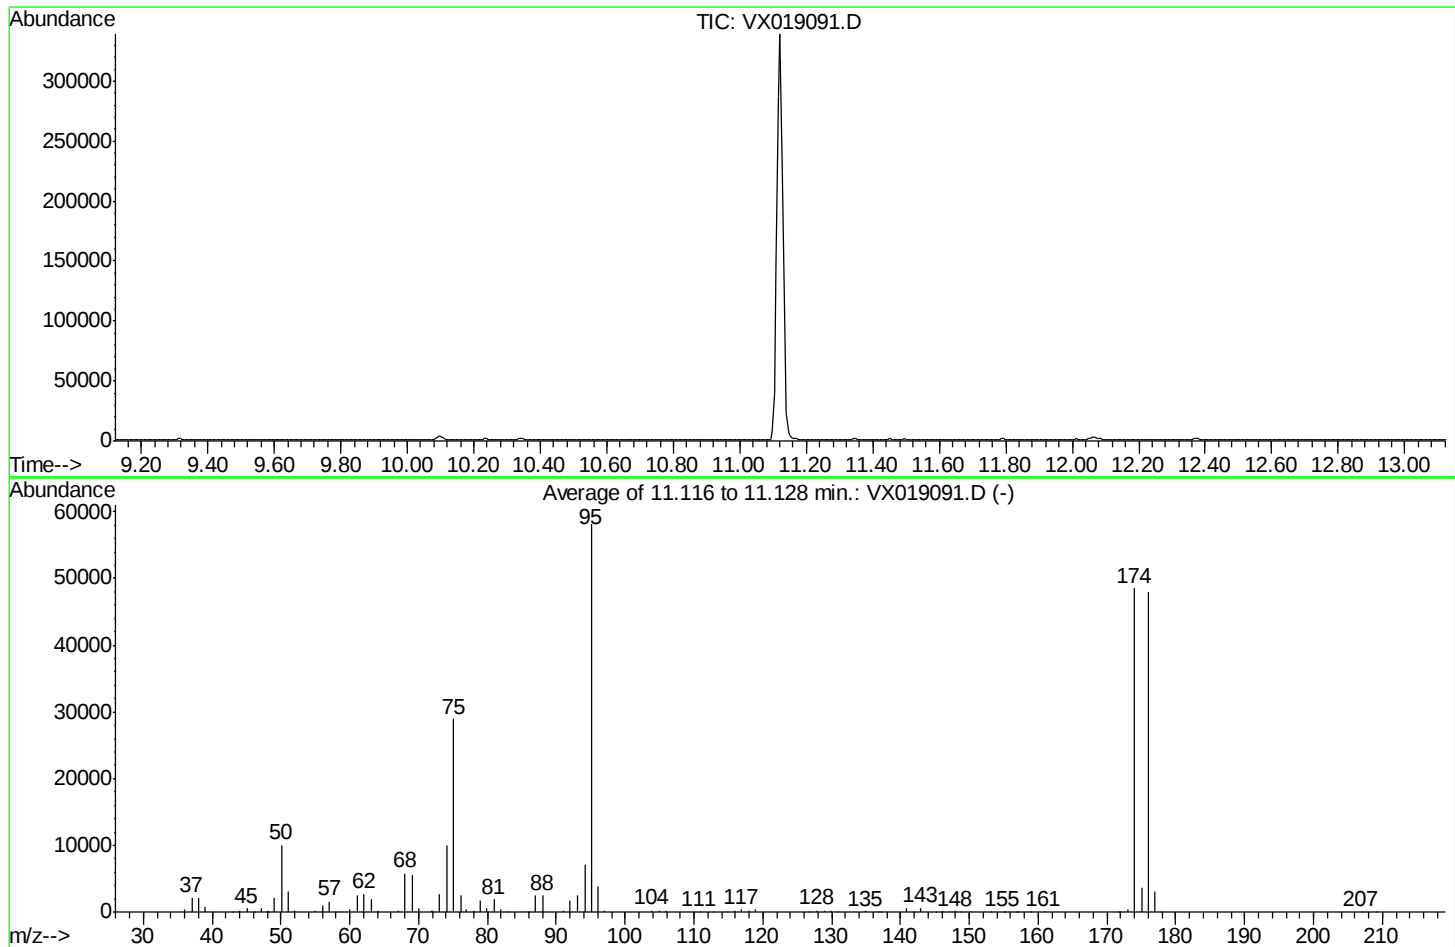

AutoFind: Scans 1645, 1646, 1647; Background Corrected with Scan 1638

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	15	40	17.2	10009	PASS
75	95	30	60	49.8	28930	PASS
95	95	100	100	100.0	58122	PASS
96	95	5	9	6.7	3912	PASS
173	174	0.00	2	0.9	441	PASS
174	95	50	100	83.5	48533	PASS
175	174	5	9	7.4	3605	PASS
176	174	95	101	98.7	47912	PASS
177	176	5	9	6.6	3148	PASS