

Quantitation Report (QT Reviewed)


Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX102321\
 Data File : VX024897.D
 Acq On : 23 Oct 2021 15:49
 Operator : JC/MD
 Sample : M4303-03
 Misc : 25.0mL/MSVOA_X/WATER
 ALS Vial : 12 Sample Multiplier: 1

Instrument :
 MSVOA_X
 Client Sampled :
 P005-TW001-02

Quant Time: Oct 25 02:34:01 2021
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXTR102221WMA.M
 Quant Title : TRACE VOA SFAM1.0
 QLast Update : Mon Oct 25 02:31:08 2021
 Response via : Initial Calibration

Manual Integrations
 APPROVED

MMDadoda
 10/25/2021 10:25:47 AM

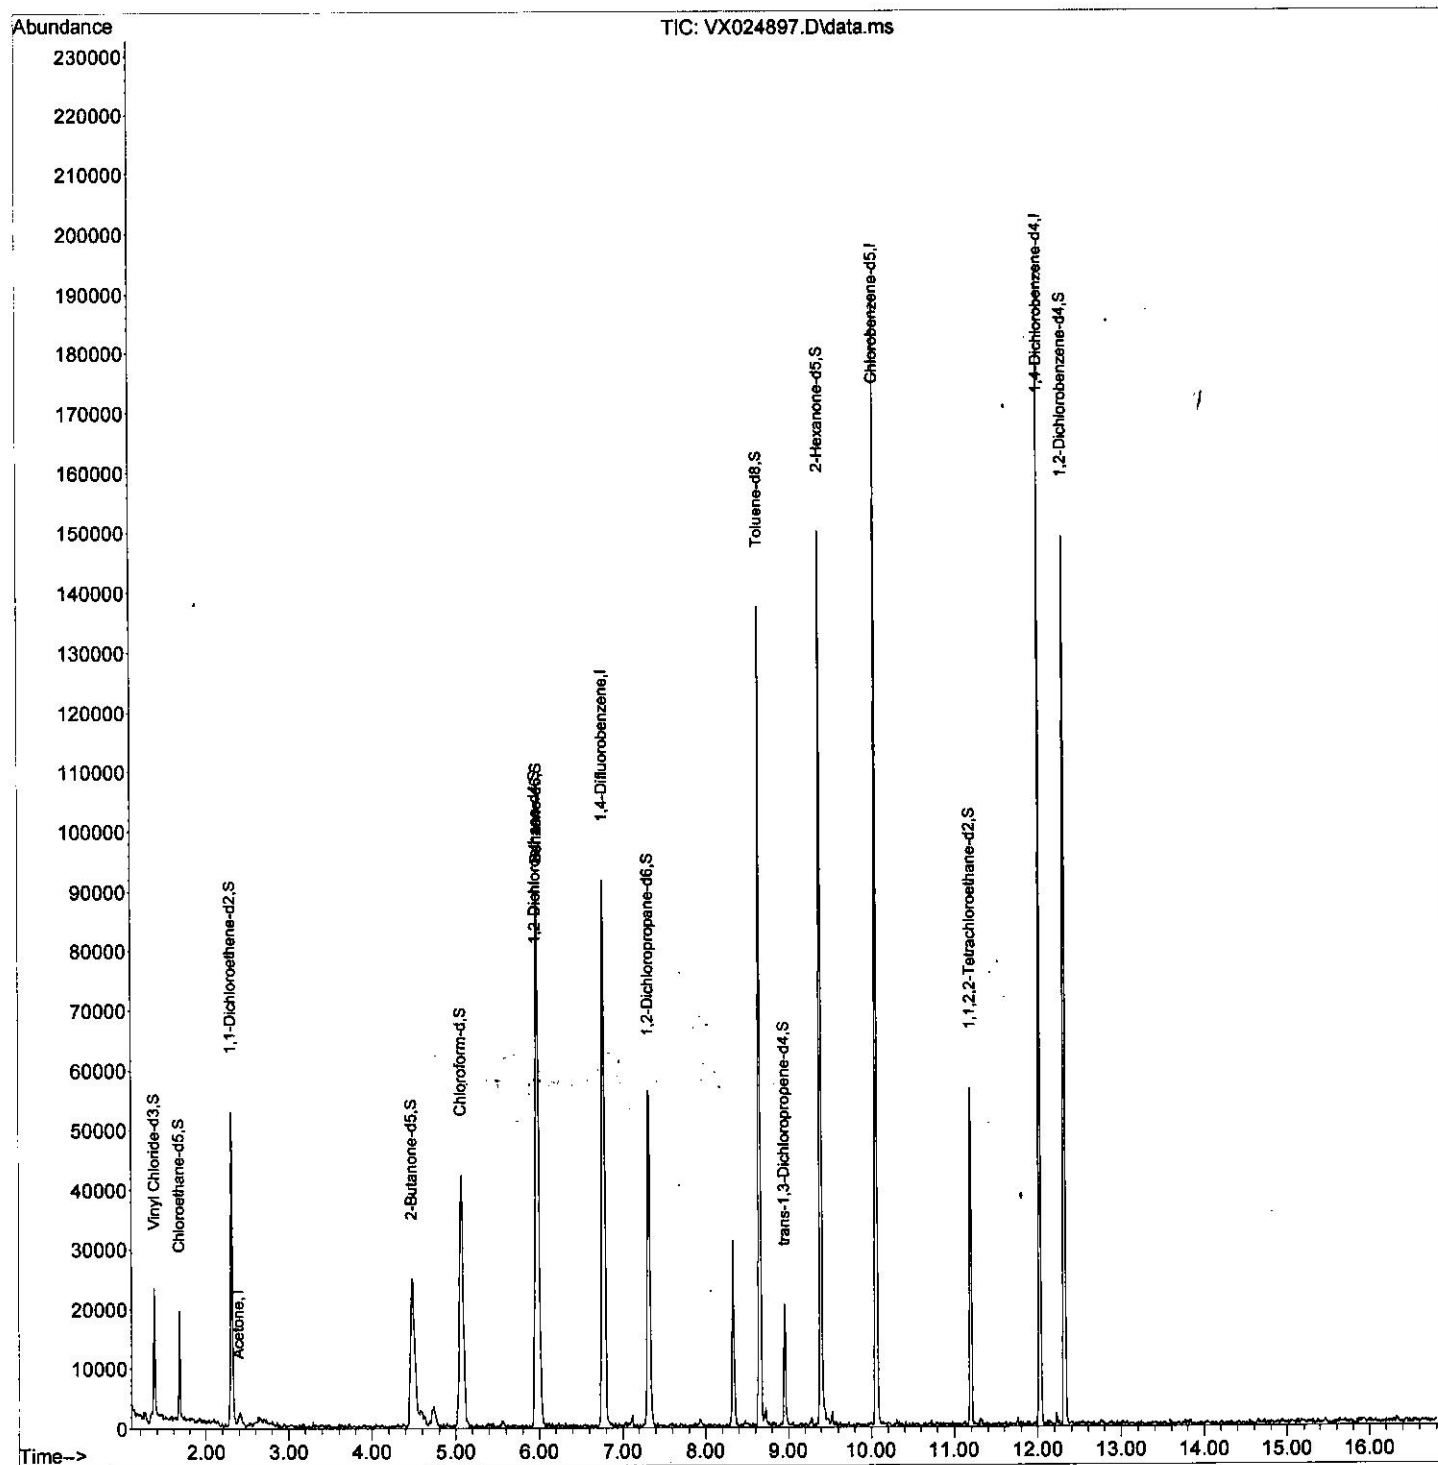

Quantitation Report (Qedit)




Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX102321\
 Data File : VX024897.D
 Acq On : 23 Oct 2021 15:49
 Operator : JC/MD
 Sample : M4303-03
 Misc : 25.0mL/MSVOA_X/WATER
 ALS Vial : 12 Sample Multiplier: 1

Instrument :
 MSVOA_X
 ClientSampleId :
 P005-TW001-02

Quant Time: Oct 25 02:34:01 2021
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXTR102221WMA.M
 Quant Title : TRACE VOA SFAM1.0
 QLast Update : Mon Oct 25 02:31:08 2021
 Response via : Initial Calibration

Manual Integrations
 APPROVED

MMDadoda
 10/25/2021 10:25:47 AM

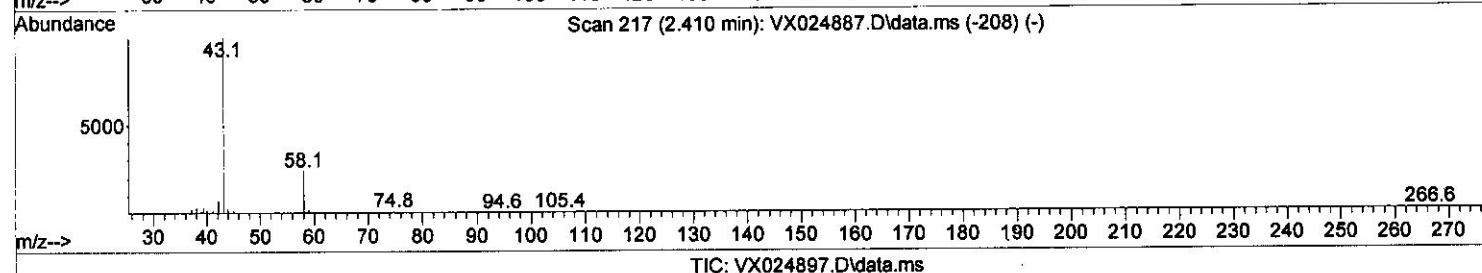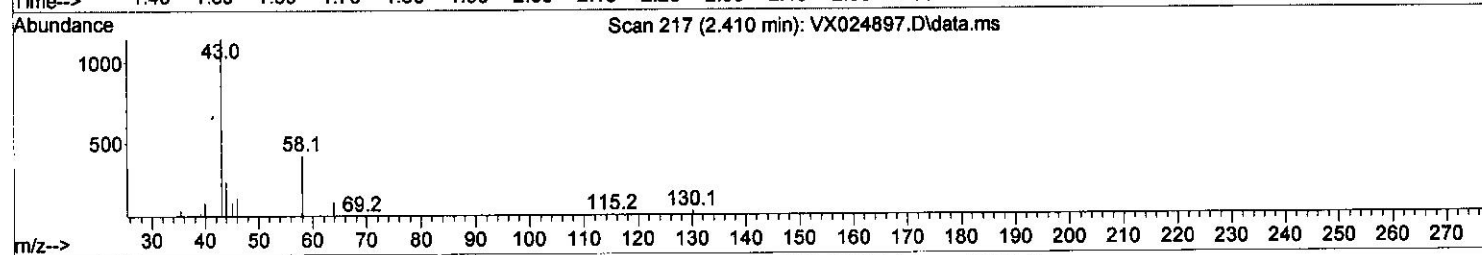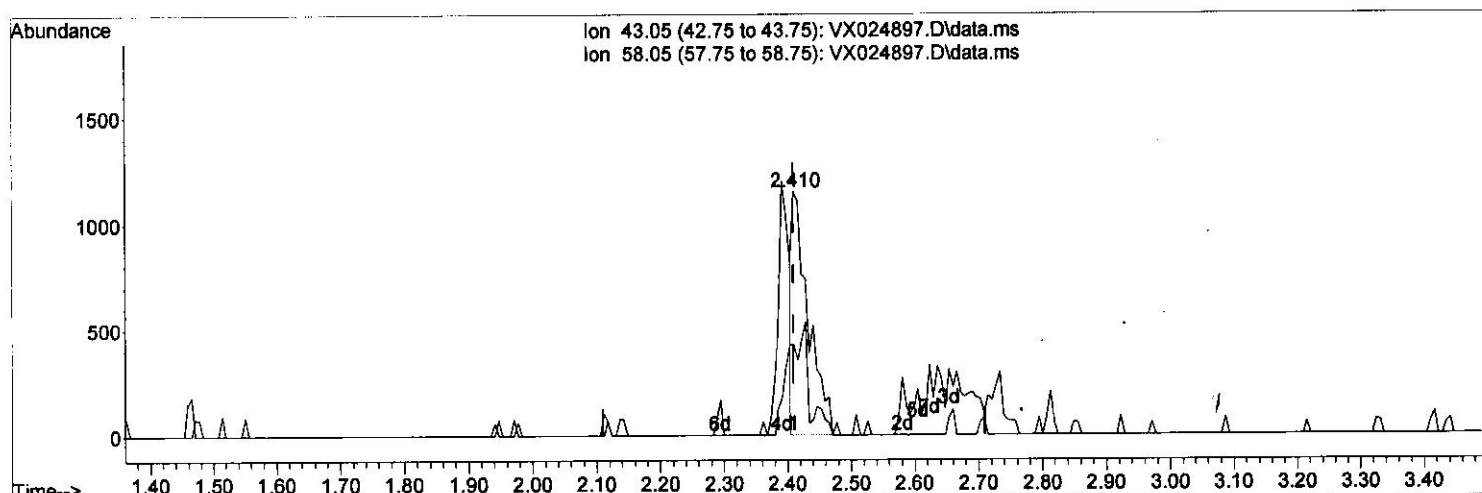

TIC: VX024897.D\data.ms

(13) Acetone (T)

2.410min (-0.000) 2.99 ug/L

response 2063

Ion	Exp%	Act%
43.05	100.00	100.00
58.05	32.10	51.77
0.00	0.00	0.00
0.00	0.00	0.00

Quantitation Report (Qedit)




Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX102321\
 Data File : VX024897.D
 Acq On : 23 Oct 2021 15:49
 Operator : JC/MD
 Sample : M4303-03
 Misc : 25.0mL/MSVOA_X/WATER
 ALS Vial : 12 Sample Multiplier: 1

Instrument :
 MSVOA_X
 ClientSampleId :
 P005-TW001-02

Quant Time: Oct 25 02:34:01 2021
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXTR102221WMA.M
 Quant Title : TRACE VOA SFAM1.0
 QLast Update : Mon Oct 25 02:31:08 2021
 Response via : Initial Calibration

Manual Integrations
 APPROVED

MMDadoda
 10/25/2021 10:25:47 AM

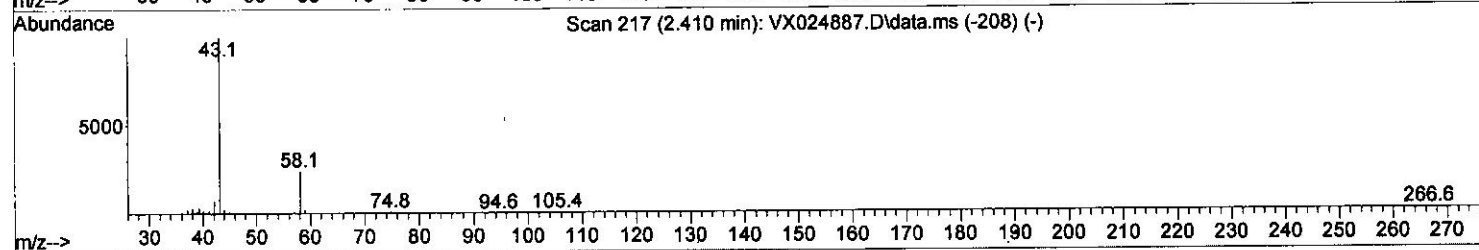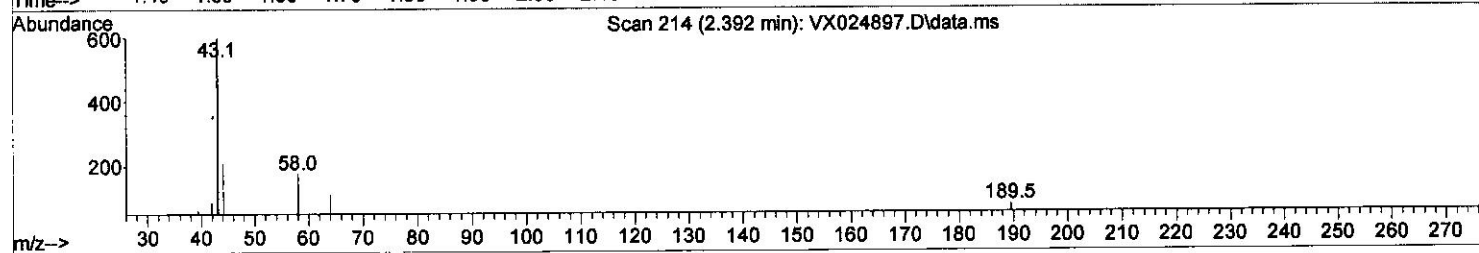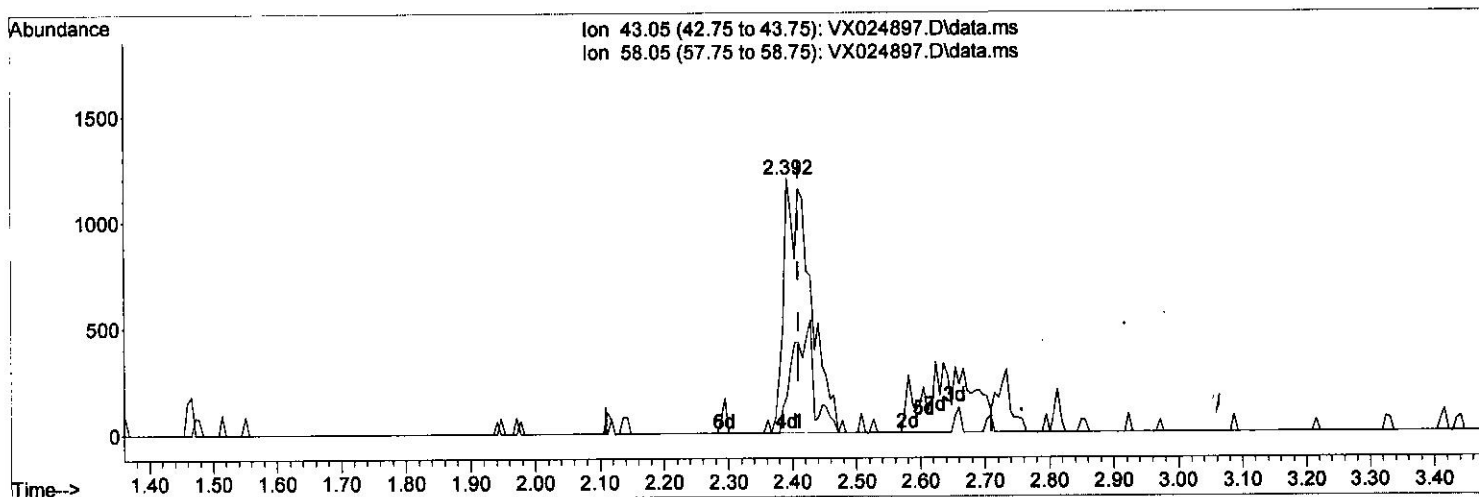

TIC: VX024897.D\data.ms

(13) Acetone (T)

2.392min (-0.018) 5.05 ug/L m

response 3478

Ion	Exp%	Act%
43.05	100.00	100.00
58.05	32.10	30.71
0.00	0.00	0.00
0.00	0.00	0.00

Quantitation Report (QT Reviewed)

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX102321\
 Data File : VX024897.D
 Acq On : 23 Oct 2021 15:49
 Operator : JC/MD
 Sample : M4303-03
 Misc : 25.0mL/MSVOA_X/WATER
 ALS Vial : 12 Sample Multiplier: 1

Instrument :
 MSVOA_X
 ClientSampled :
 P005-TW001-02

Manual Integrations
 APPROVED

MMDadoda
 10/25/2021 10:25:47 AM

Quant Time: Oct 25 02:34:01 2021
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXTR102221WMA.M
 Quant Title : TRACE VOA SFAM1.0
 QLast Update : Mon Oct 25 02:31:08 2021
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)
Internal Standards						
1) 1,4-Difluorobenzene	6.769	114	85596	5.000	ug/L	0.00
28) Chlorobenzene-d5	10.055	117	80496	5.000	ug/L	0.00
58) 1,4-Dichlorobenzene-d4	12.030	152	35822	5.000	ug/L	0.00
System Monitoring Compounds						
4) Vinyl Chloride-d3	1.368	65	11605	4.618	ug/L	0.00
Spiked Amount	5.000	Range 40 - 130	Recovery	=	92.400%	
7) Chloroethane-d5	1.672	69	11768	5.198	ug/L	0.00
Spiked Amount	5.000	Range 65 - 130	Recovery	=	104.000%	
11) 1,1-Dichloroethene-d2	2.306	63	32058	3.422	ug/L	0.00
Spiked Amount	5.000	Range 60 - 125	Recovery	=	68.400%	
20) 2-Butanone-d5	4.477	46	50465	54.928	ug/L	0.00
Spiked Amount	50.000	Range 40 - 130	Recovery	=	109.860%	
24) Chloroform-d	5.068	84	52933	4.376	ug/L	0.00
Spiked Amount	5.000	Range 70 - 125	Recovery	=	87.600%	
26) 1,2-Dichloroethane-d4	5.964	65	29712	4.494	ug/L	0.00
Spiked Amount	5.000	Range 70 - 130	Recovery	=	89.800%	
32) Benzene-d6	5.983	84	86396	4.606	ug/L	0.00
Spiked Amount	5.000	Range 70 - 125	Recovery	=	92.200%	
36) 1,2-Dichloropropane-d6	7.318	67	27842	4.653	ug/L	0.00
Spiked Amount	5.000	Range 60 - 140	Recovery	=	93.000%	
41) Toluene-d8	8.653	98	80146	4.262	ug/L	0.00
Spiked Amount	5.000	Range 70 - 130	Recovery	=	85.200%	
43) trans-1,3-Dichloroprop...	8.952	79	10251	3.732	ug/L	0.00
Spiked Amount	5.000	Range 55 - 130	Recovery	=	74.600%	
46) 2-Hexanone-d5	9.390	63	46036	46.573	ug/L	0.00
Spiked Amount	50.000	Range 45 - 130	Recovery	=	93.140%	
56) 1,1,2,2-Tetrachloroeth...	11.195	84	20993	4.590	ug/L	0.00
Spiked Amount	5.000	Range 65 - 120	Recovery	=	91.800%	
66) 1,2-Dichlorobenzene-d4	12.323	152	26626	4.411	ug/L	0.00
Spiked Amount	5.000	Range 80 - 120	Recovery	=	88.200%	
Target Compounds						
13) Acetone	2.392	43	3478m	5.047	ug/L	Qvalue

m D
 10/28/21

(#) = qualifier out of range (m) = manual integration (+) = signals summed