

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX102321\
 Data File : VX024893.D
 Acq On : 23 Oct 2021 14:14
 Operator : JC/MD
 Sample : M4291-23
 Misc : 25.0mL/MSVOA_X/WATER
 ALS Vial : 8 Sample Multiplier: 1

Instrument :
 MSVOA_X
 ClientSampleId :
 P050-TW001-01

Quant Time: Oct 25 02:33:07 2021
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXTR102221WMA.M
 Quant Title : TRACE VOA SFAM1.0
 QLast Update : Mon Oct 25 02:31:08 2021
 Response via : Initial Calibration

Compound	R.T. QIon		Response	Conc	Units	Dev(Min)


Internal Standards						
1) 1,4-Difluorobenzene	6.769	114	64805	5.000	ug/L	0.00
28) Chlorobenzene-d5	10.055	117	58116	5.000	ug/L	0.00
58) 1,4-Dichlorobenzene-d4	12.024	152	24499	5.000	ug/L	0.00
System Monitoring Compounds						
4) Vinyl Chloride-d3	1.368	65	13762	7.233	ug/L	0.00
Spiked Amount	5.000	Range 40 - 130	Recovery	= 144.600%#		
7) Chloroethane-d5	1.672	69	12773	7.451	ug/L	0.00
Spiked Amount	5.000	Range 65 - 130	Recovery	= 149.000%#		
11) 1,1-Dichloroethene-d2	2.306	63	29424	4.149	ug/L	0.00
Spiked Amount	5.000	Range 60 - 125	Recovery	= 83.000%		
20) 2-Butanone-d5	4.477	46	56663	81.461	ug/L	0.00
Spiked Amount	50.000	Range 40 - 130	Recovery	= 162.920%#		
24) Chloroform-d	5.068	84	56432	6.161	ug/L	0.00
Spiked Amount	5.000	Range 70 - 125	Recovery	= 123.200%		
26) 1,2-Dichloroethane-d4	5.970	65	31692	6.331	ug/L	0.00
Spiked Amount	5.000	Range 70 - 130	Recovery	= 126.600%		
32) Benzene-d6	5.983	84	87130	6.434	ug/L	0.00
Spiked Amount	5.000	Range 70 - 125	Recovery	= 128.600%#		
36) 1,2-Dichloropropane-d6	7.312	67	29308	6.784	ug/L	0.00
Spiked Amount	5.000	Range 60 - 140	Recovery	= 135.600%		
41) Toluene-d8	8.653	98	74287	5.472	ug/L	0.00
Spiked Amount	5.000	Range 70 - 130	Recovery	= 109.400%		
43) trans-1,3-Dichloroprop...	8.952	79	9812	4.948	ug/L	0.00
Spiked Amount	5.000	Range 55 - 130	Recovery	= 99.000%		
46) 2-Hexanone-d5	9.391	63	49058	68.743	ug/L	0.00
Spiked Amount	50.000	Range 45 - 130	Recovery	= 137.480%#		
56) 1,1,2,2-Tetrachloroeth...	11.195	84	22028	6.671	ug/L	0.00
Spiked Amount	5.000	Range 65 - 120	Recovery	= 133.400%#		
66) 1,2-Dichlorobenzene-d4	12.323	152	24960	6.046	ug/L	0.00
Spiked Amount	5.000	Range 80 - 120	Recovery	= 121.000%#		
Target Compounds						
					Qvalue	
13) Acetone	2.404	43	861	1.650	ug/L	95
16) Methylene chloride	2.800	84	1844	0.399	ug/L	92


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX102321\
Data File : VX024893.D
Acq On : 23 Oct 2021 14:14
Operator : JC/MD
Sample : M4291-23
Misc : 25.0mL/MSVOA_X/WATER
ALS Vial : 8 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
P050-TW001-01

Quant Time: Oct 25 02:33:07 2021
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXTR102221WMA.M
Quant Title : TRACE VOA SFAM1.0
QLast Update : Mon Oct 25 02:31:08 2021
Response via : Initial Calibration




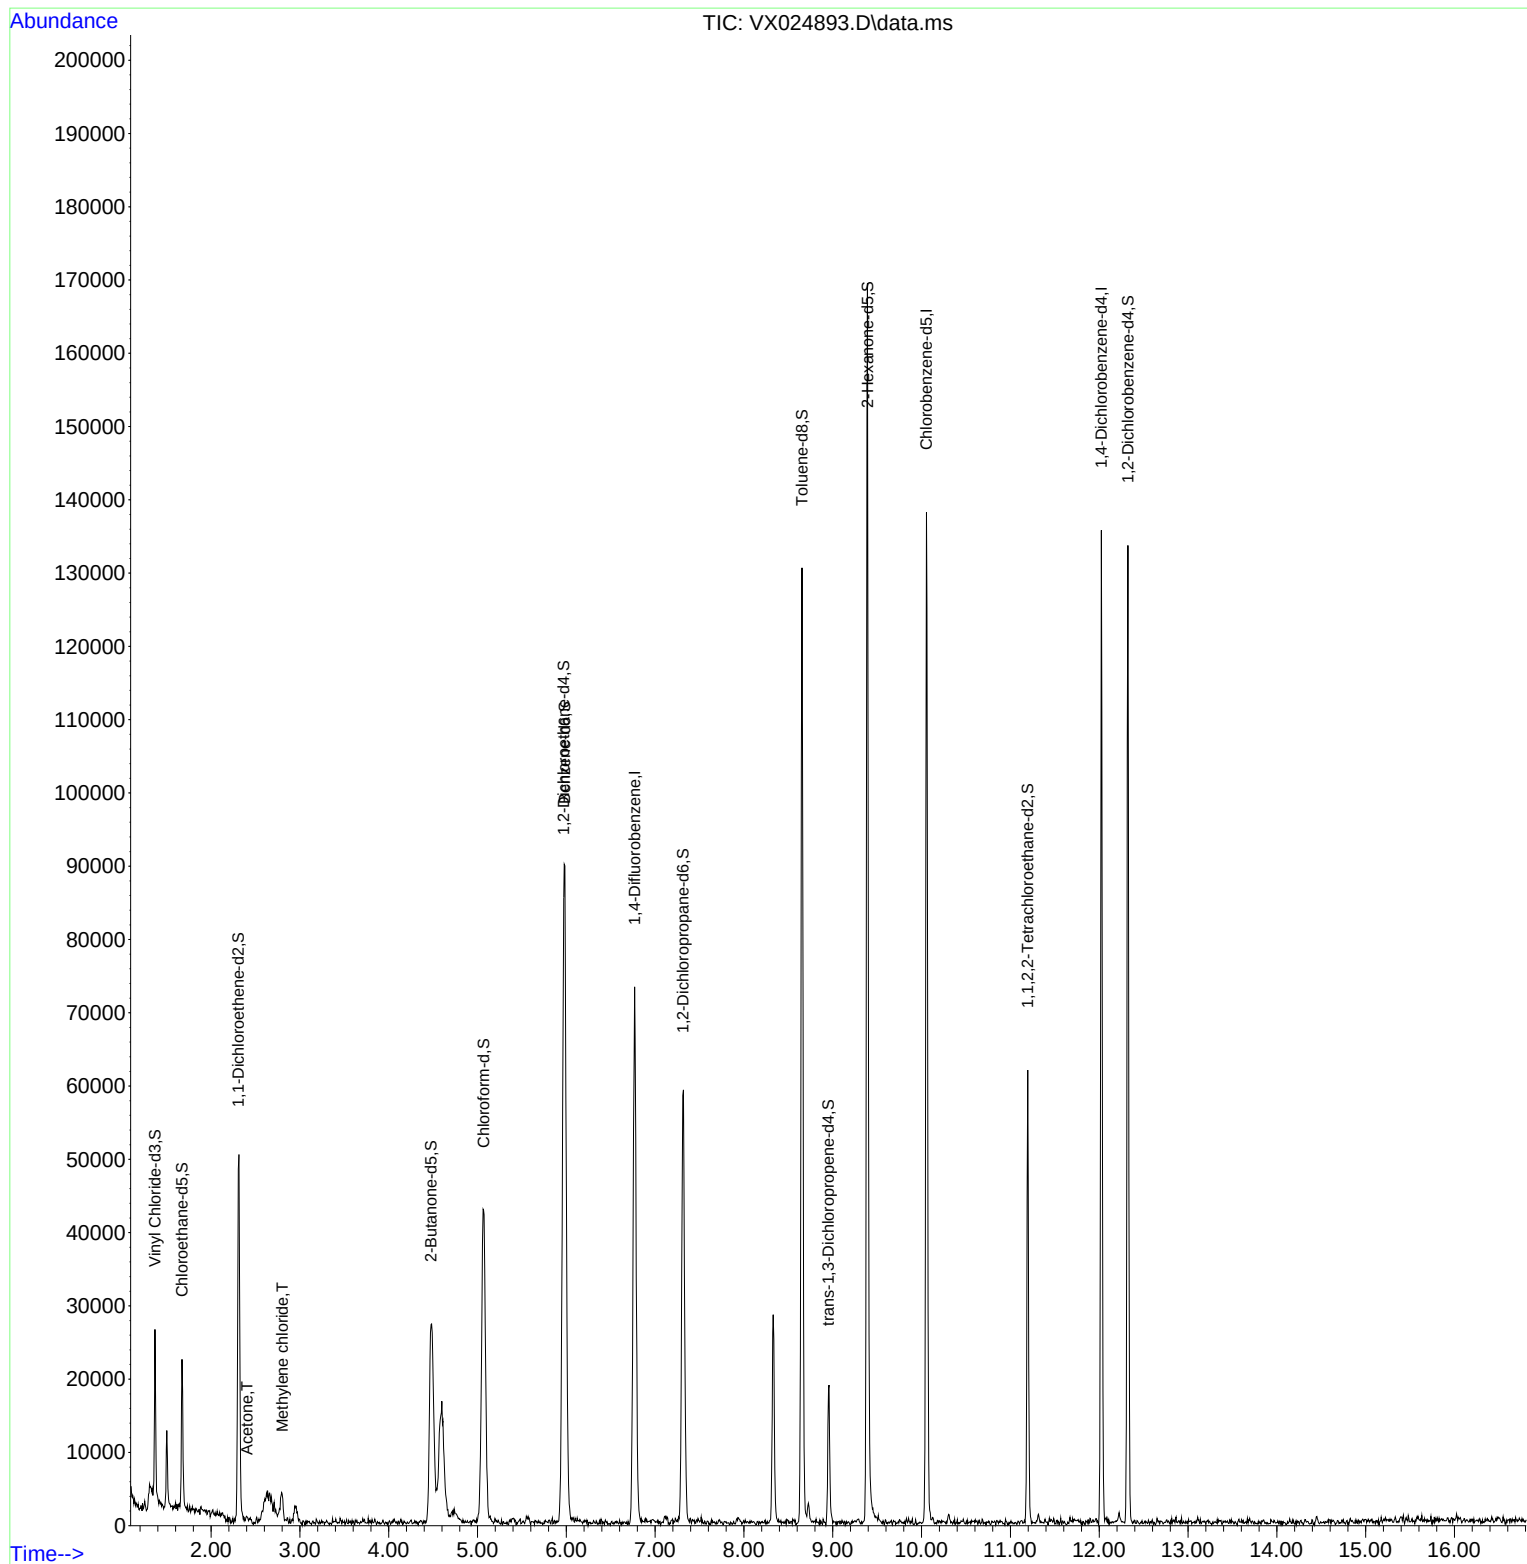


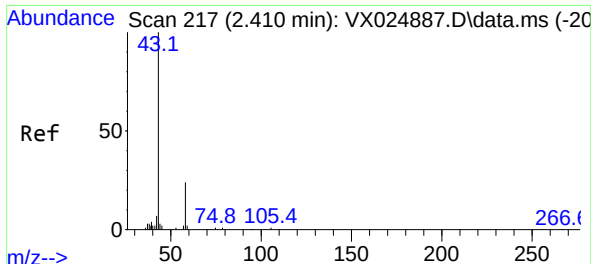

#13
Acetone
Concen: 1.650 ug/L
RT: 2.404 min Scan# 216
Delta R.T. -0.006 min
Lab File: VX024893.D
Acq: 23 Oct 2021 14:14

Instrument :
MSVOA_X
ClientSampleId :
P050-TW001-01

Tgt Ion: 43 Resp: 861
Ion Ratio Lower Upper
43 100
58 29.3 0.0 64.2

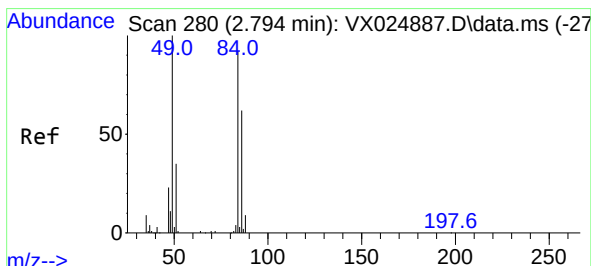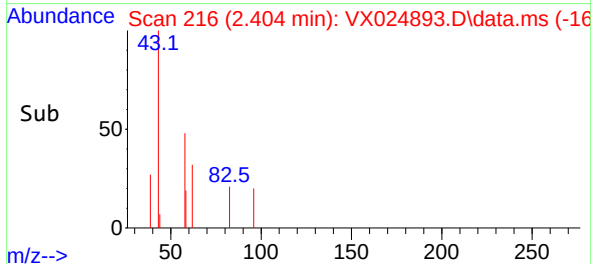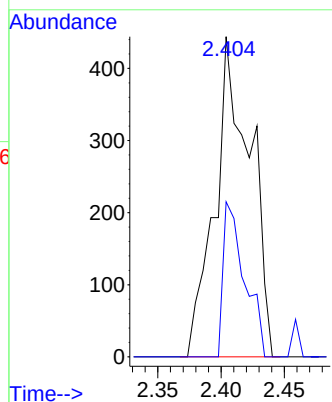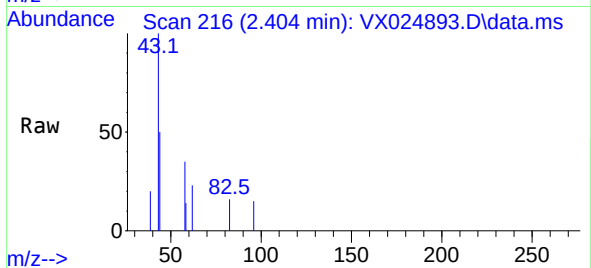

#16
Methylene chloride
Concen: 0.399 ug/L
RT: 2.800 min Scan# 281
Delta R.T. 0.006 min
Lab File: VX024893.D
Acq: 23 Oct 2021 14:14

Tgt Ion: 84 Resp: 1844
Ion Ratio Lower Upper
84 100
86 71.7 49.5 91.9
49 101.9 62.7 116.5

