

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX102321\
 Data File : VX024897.D
 Acq On : 23 Oct 2021 15:49
 Operator : JC/MD
 Sample : M4303-03
 Misc : 25.0mL/MSVOA_X/WATER
 ALS Vial : 12 Sample Multiplier: 1

Instrument :
 MSVOA_X
 ClientSampleId :
 P005-TW001-02

Manual Integrations
 APPROVED

MMDadoda
 10/25/2021 10:25:47 AM

Quant Time: Oct 25 02:34:01 2021
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXTR102221WMA.M
 Quant Title : TRACE VOA SFAM1.0
 QLast Update : Mon Oct 25 02:31:08 2021
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)

Internal Standards						
1) 1,4-Difluorobenzene	6.769	114	85596	5.000	ug/L	0.00
28) Chlorobenzene-d5	10.055	117	80496	5.000	ug/L	0.00
58) 1,4-Dichlorobenzene-d4	12.030	152	35822	5.000	ug/L	0.00
System Monitoring Compounds						
4) Vinyl Chloride-d3	1.368	65	11605	4.618	ug/L	0.00
Spiked Amount	5.000	Range	40 - 130	Recovery	=	92.400%
7) Chloroethane-d5	1.672	69	11768	5.198	ug/L	0.00
Spiked Amount	5.000	Range	65 - 130	Recovery	=	104.000%
11) 1,1-Dichloroethene-d2	2.306	63	32058	3.422	ug/L	0.00
Spiked Amount	5.000	Range	60 - 125	Recovery	=	68.400%
20) 2-Butanone-d5	4.477	46	50465	54.928	ug/L	0.00
Spiked Amount	50.000	Range	40 - 130	Recovery	=	109.860%
24) Chloroform-d	5.068	84	52933	4.376	ug/L	0.00
Spiked Amount	5.000	Range	70 - 125	Recovery	=	87.600%
26) 1,2-Dichloroethane-d4	5.964	65	29712	4.494	ug/L	0.00
Spiked Amount	5.000	Range	70 - 130	Recovery	=	89.800%
32) Benzene-d6	5.983	84	86396	4.606	ug/L	0.00
Spiked Amount	5.000	Range	70 - 125	Recovery	=	92.200%
36) 1,2-Dichloropropane-d6	7.318	67	27842	4.653	ug/L	0.00
Spiked Amount	5.000	Range	60 - 140	Recovery	=	93.000%
41) Toluene-d8	8.653	98	80146	4.262	ug/L	0.00
Spiked Amount	5.000	Range	70 - 130	Recovery	=	85.200%
43) trans-1,3-Dichloroprop...	8.952	79	10251	3.732	ug/L	0.00
Spiked Amount	5.000	Range	55 - 130	Recovery	=	74.600%
46) 2-Hexanone-d5	9.390	63	46036	46.573	ug/L	0.00
Spiked Amount	50.000	Range	45 - 130	Recovery	=	93.140%
56) 1,1,2,2-Tetrachloroeth...	11.195	84	20993	4.590	ug/L	0.00
Spiked Amount	5.000	Range	65 - 120	Recovery	=	91.800%
66) 1,2-Dichlorobenzene-d4	12.323	152	26626	4.411	ug/L	0.00
Spiked Amount	5.000	Range	80 - 120	Recovery	=	88.200%
Target Compounds					Qvalue	
13) Acetone	2.392	43	3478m	5.047	ug/L	

(#) = qualifier out of range (m) = manual integration (+) = signals summed


Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX102321\
Data File : VX024897.D
Acq On : 23 Oct 2021 15:49
Operator : JC/MD
Sample : M4303-03
Misc : 25.0mL/MSVOA_X/WATER
ALS Vial : 12 Sample Multiplier: 1


Instrument :
MSVOA_X
ClientSampleId :
P005-TW001-02

Manual Integrations
APPROVED

MMDadoda
10/25/2021 10:25:47 AM

Quant Time: Oct 25 02:34:01 2021
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXTR102221WMA.M
Quant Title : TRACE VOA SFAM1.0
QLast Update : Mon Oct 25 02:31:08 2021
Response via : Initial Calibration

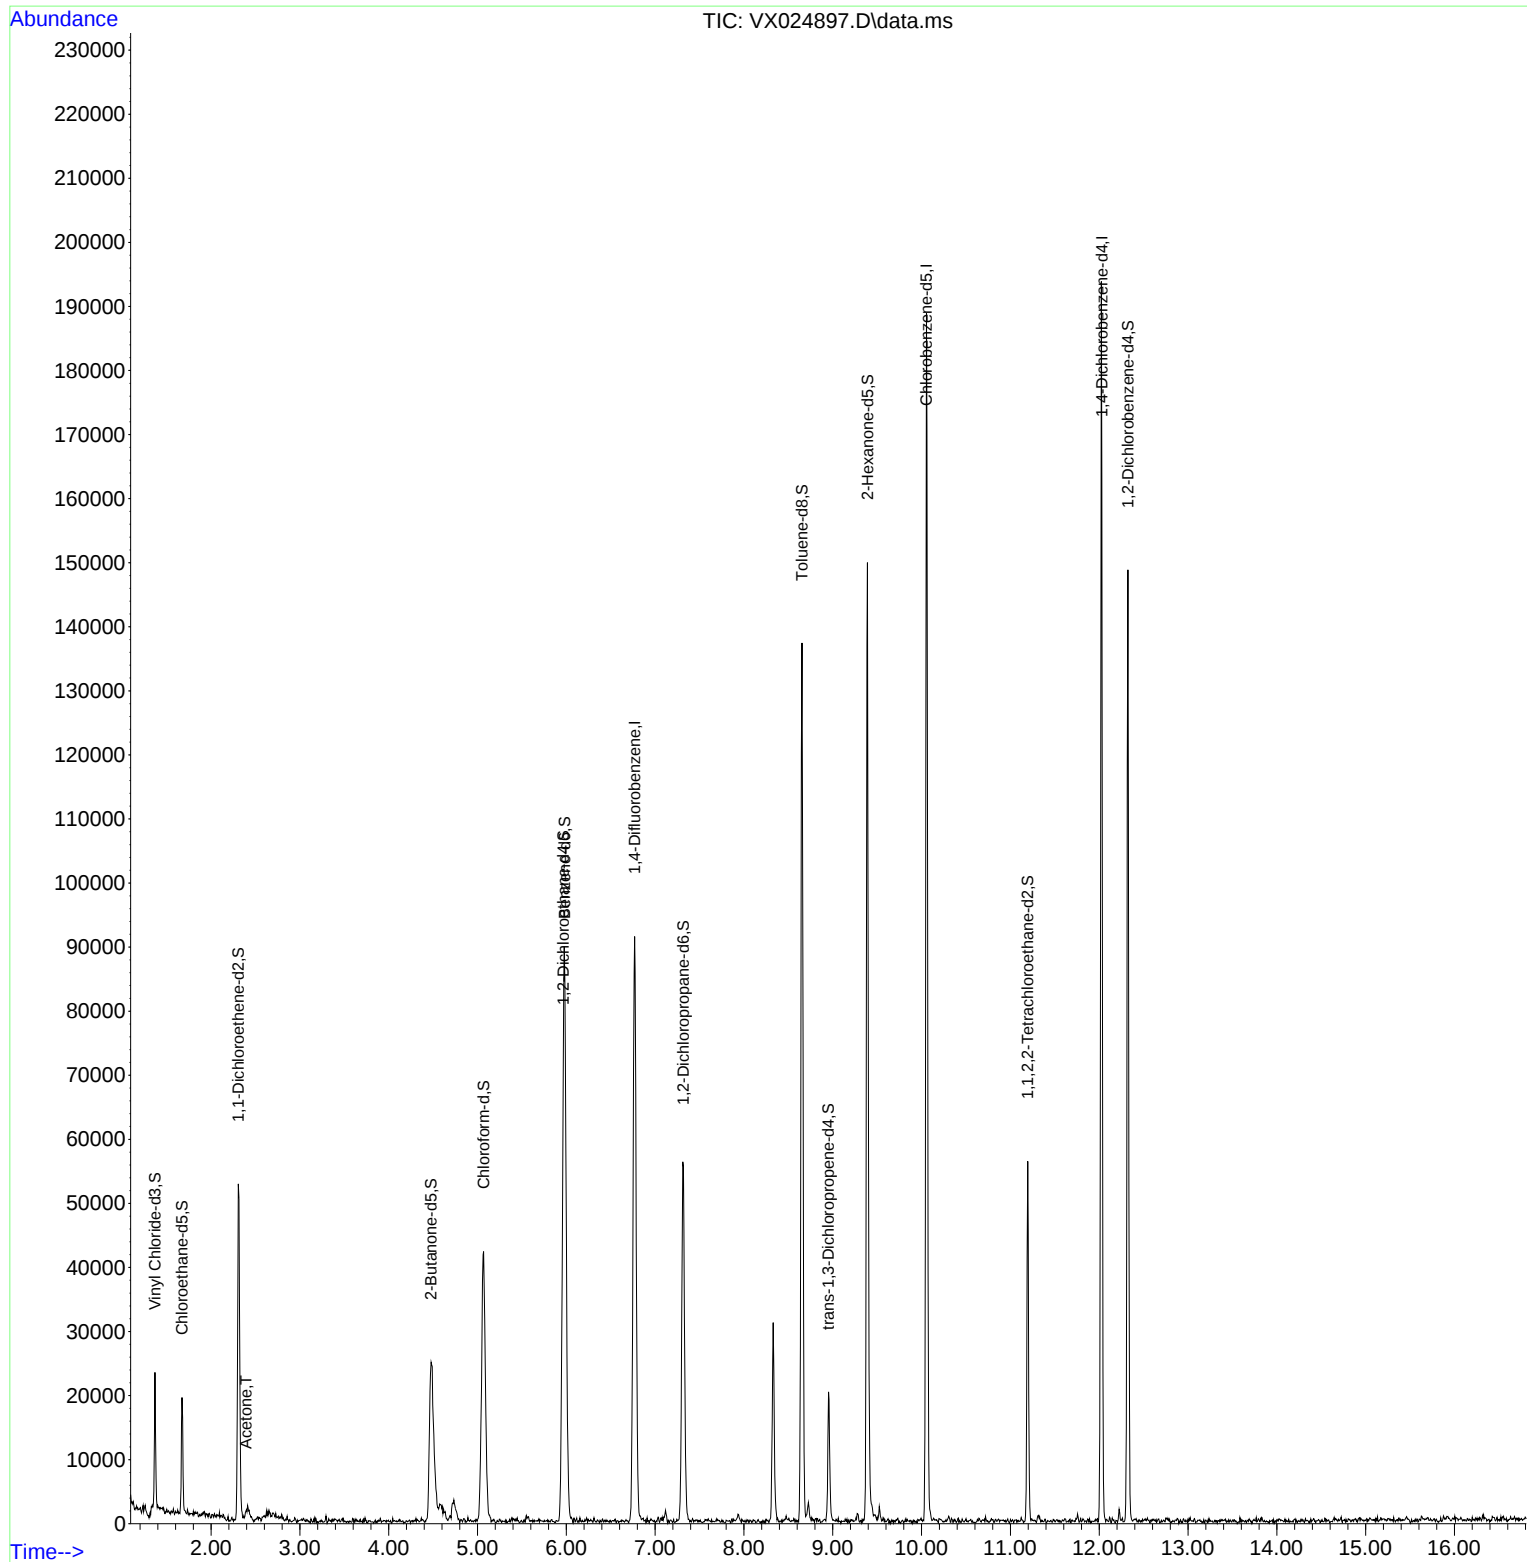

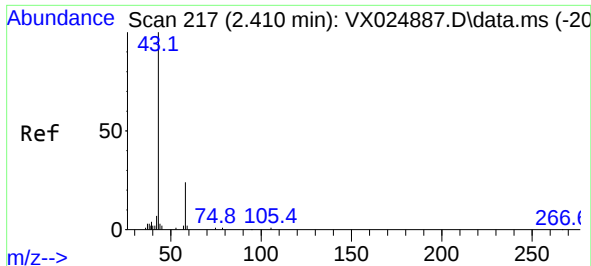

#13
Acetone
Concen: 5.047 ug/L m
RT: 2.392 min Scan# 214
Delta R.T. -0.018 min
Lab File: VX024897.D
Acq: 23 Oct 2021 15:49

Tgt Ion: 43 Resp: 3478
Ion Ratio Lower Upper
43 100
58 30.7 0.0 64.2

Instrument :
MSVOA_X
ClientSampleId :
P005-TW001-02

Manual Integrations
APPROVED

MMDadoda
10/25/2021 10:25:47 AM

