

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX102321\
 Data File : VX024899.D
 Acq On : 23 Oct 2021 16:37
 Operator : JC/MD
 Sample : M4303-05
 Misc : 25.0mL/MSVOA_X/WATER
 ALS Vial : 14 Sample Multiplier: 1

Instrument :
 MSVOA_X
 ClientSampleId :
 P010-TW001-02

Quant Time: Oct 25 02:34:25 2021
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXTR102221WMA.M
 Quant Title : TRACE VOA SFAM1.0
 QLast Update : Mon Oct 25 02:31:08 2021
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) 1,4-Difluorobenzene	6.769	114	84817	5.000	ug/L	0.00
28) Chlorobenzene-d5	10.055	117	79370	5.000	ug/L	0.00
58) 1,4-Dichlorobenzene-d4	12.024	152	36836	5.000	ug/L	0.00
System Monitoring Compounds						
4) Vinyl Chloride-d3	1.368	65	10878	4.369	ug/L	0.00
Spiked Amount	5.000	Range	40 - 130	Recovery	=	87.400%
7) Chloroethane-d5	1.672	69	10974	4.891	ug/L	0.00
Spiked Amount	5.000	Range	65 - 130	Recovery	=	97.800%
11) 1,1-Dichloroethene-d2	2.306	63	29936	3.225	ug/L	0.00
Spiked Amount	5.000	Range	60 - 125	Recovery	=	64.600%
20) 2-Butanone-d5	4.477	46	47176	51.820	ug/L	0.00
Spiked Amount	50.000	Range	40 - 130	Recovery	=	103.640%
24) Chloroform-d	5.068	84	52978	4.420	ug/L	0.00
Spiked Amount	5.000	Range	70 - 125	Recovery	=	88.400%
26) 1,2-Dichloroethane-d4	5.964	65	29554	4.511	ug/L	0.00
Spiked Amount	5.000	Range	70 - 130	Recovery	=	90.200%
32) Benzene-d6	5.983	84	85426	4.619	ug/L	0.00
Spiked Amount	5.000	Range	70 - 125	Recovery	=	92.400%
36) 1,2-Dichloropropane-d6	7.318	67	26628	4.513	ug/L	0.00
Spiked Amount	5.000	Range	60 - 140	Recovery	=	90.200%
41) Toluene-d8	8.653	98	79338	4.279	ug/L	0.00
Spiked Amount	5.000	Range	70 - 130	Recovery	=	85.600%
43) trans-1,3-Dichloroprop...	8.958	79	10935	4.038	ug/L	0.00
Spiked Amount	5.000	Range	55 - 130	Recovery	=	80.800%
46) 2-Hexanone-d5	9.390	63	45160	46.335	ug/L	0.00
Spiked Amount	50.000	Range	45 - 130	Recovery	=	92.680%
56) 1,1,2,2-Tetrachloroeth...	11.195	84	20123	4.462	ug/L	0.00
Spiked Amount	5.000	Range	65 - 120	Recovery	=	89.200%
66) 1,2-Dichlorobenzene-d4	12.323	152	25993	4.187	ug/L	0.00
Spiked Amount	5.000	Range	80 - 120	Recovery	=	83.800%
Target Compounds					Qvalue	
13) Acetone	2.410	43	1228	1.798	ug/L	61


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX102321\
Data File : VX024899.D
Acq On : 23 Oct 2021 16:37
Operator : JC/MD
Sample : M4303-05
Misc : 25.0mL/MSVOA_X/WATER
ALS Vial : 14 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
P010-TW001-02

Quant Time: Oct 25 02:34:25 2021
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXTR102221WMA.M
Quant Title : TRACE VOA SFAM1.0
QLast Update : Mon Oct 25 02:31:08 2021
Response via : Initial Calibration

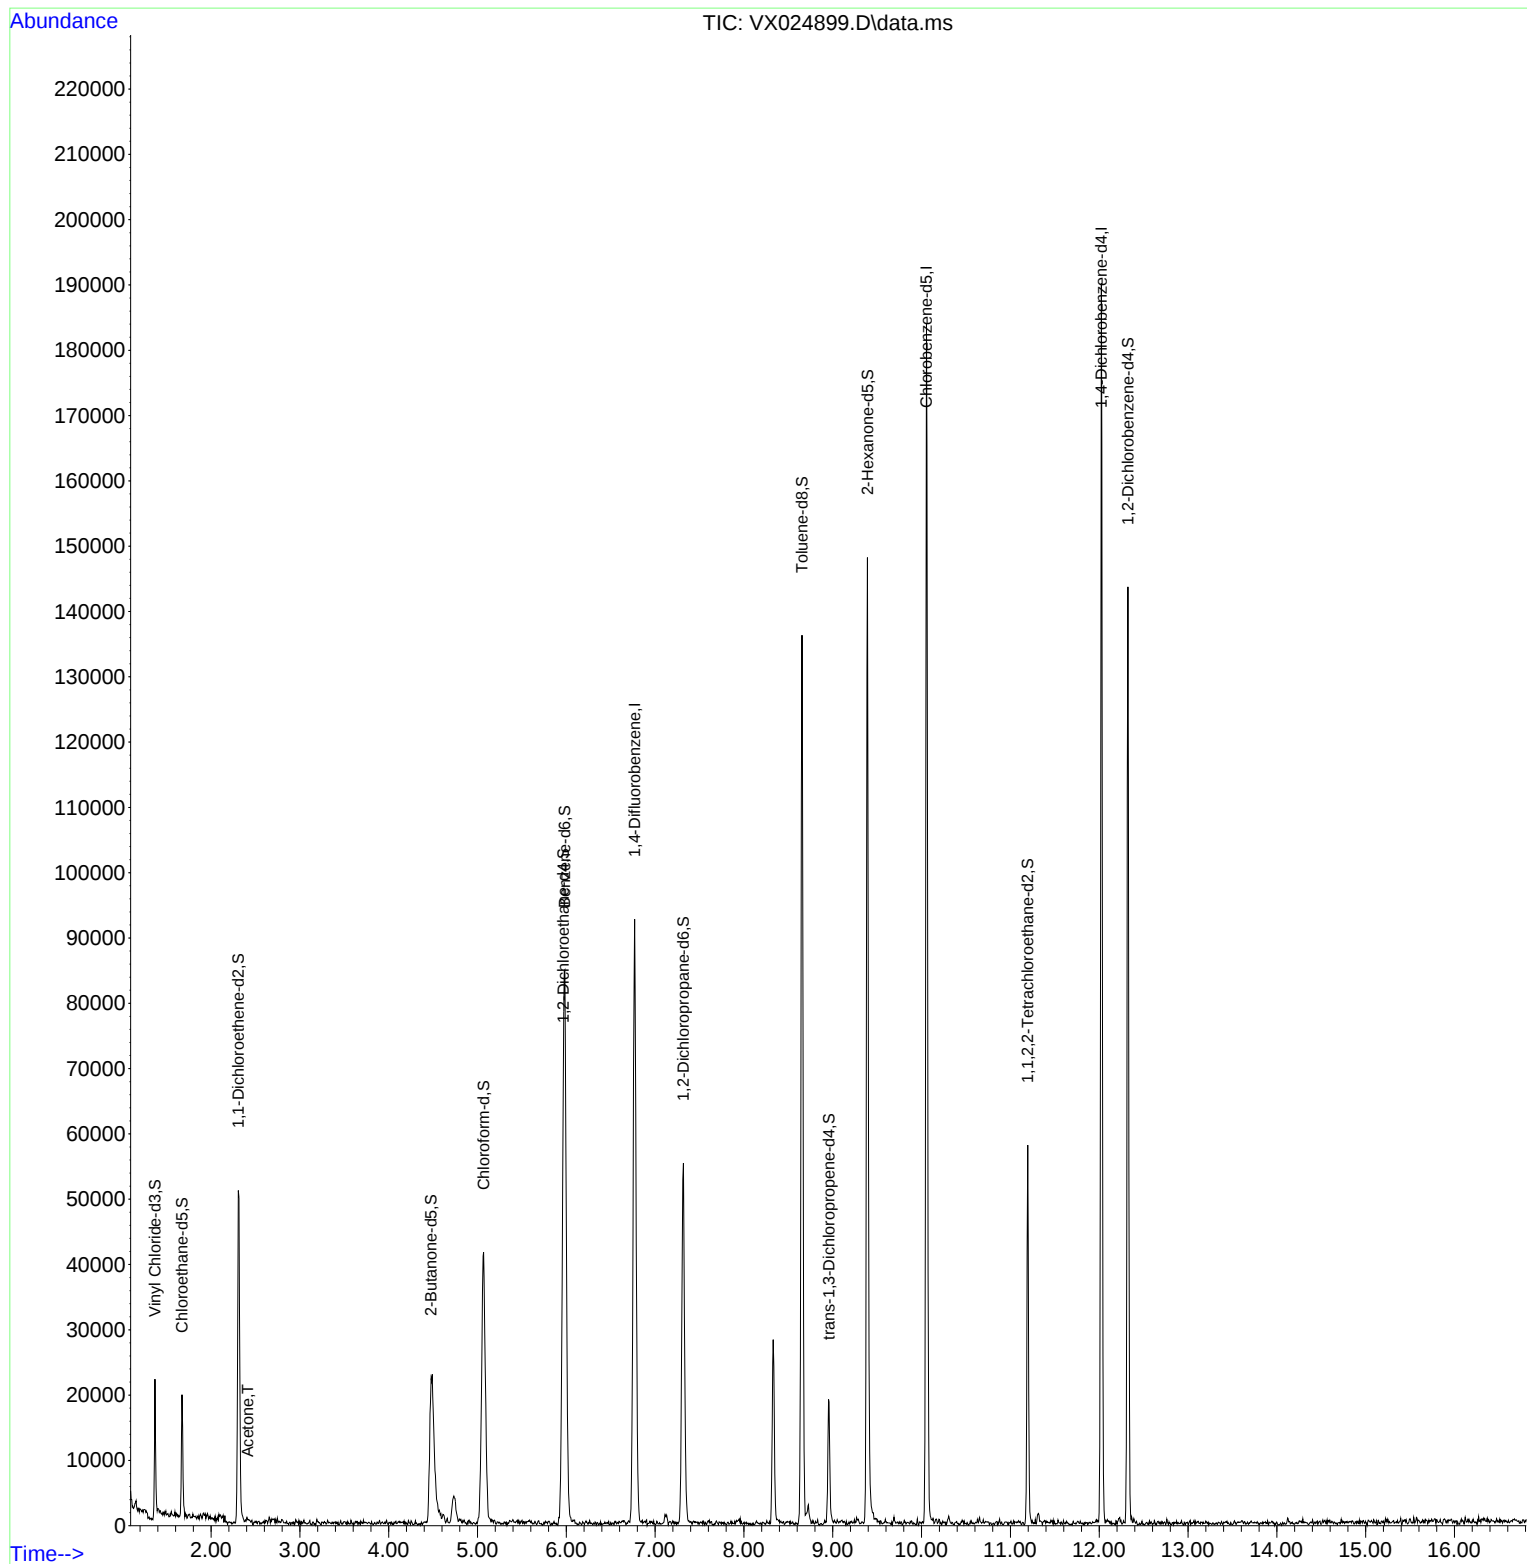

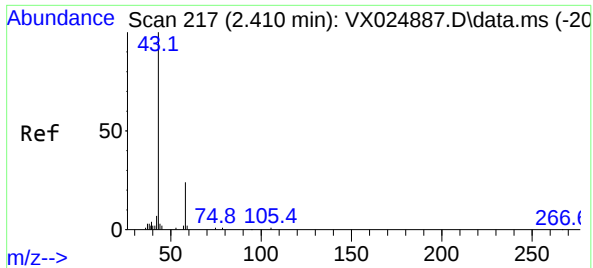

#13
 Acetone
 Concen: 1.798 ug/L
 RT: 2.410 min Scan# 217
 Delta R.T. -0.000 min
 Lab File: VX024899.D
 Acq: 23 Oct 2021 16:37

Instrument :
 MSVOA_X
 ClientSampleId :
 P010-TW001-02

Tgt Ion: 43 Resp: 1228
 Ion Ratio Lower Upper
 43 100
 58 10.5 0.0 64.2

