

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX102321\
 Data File : VX024902.D
 Acq On : 23 Oct 2021 17:48
 Operator : JC/MD
 Sample : M4303-10
 Misc : 25.0mL/MSVOA_X/WATER
 ALS Vial : 17 Sample Multiplier: 1

Instrument :
 MSVOA_X
 ClientSampleId :
 P013-TW001-03

Quant Time: Oct 25 02:35:01 2021
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXTR102221WMA.M
 Quant Title : TRACE VOA SFAM1.0
 QLast Update : Mon Oct 25 02:31:08 2021
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) 1,4-Difluorobenzene	6.769	114	74127	5.000	ug/L	0.00
28) Chlorobenzene-d5	10.055	117	68741	5.000	ug/L	0.00
58) 1,4-Dichlorobenzene-d4	12.024	152	31577	5.000	ug/L	0.00
System Monitoring Compounds						
4) Vinyl Chloride-d3	1.368	65	10742	4.936	ug/L	0.00
Spiked Amount	5.000	Range	40 - 130	Recovery	=	98.800%
7) Chloroethane-d5	1.672	69	10673	5.443	ug/L	0.00
Spiked Amount	5.000	Range	65 - 130	Recovery	=	108.800%
11) 1,1-Dichloroethene-d2	2.306	63	28032	3.456	ug/L	0.00
Spiked Amount	5.000	Range	60 - 125	Recovery	=	69.200%
20) 2-Butanone-d5	4.477	46	46665	58.650	ug/L	0.00
Spiked Amount	50.000	Range	40 - 130	Recovery	=	117.300%
24) Chloroform-d	5.074	84	52561	5.017	ug/L	0.01
Spiked Amount	5.000	Range	70 - 125	Recovery	=	100.400%
26) 1,2-Dichloroethane-d4	5.964	65	29067	5.076	ug/L	0.00
Spiked Amount	5.000	Range	70 - 130	Recovery	=	101.600%
32) Benzene-d6	5.983	84	80216	5.008	ug/L	0.00
Spiked Amount	5.000	Range	70 - 125	Recovery	=	100.200%
36) 1,2-Dichloropropane-d6	7.318	67	26518	5.189	ug/L	0.00
Spiked Amount	5.000	Range	60 - 140	Recovery	=	103.800%
41) Toluene-d8	8.653	98	75484	4.701	ug/L	0.00
Spiked Amount	5.000	Range	70 - 130	Recovery	=	94.000%
43) trans-1,3-Dichloroprop...	8.958	79	9392	4.004	ug/L	0.00
Spiked Amount	5.000	Range	55 - 130	Recovery	=	80.000%
46) 2-Hexanone-d5	9.391	63	43853	51.951	ug/L	0.00
Spiked Amount	50.000	Range	45 - 130	Recovery	=	103.900%
56) 1,1,2,2-Tetrachloroeth...	11.195	84	19916	5.099	ug/L	0.00
Spiked Amount	5.000	Range	65 - 120	Recovery	=	102.000%
66) 1,2-Dichlorobenzene-d4	12.323	152	25269	4.749	ug/L	0.00
Spiked Amount	5.000	Range	80 - 120	Recovery	=	95.000%
Target Compounds						Qvalue
3) Chloromethane	1.294	50	626	0.211	ug/L	100

(#) = qualifier out of range (m) = manual integration (+) = signals summed


Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX102321\
Data File : VX024902.D
Acq On : 23 Oct 2021 17:48
Operator : JC/MD
Sample : M4303-10
Misc : 25.0mL/MSVOA_X/WATER
ALS Vial : 17 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
P013-TW001-03

Quant Time: Oct 25 02:35:01 2021
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXTR102221WMA.M
Quant Title : TRACE VOA SFAM1.0
QLast Update : Mon Oct 25 02:31:08 2021
Response via : Initial Calibration

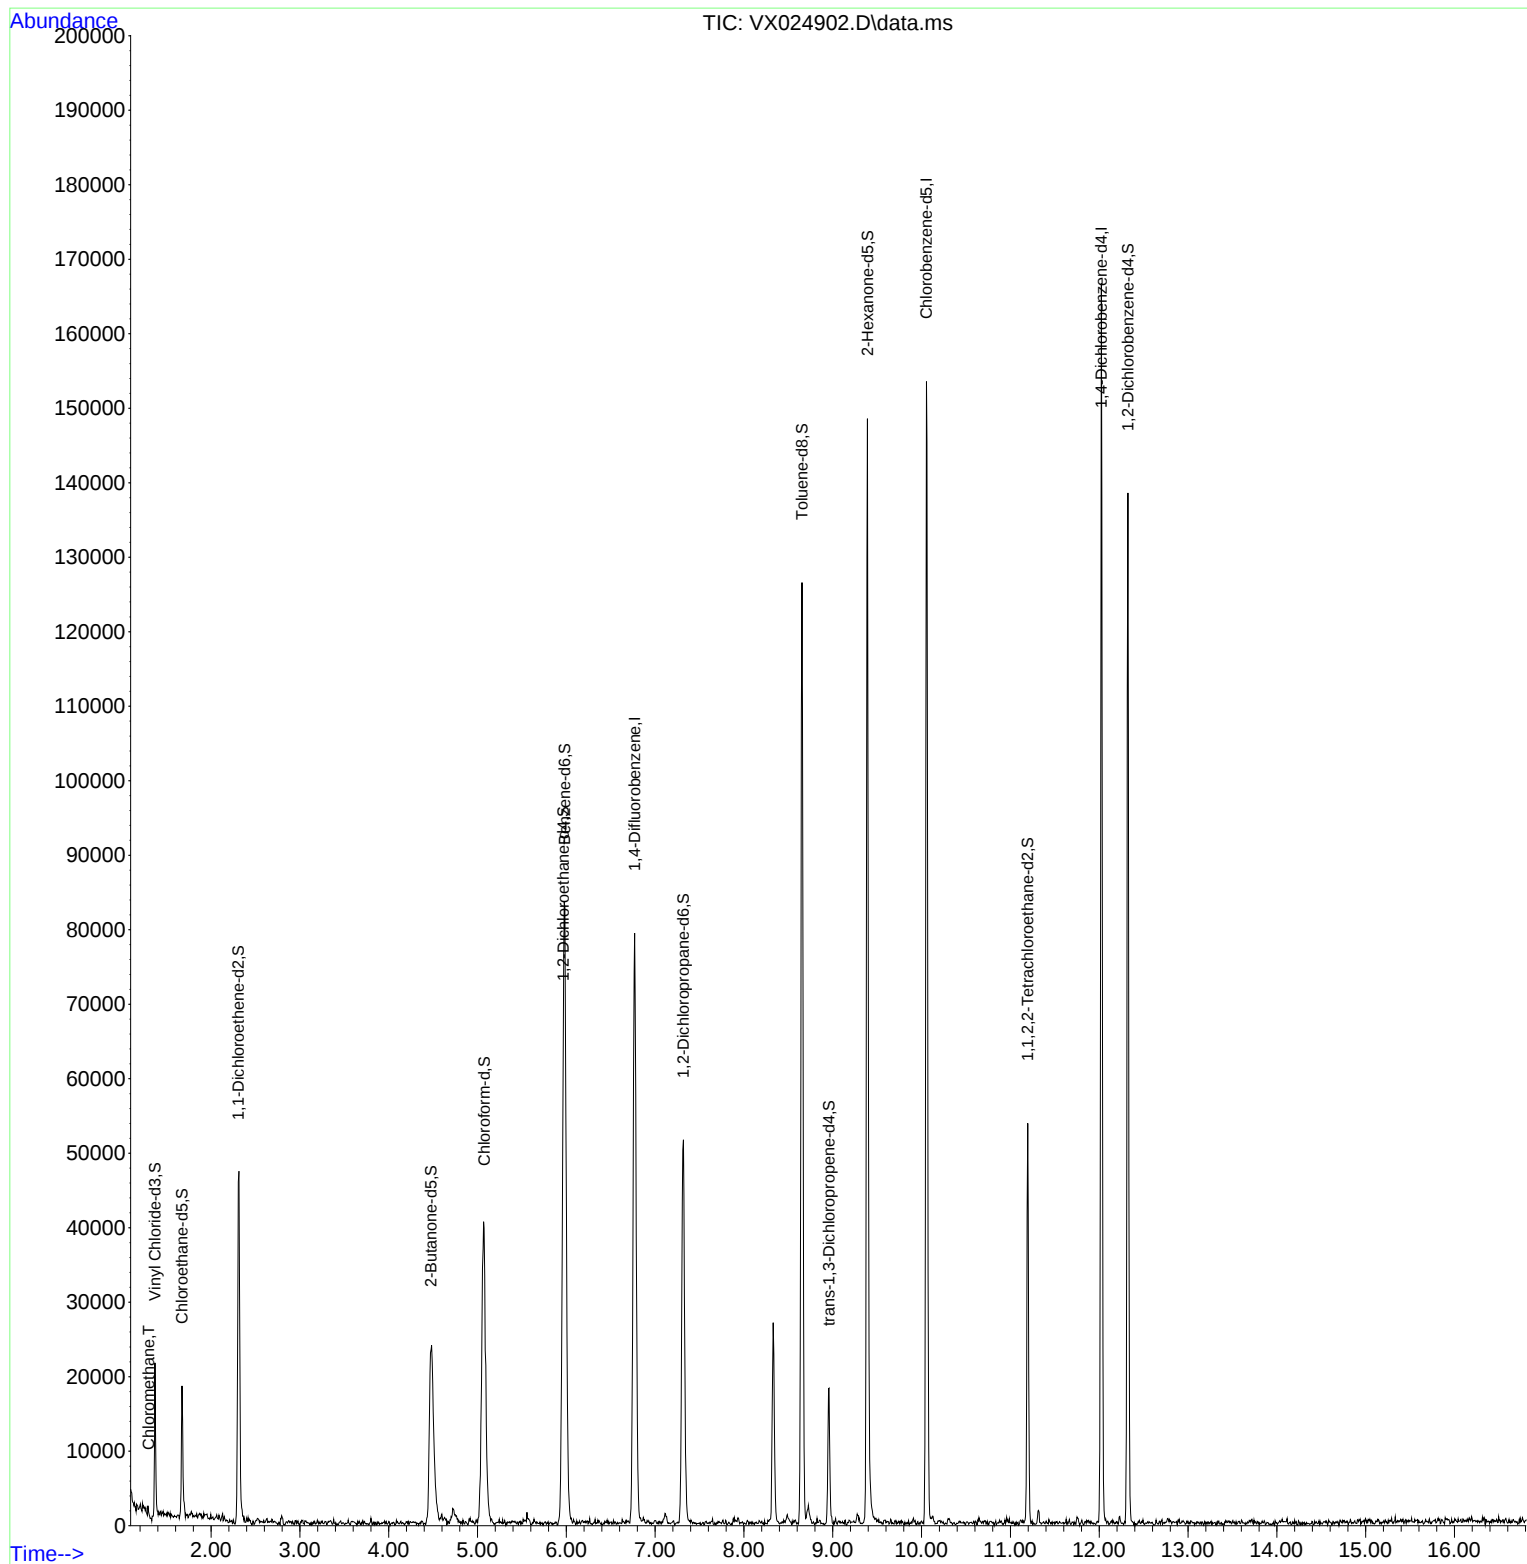


Abundance Scan 33 (1.288 min): VX024887.D\data.ms (-28)

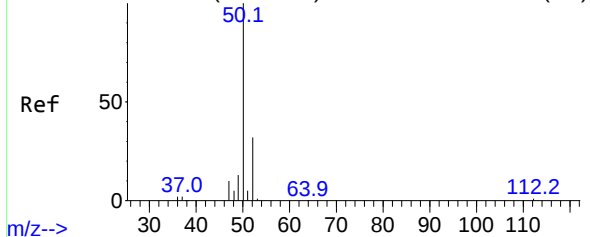


m/z-->

Abundance Scan 34 (1.294 min): VX024902.D\data.ms

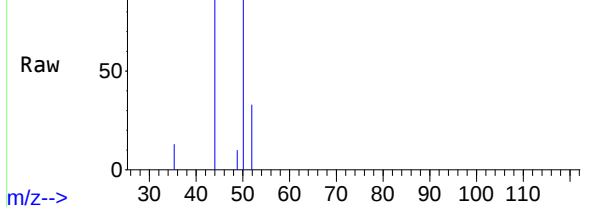

m/z-->


Abundance Scan 34 (1.294 min): VX024902.D\data.ms (-1) (

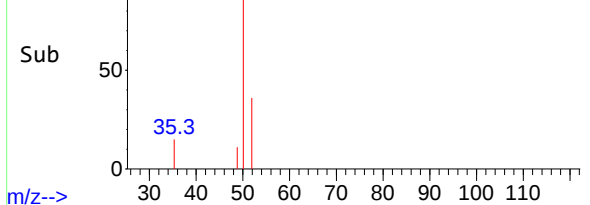

m/z-->

#3
Chloromethane
Concen: 0.211 ug/L
RT: 1.294 min Scan# 34
Delta R.T. 0.006 min
Lab File: VX024902.D
Acq: 23 Oct 2021 17:48

Tgt Ion: 50 Resp: 626
Ion Ratio Lower Upper
50 100
52 36.1 25.5 47.3

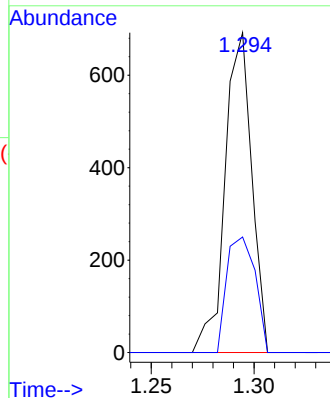

Instrument :
MSVOA_X
ClientSampleId :
P013-TW001-03