

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX102321\
 Data File : VX024903.D
 Acq On : 23 Oct 2021 18:12
 Operator : JC/MD
 Sample : M4303-11
 Misc : 25.0mL/MSVOA_X/WATER
 ALS Vial : 18 Sample Multiplier: 1

Instrument :
 MSVOA_X
 ClientSampleId :
 P014-TW001-02

Quant Time: Oct 25 02:35:13 2021
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXTR102221WMA.M
 Quant Title : TRACE VOA SFAM1.0
 QLast Update : Mon Oct 25 02:31:08 2021
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) 1,4-Difluorobenzene	6.769	114	80651	5.000	ug/L	0.00
28) Chlorobenzene-d5	10.055	117	76130	5.000	ug/L	0.00
58) 1,4-Dichlorobenzene-d4	12.024	152	34285	5.000	ug/L	0.00
System Monitoring Compounds						
4) Vinyl Chloride-d3	1.367	65	11076	4.678	ug/L	0.00
Spiked Amount	5.000	Range	40 - 130	Recovery	=	93.600%
7) Chloroethane-d5	1.672	69	11037	5.174	ug/L	0.00
Spiked Amount	5.000	Range	65 - 130	Recovery	=	103.400%
11) 1,1-Dichloroethene-d2	2.312	63	29613	3.355	ug/L	0.00
Spiked Amount	5.000	Range	60 - 125	Recovery	=	67.200%
20) 2-Butanone-d5	4.476	46	47829	55.251	ug/L	0.00
Spiked Amount	50.000	Range	40 - 130	Recovery	=	110.500%
24) Chloroform-d	5.068	84	54570	4.787	ug/L	0.00
Spiked Amount	5.000	Range	70 - 125	Recovery	=	95.800%
26) 1,2-Dichloroethane-d4	5.964	65	29149	4.679	ug/L	0.00
Spiked Amount	5.000	Range	70 - 130	Recovery	=	93.600%
32) Benzene-d6	5.982	84	85162	4.801	ug/L	0.00
Spiked Amount	5.000	Range	70 - 125	Recovery	=	96.000%
36) 1,2-Dichloropropane-d6	7.317	67	27140	4.796	ug/L	0.00
Spiked Amount	5.000	Range	60 - 140	Recovery	=	96.000%
41) Toluene-d8	8.653	98	79745	4.484	ug/L	0.00
Spiked Amount	5.000	Range	70 - 130	Recovery	=	89.600%
43) trans-1,3-Dichloroprop...	8.957	79	10542	4.058	ug/L	0.00
Spiked Amount	5.000	Range	55 - 130	Recovery	=	81.200%
46) 2-Hexanone-d5	9.390	63	45801	48.993	ug/L	0.00
Spiked Amount	50.000	Range	45 - 130	Recovery	=	97.980%
56) 1,1,2,2-Tetrachloroeth...	11.195	84	20524	4.745	ug/L	0.00
Spiked Amount	5.000	Range	65 - 120	Recovery	=	94.800%
66) 1,2-Dichlorobenzene-d4	12.323	152	27583	4.774	ug/L	0.00
Spiked Amount	5.000	Range	80 - 120	Recovery	=	95.400%
Target Compounds						Qvalue
3) Chloromethane	1.288	50	1323	0.409	ug/L	87

(#) = qualifier out of range (m) = manual integration (+) = signals summed




Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX102321\
Data File : VX024903.D
Acq On : 23 Oct 2021 18:12
Operator : JC/MD
Sample : M4303-11
Misc : 25.0mL/MSVOA_X/WATER
ALS Vial : 18 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
P014-TW001-02

Quant Time: Oct 25 02:35:13 2021
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXTR102221WMA.M
Quant Title : TRACE VOA SFAM1.0
QLast Update : Mon Oct 25 02:31:08 2021
Response via : Initial Calibration

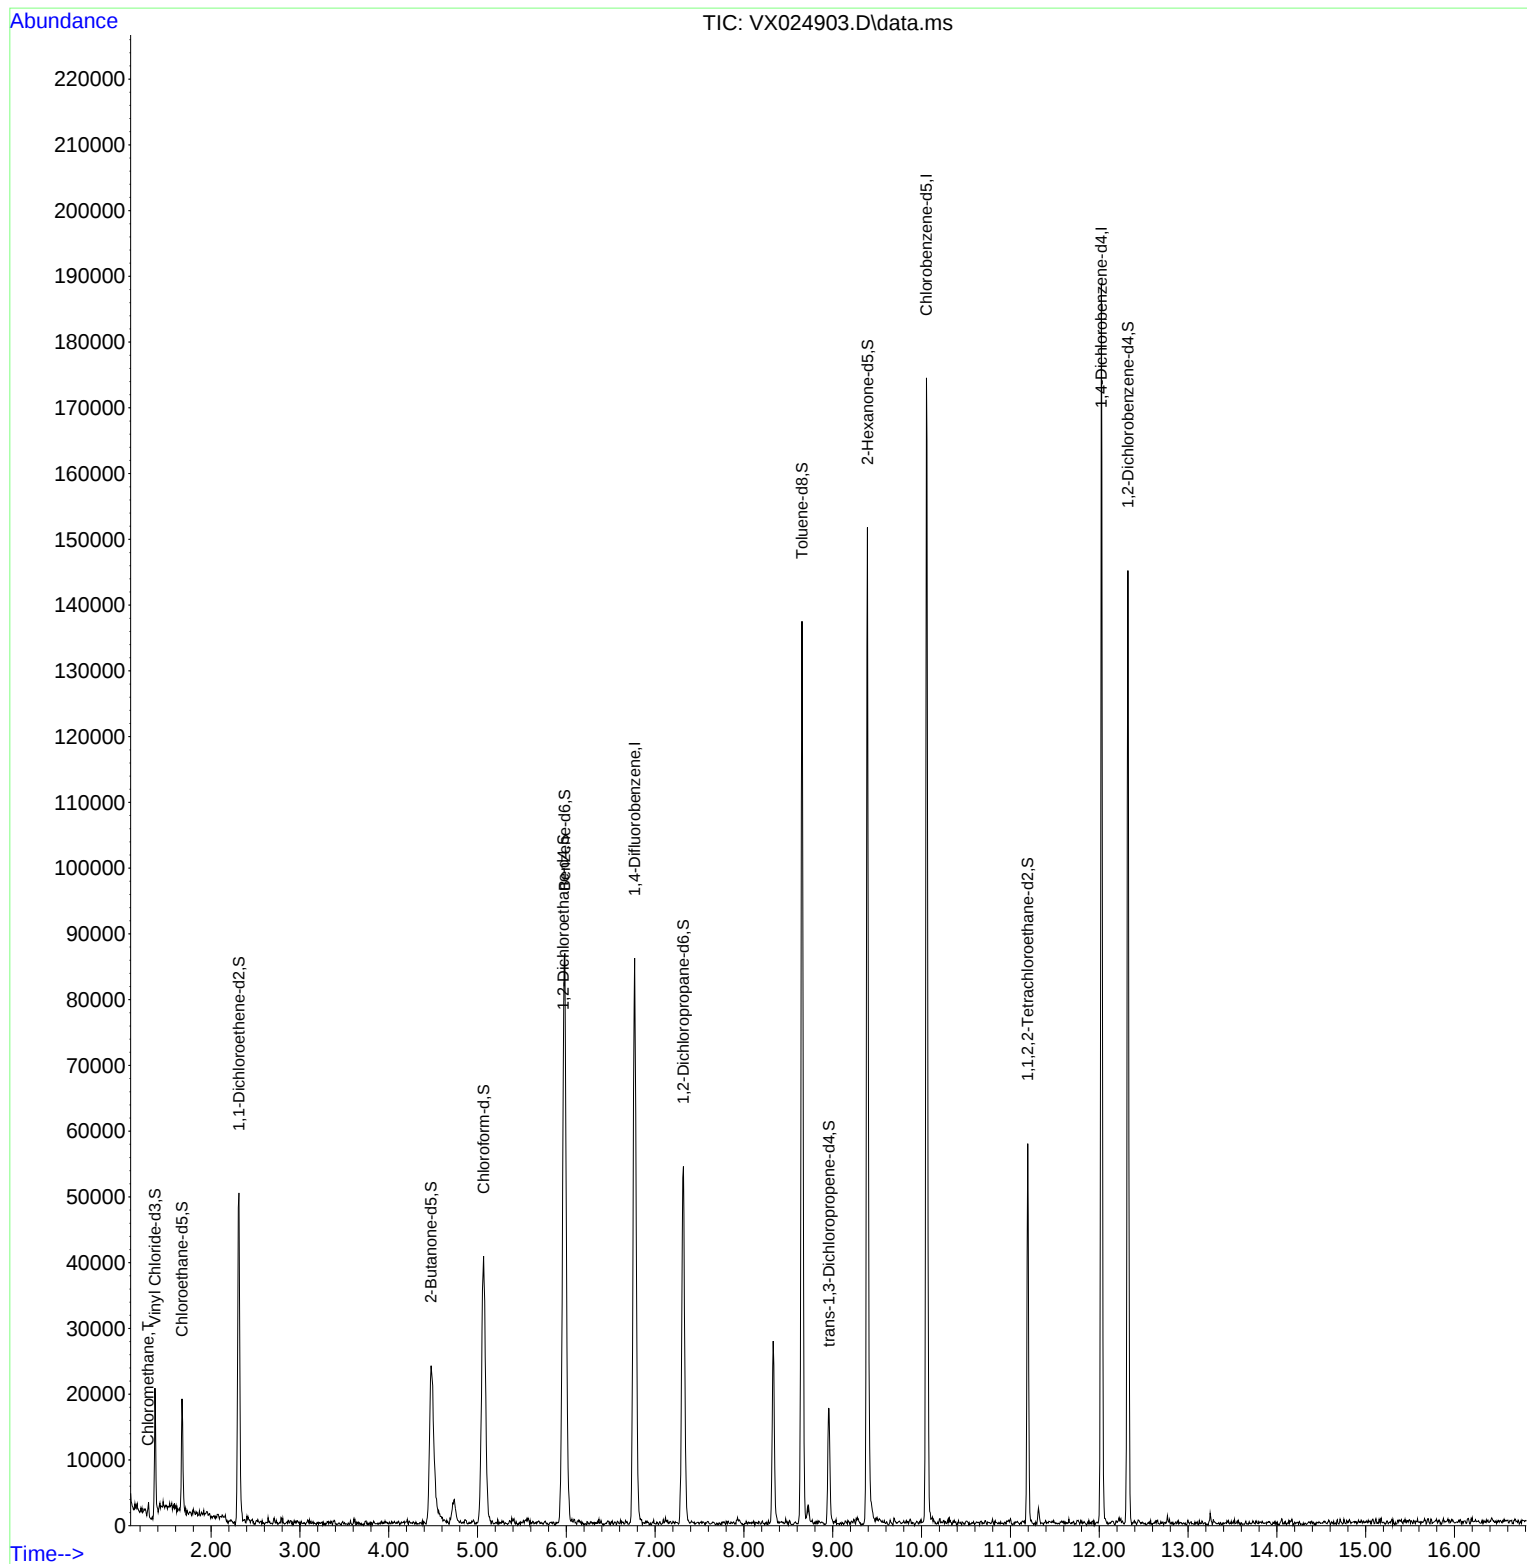


Abundance Scan 33 (1.288 min): VX024887.D\data.ms (-28)

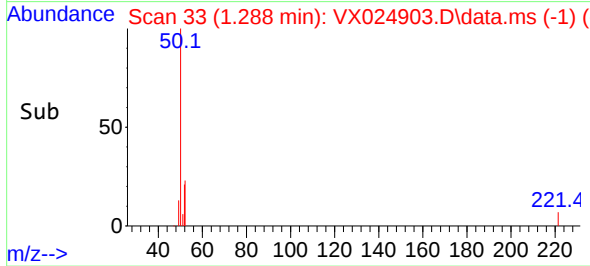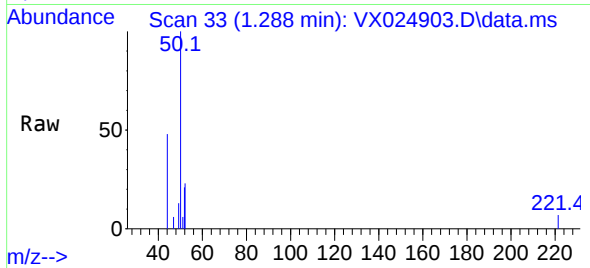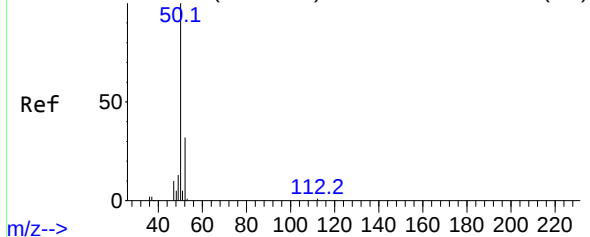

#3
Chloromethane
Concen: 0.409 ug/L
RT: 1.288 min Scan# 33
Delta R.T. -0.000 min
Lab File: VX024903.D
Acq: 23 Oct 2021 18:12

Tgt Ion: 50 Resp: 1323
Ion Ratio Lower Upper
50 100
52 44.1 25.5 47.3

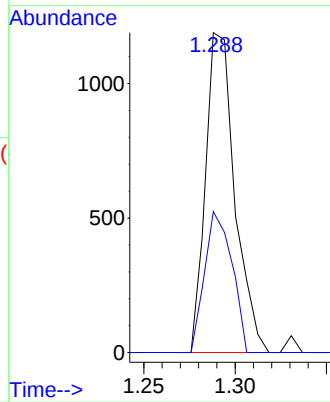

Instrument :
MSVOA_X
ClientSampleId :
P014-TW001-02