

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX102321\
 Data File : VX024910.D
 Acq On : 23 Oct 2021 20:59
 Operator : JC/MD
 Sample : M4303-18
 Misc : 25.0mL/MSVOA_X/WATER
 ALS Vial : 25 Sample Multiplier: 1

Instrument :
 MSVOA_X
 ClientSampleId :
 P034-TW001-01

Quant Time: Oct 25 02:36:36 2021
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXTR102221WMA.M
 Quant Title : TRACE VOA SFAM1.0
 QLast Update : Mon Oct 25 02:31:08 2021
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) 1,4-Difluorobenzene	6.769	114	80477	5.000	ug/L	0.00
28) Chlorobenzene-d5	10.055	117	73675	5.000	ug/L	0.00
58) 1,4-Dichlorobenzene-d4	12.024	152	34251	5.000	ug/L	0.00
System Monitoring Compounds						
4) Vinyl Chloride-d3	1.368	65	8860	3.750	ug/L	0.00
Spiked Amount	5.000	Range	40 - 130	Recovery	=	75.000%
7) Chloroethane-d5	1.672	69	9481	4.454	ug/L	0.00
Spiked Amount	5.000	Range	65 - 130	Recovery	=	89.000%
11) 1,1-Dichloroethene-d2	2.306	63	24785	2.814	ug/L	0.00
Spiked Amount	5.000	Range	60 - 125	Recovery	=	56.200%#
20) 2-Butanone-d5	4.477	46	41590	48.148	ug/L	0.00
Spiked Amount	50.000	Range	40 - 130	Recovery	=	96.300%
24) Chloroform-d	5.062	84	48045	4.224	ug/L	0.00
Spiked Amount	5.000	Range	70 - 125	Recovery	=	84.400%
26) 1,2-Dichloroethane-d4	5.964	65	25495	4.101	ug/L	0.00
Spiked Amount	5.000	Range	70 - 130	Recovery	=	82.000%
32) Benzene-d6	5.983	84	73928	4.307	ug/L	0.00
Spiked Amount	5.000	Range	70 - 125	Recovery	=	86.200%
36) 1,2-Dichloropropane-d6	7.318	67	24130	4.406	ug/L	0.00
Spiked Amount	5.000	Range	60 - 140	Recovery	=	88.200%
41) Toluene-d8	8.653	98	68515	3.981	ug/L	0.00
Spiked Amount	5.000	Range	70 - 130	Recovery	=	79.600%
43) trans-1,3-Dichloroprop...	8.952	79	8715	3.467	ug/L	0.00
Spiked Amount	5.000	Range	55 - 130	Recovery	=	69.400%
46) 2-Hexanone-d5	9.391	63	38441	42.490	ug/L	0.00
Spiked Amount	50.000	Range	45 - 130	Recovery	=	84.980%
56) 1,1,2,2-Tetrachloroeth...	11.195	84	17951	4.288	ug/L	0.00
Spiked Amount	5.000	Range	65 - 120	Recovery	=	85.800%
66) 1,2-Dichlorobenzene-d4	12.323	152	24414	4.230	ug/L	0.00
Spiked Amount	5.000	Range	80 - 120	Recovery	=	84.600%
Target Compounds					Qvalue	
13) Acetone	2.404	43	1564	2.414	ug/L	83


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX102321\
Data File : VX024910.D
Acq On : 23 Oct 2021 20:59
Operator : JC/MD
Sample : M4303-18
Misc : 25.0mL/MSVOA_X/WATER
ALS Vial : 25 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
P034-TW001-01


Quant Time: Oct 25 02:36:36 2021
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXTR102221WMA.M
Quant Title : TRACE VOA SFAM1.0
QLast Update : Mon Oct 25 02:31:08 2021
Response via : Initial Calibration

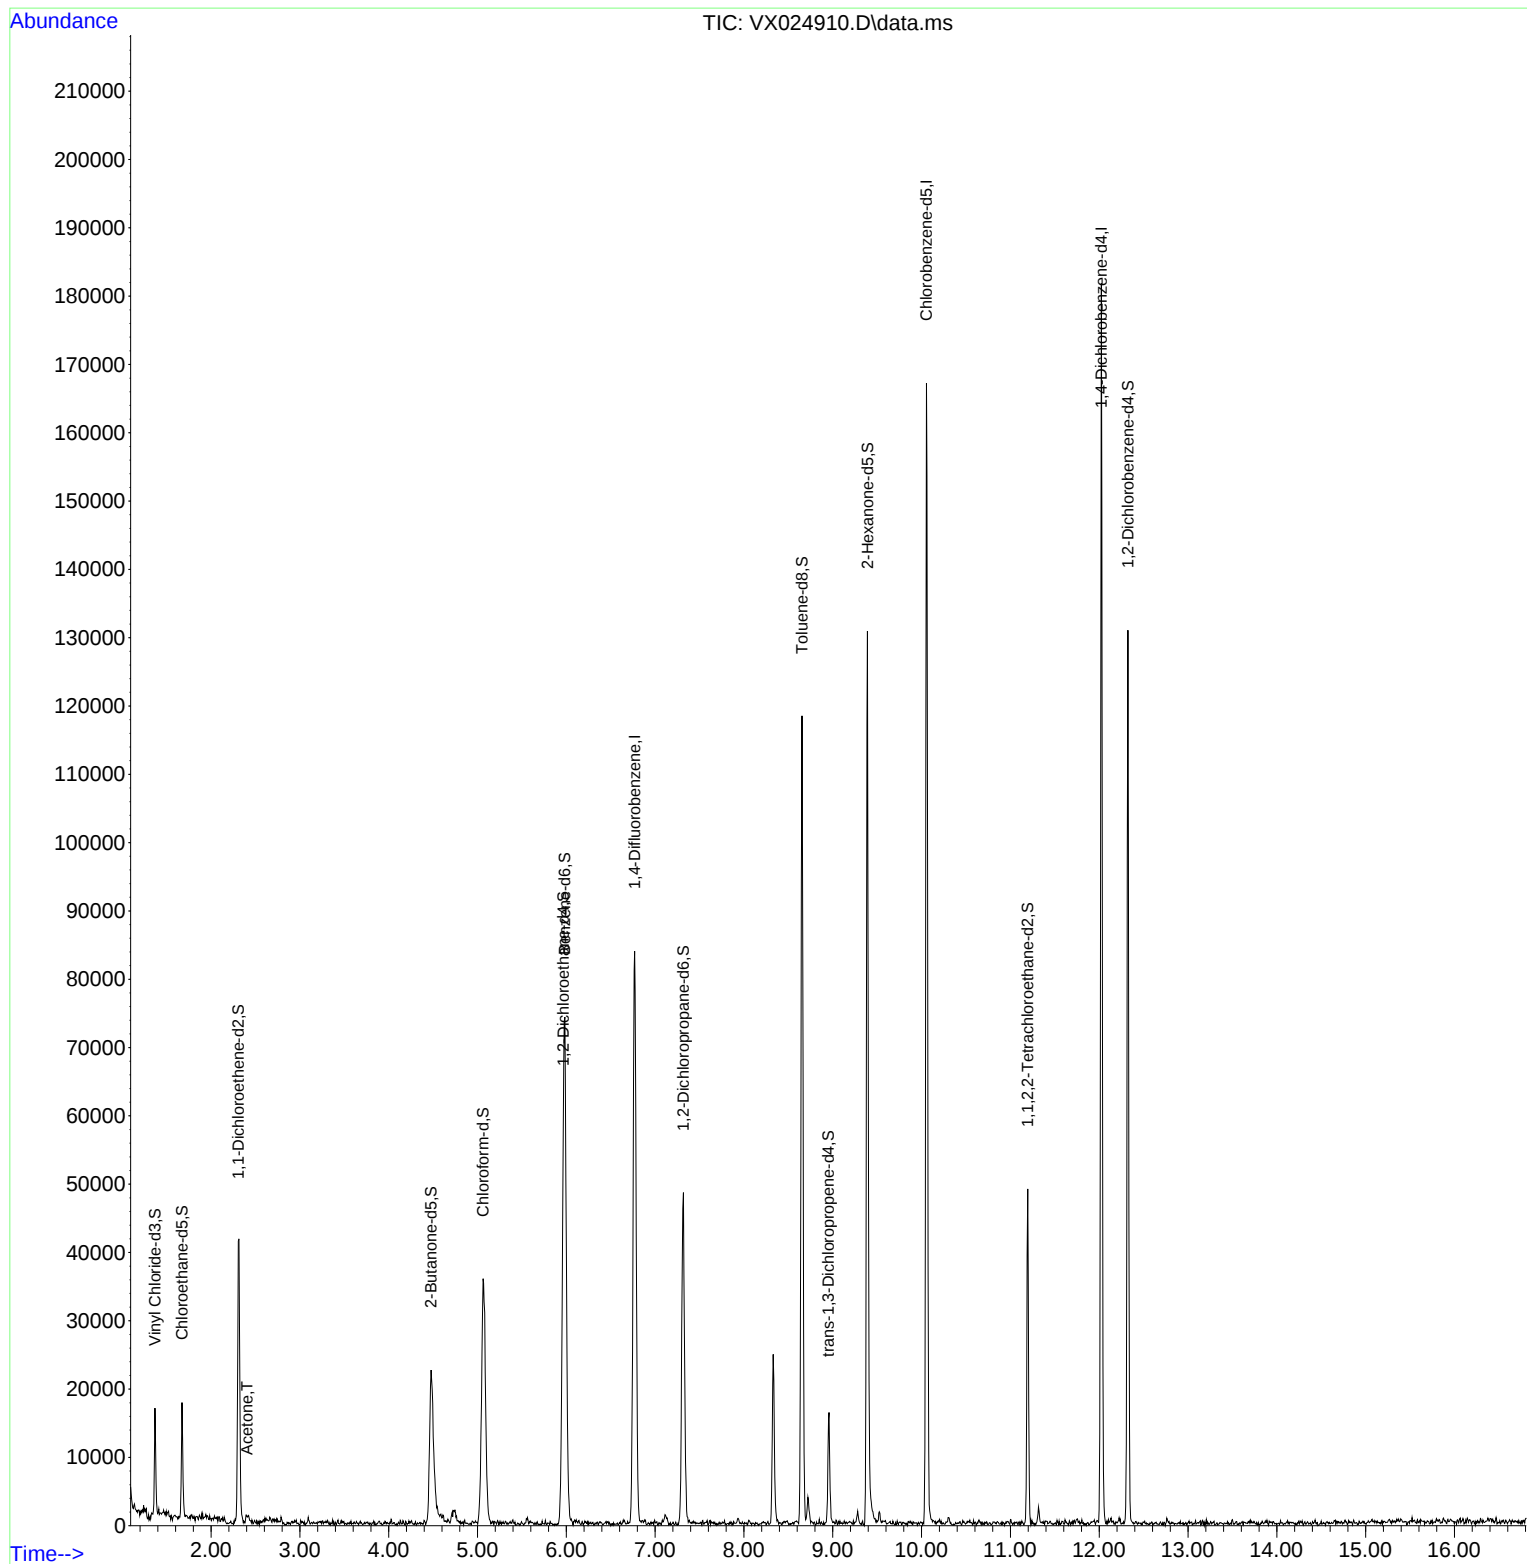

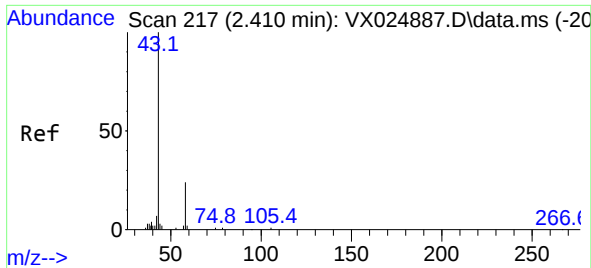

#13
Acetone
Concen: 2.414 ug/L
RT: 2.404 min Scan# 216
Delta R.T. -0.006 min
Lab File: VX024910.D
Acq: 23 Oct 2021 20:59

Instrument :
MSVOA_X
ClientSampleId :
P034-TW001-01

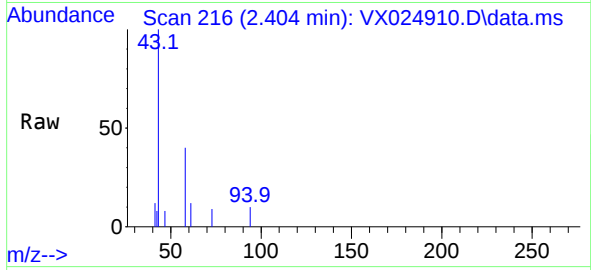

Tgt Ion: 43 Resp: 1564
Ion Ratio Lower Upper
43 100
58 22.8 0.0 64.2

