

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX102321\
 Data File : VX024893.D
 Acq On : 23 Oct 2021 14:14
 Operator : JC/MD
 Sample : M4291-23
 Misc : 25.0mL/MSVOA_X/WATER
 ALS Vial : 8 Sample Multiplier: 1

Instrument :
 MSVOA_X
 ClientSampleId :
 P050-TW001-01

Integration Parameters: rteint.p

Integrator: RTE

Smoothing : ON

Filtering: 5

Sampling : 1

Min Area: 3 % of largest Peak

Start Thrs: 0.1

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXTR102221WMA.M

Title : TRACE VOA SFAM1.0

Signal : TIC: VX024893.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.307	31	36	40	rBV2	3504	7427	2.80%	0.343%
2	1.368	43	46	53	rVB	23949	25197	9.49%	1.164%
3	1.502	64	68	75	rVB	10426	11952	4.50%	0.552%
4	1.672	92	96	105	rVB	20566	25672	9.67%	1.186%
5	2.313	191	201	209	rBV	50331	82068	30.92%	3.792%
6	2.794	272	280	285	rVB4	3787	9181	3.46%	0.424%
7	4.483	546	557	565	rBV2	27163	91496	34.47%	4.228%
8	4.599	567	576	589	rVB	15870	60711	22.87%	2.805%
9	5.062	641	652	663	rBV3	42622	131927	49.70%	6.096%
10	5.977	791	802	816	rBV2	89719	265451	100.00%	12.266%
11	6.769	922	932	943	rBV	73370	173542	65.38%	8.019%
12	7.318	1012	1022	1033	rVB2	58996	132549	49.93%	6.125%
13	8.330	1182	1188	1197	rVB2	28303	47869	18.03%	2.212%
14	8.653	1230	1241	1250	rBV	130596	202732	76.37%	9.368%
15	8.726	1250	1253	1259	rVB5	2629	4191	1.58%	0.194%
16	8.958	1285	1291	1298	rBV	19121	30695	11.56%	1.418%
17	9.391	1356	1362	1376	rBV	168842	244548	92.13%	11.300%
18	10.055	1462	1471	1480	rBV	137993	193146	72.76%	8.925%
19	11.195	1653	1658	1665	rVB	61852	77932	29.36%	3.601%
20	12.024	1789	1794	1800	rBV	135747	171058	64.44%	7.904%
21	12.323	1837	1843	1852	rVB	133483	174761	65.84%	8.075%


Sum of corrected areas: 2164105

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX102321\
Data File : VX024893.D
Acq On : 23 Oct 2021 14:14
Operator : JC/MD
Sample : M4291-23
Misc : 25.0mL/MSVOA_X/WATER
ALS Vial : 8 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
P050-TW001-01

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXTR102221WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

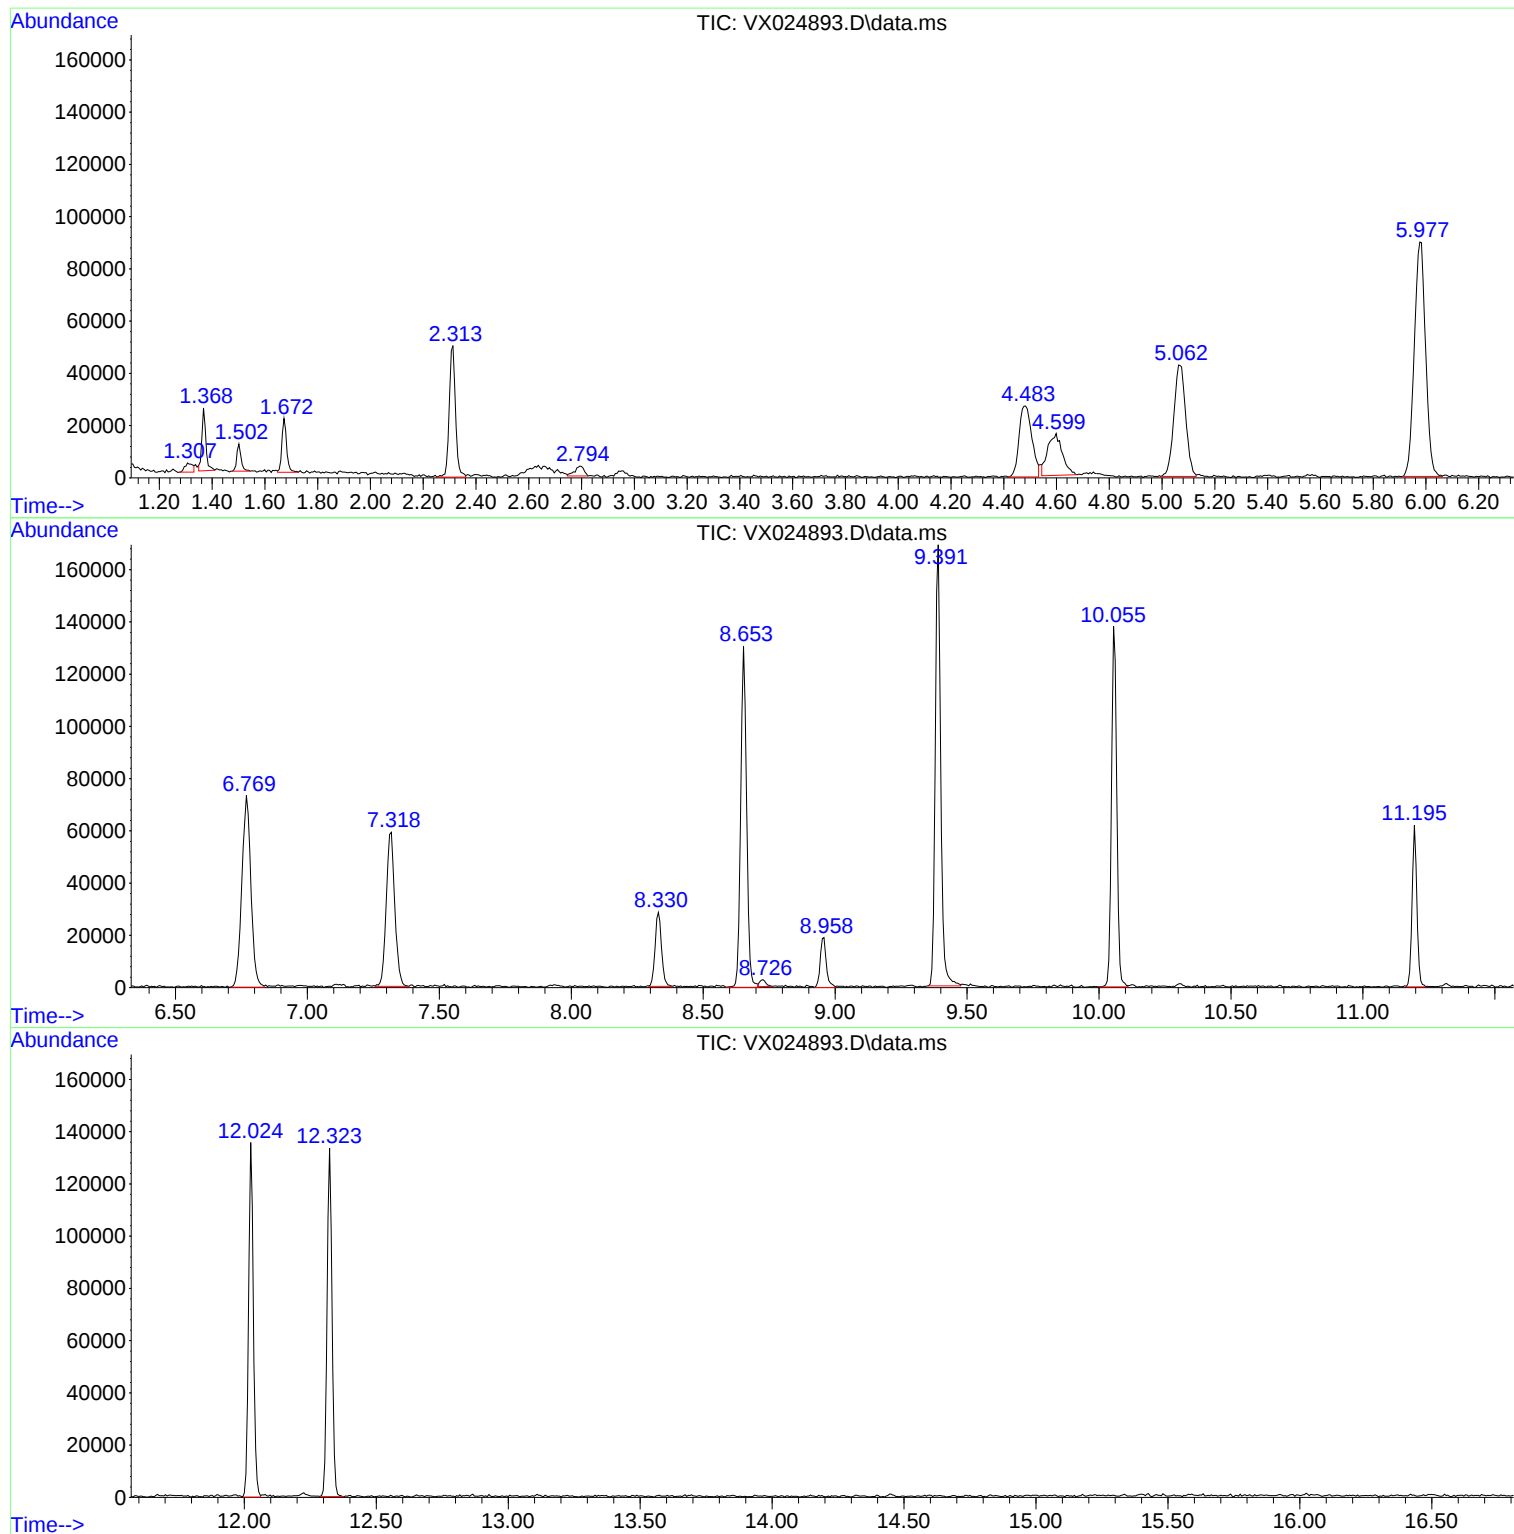

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX102321\
Data File : VX024893.D
Acq On : 23 Oct 2021 14:14
Operator : JC/MD
Sample : M4291-23
Misc : 25.0mL/MSVOA_X/WATER
ALS Vial : 8 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
P050-TW001-01

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXTR102221WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX102321\
Data File : VX024893.D
Acq On : 23 Oct 2021 14:14
Operator : JC/MD
Sample : M4291-23
Misc : 25.0mL/MSVOA_X/WATER
ALS Vial : 8 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
P050-TW001-01

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXTR102221WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST0.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc
