

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX102321\
 Data File : VX024895.D
 Acq On : 23 Oct 2021 15:01
 Operator : JC/MD
 Sample : M4303-01
 Misc : 25.0mL/MSVOA_X/WATER
 ALS Vial : 10 Sample Multiplier: 1

Instrument :
 MSVOA_X
 ClientSampleId :
 P003-TW001-02

Integration Parameters: rteint.p

Integrator: RTE

Smoothing : ON

Filtering: 5

Sampling : 1

Min Area: 3 % of largest Peak

Start Thrs: 0.1

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXTR102221WMA.M
 Title : TRACE VOA SFAM1.0

Signal : TIC: VX024895.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.367	43	46	51	rVB	20172	20131	7.78%	0.893%
2	1.672	93	96	104	rVB	19564	24212	9.36%	1.074%
3	2.312	195	201	208	rBV	50799	83163	32.16%	3.691%
4	4.477	547	556	567	rBV	26237	85424	33.03%	3.791%
5	4.574	567	572	573	rVV	3093	5088	1.97%	0.226%
6	4.593	573	575	580	rVB2	3521	4727	1.83%	0.210%
7	4.733	587	598	607	rBV2	6679	17850	6.90%	0.792%
8	5.068	641	653	666	rBV3	41320	128495	49.68%	5.702%
9	5.976	791	802	815	rBV3	88917	258626	100.00%	11.477%
10	6.769	923	932	942	rBV	89127	211972	81.96%	9.407%
11	7.318	1013	1022	1033	rBV	54912	123714	47.84%	5.490%
12	8.330	1183	1188	1199	rVB2	30229	50670	19.59%	2.249%
13	8.653	1234	1241	1248	rBV	139524	219894	85.02%	9.758%
14	8.726	1250	1253	1260	rVB	2703	4861	1.88%	0.216%
15	8.951	1284	1290	1296	rBV2	18405	28968	11.20%	1.286%
16	9.390	1356	1362	1372	rBV	151744	219122	84.73%	9.724%
17	10.055	1465	1471	1479	rBV	176619	252734	97.72%	11.216%
18	11.195	1651	1658	1663	rBV	56869	72378	27.99%	3.212%
19	11.317	1675	1678	1683	rVB3	1601	2618	1.01%	0.116%
20	12.024	1789	1794	1803	rVB	196982	246903	95.47%	10.957%
21	12.323	1837	1843	1849	rBV	151979	191882	74.19%	8.515%


Sum of corrected areas: 2253432

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX102321\
Data File : VX024895.D
Acq On : 23 Oct 2021 15:01
Operator : JC/MD
Sample : M4303-01
Misc : 25.0mL/MSVOA_X/WATER
ALS Vial : 10 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
P003-TW001-02

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXTR102221WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

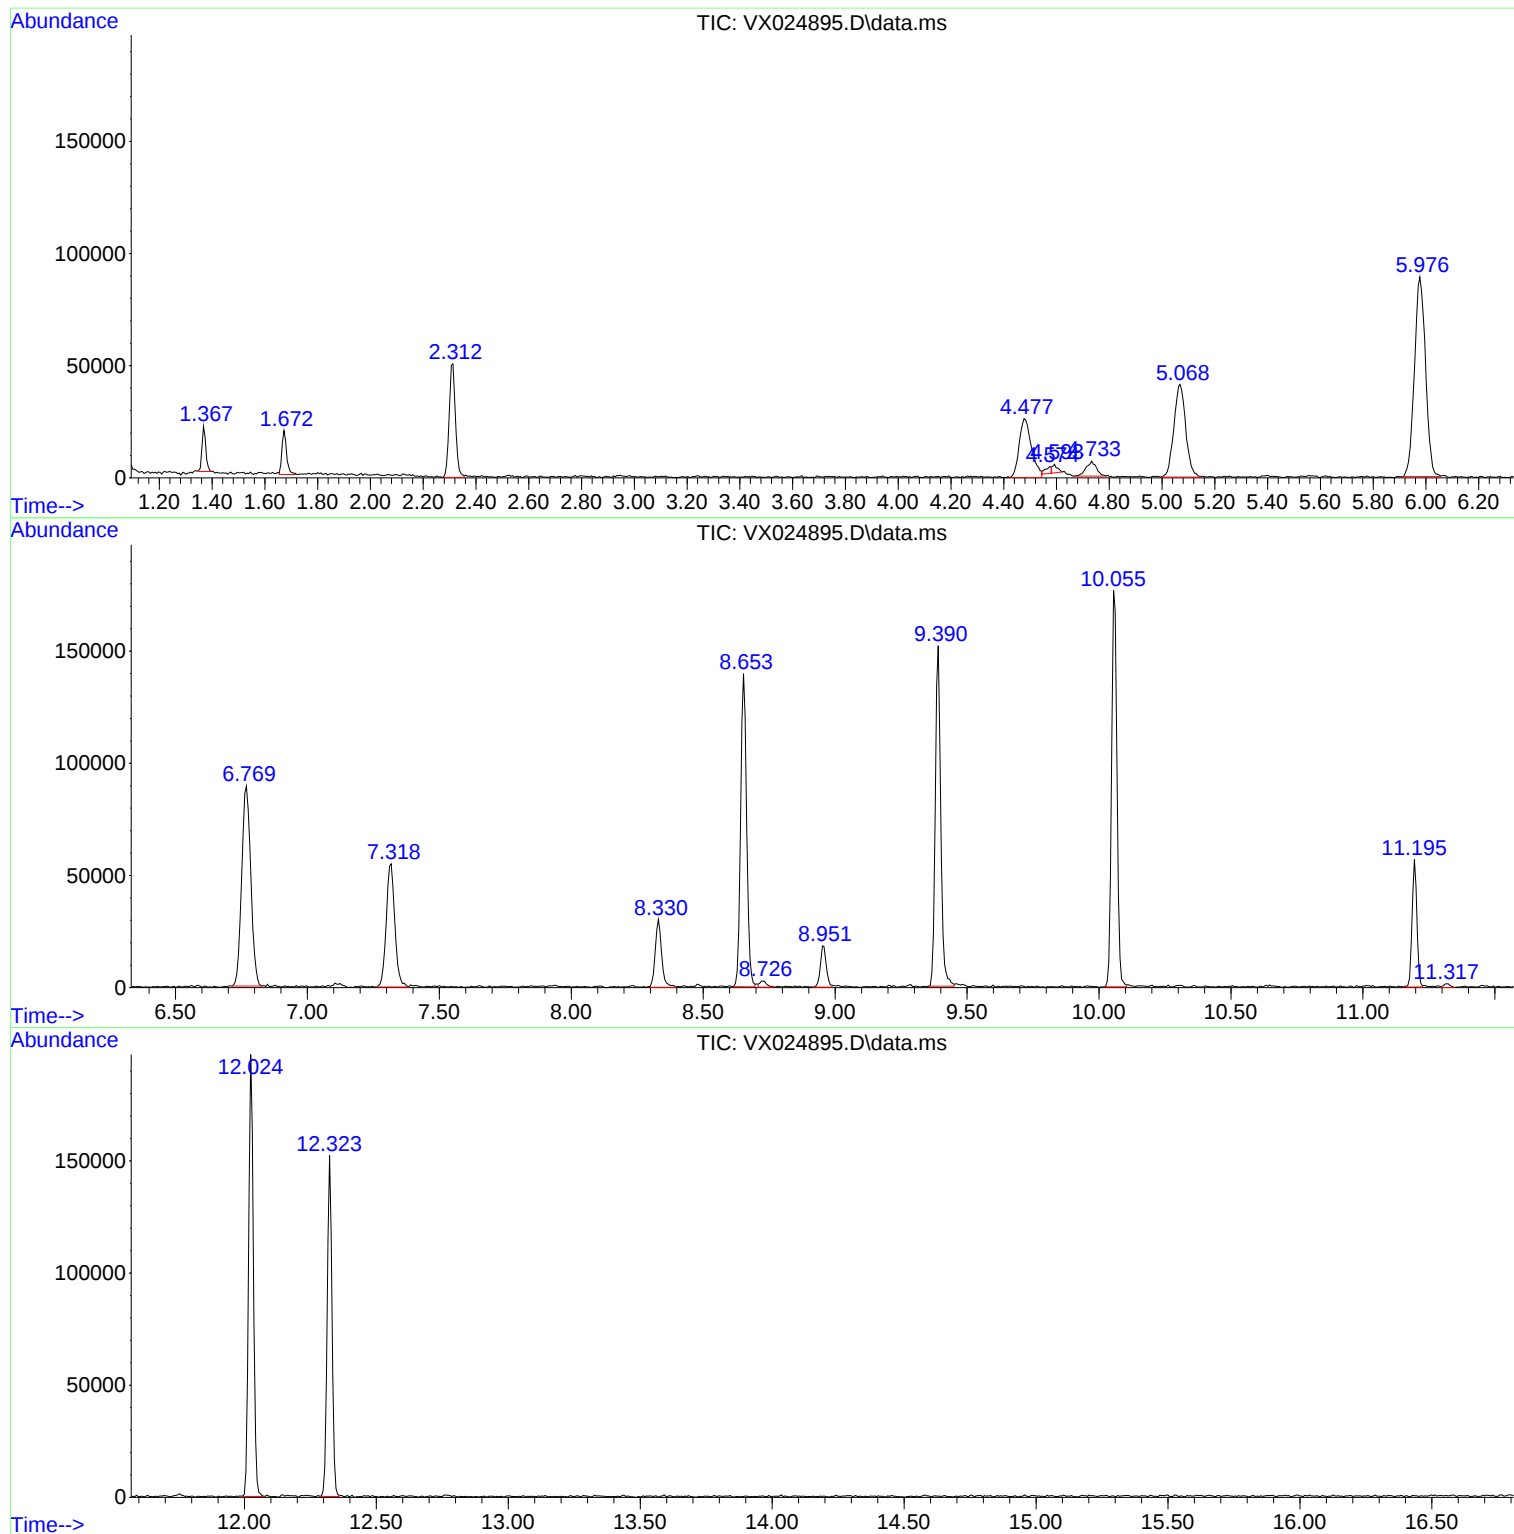

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX102321\
Data File : VX024895.D
Acq On : 23 Oct 2021 15:01
Operator : JC/MD
Sample : M4303-01
Misc : 25.0mL/MSVOA_X/WATER
ALS Vial : 10 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
P003-TW001-02

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXTR102221WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX102321\
Data File : VX024895.D
Acq On : 23 Oct 2021 15:01
Operator : JC/MD
Sample : M4303-01
Misc : 25.0mL/MSVOA_X/WATER
ALS Vial : 10 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
P003-TW001-02

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXTR102221WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	#	RT	Resp	Conc
------------------	----	---------	-------	----------	---	----	------	------