

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX102321\
 Data File : VX024897.D
 Acq On : 23 Oct 2021 15:49
 Operator : JC/MD
 Sample : M4303-03
 Misc : 25.0mL/MSVOA_X/WATER
 ALS Vial : 12 Sample Multiplier: 1

Instrument :
 MSVOA_X
 ClientSampleId :
 P005-TW001-02

Integration Parameters: rteint.p

Integrator: RTE

Smoothing : ON

Filtering: 5

Sampling : 1

Min Area: 3 % of largest Peak

Start Thrs: 0.1

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXTR102221WMA.M

Title : TRACE VOA SFAM1.0

Signal : TIC: VX024897.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.368	42	46	50	rVB	21130	20437	7.85%	0.906%
2	1.672	92	96	101	rBV	18119	22216	8.53%	0.984%
3	2.306	194	200	208	rBV	52478	83494	32.07%	3.700%
4	2.410	216	217	228	rVB3	2537	4729	1.82%	0.210%
5	4.477	548	556	570	rBV2	24432	84745	32.55%	3.755%
6	4.721	593	596	597	rBV2	2357	3082	1.18%	0.137%
7	4.733	597	598	606	rVB4	3071	4912	1.89%	0.218%
8	5.068	641	653	667	rVB2	42194	128497	49.36%	5.694%
9	5.976	791	802	818	rVB3	89943	260341	100.00%	11.536%
10	6.769	921	932	941	rBV	91503	221400	85.04%	9.810%
11	7.116	985	989	993	rVB2	2009	3092	1.19%	0.137%
12	7.312	1011	1021	1031	rBV	56050	122767	47.16%	5.440%
13	8.330	1180	1188	1195	rBV2	31170	50356	19.34%	2.231%
14	8.653	1235	1241	1248	rBV	137194	219478	84.30%	9.725%
15	8.726	1248	1253	1258	rVB2	2822	4670	1.79%	0.207%
16	8.952	1285	1290	1298	rBV	20167	30259	11.62%	1.341%
17	9.390	1355	1362	1373	rBV	149522	222662	85.53%	9.866%
18	10.055	1466	1471	1481	rBV	188410	255518	98.15%	11.322%
19	11.195	1652	1658	1664	rBV	56257	72138	27.71%	3.196%
20	12.024	1788	1794	1802	rBV	193648	248509	95.46%	11.012%
21	12.323	1834	1843	1852	rVV	148619	193506	74.33%	8.574%




Sum of corrected areas: 2256808

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX102321\
Data File : VX024897.D
Acq On : 23 Oct 2021 15:49
Operator : JC/MD
Sample : M4303-03
Misc : 25.0mL/MSVOA_X/WATER
ALS Vial : 12 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
P005-TW001-02

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXTR102221WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

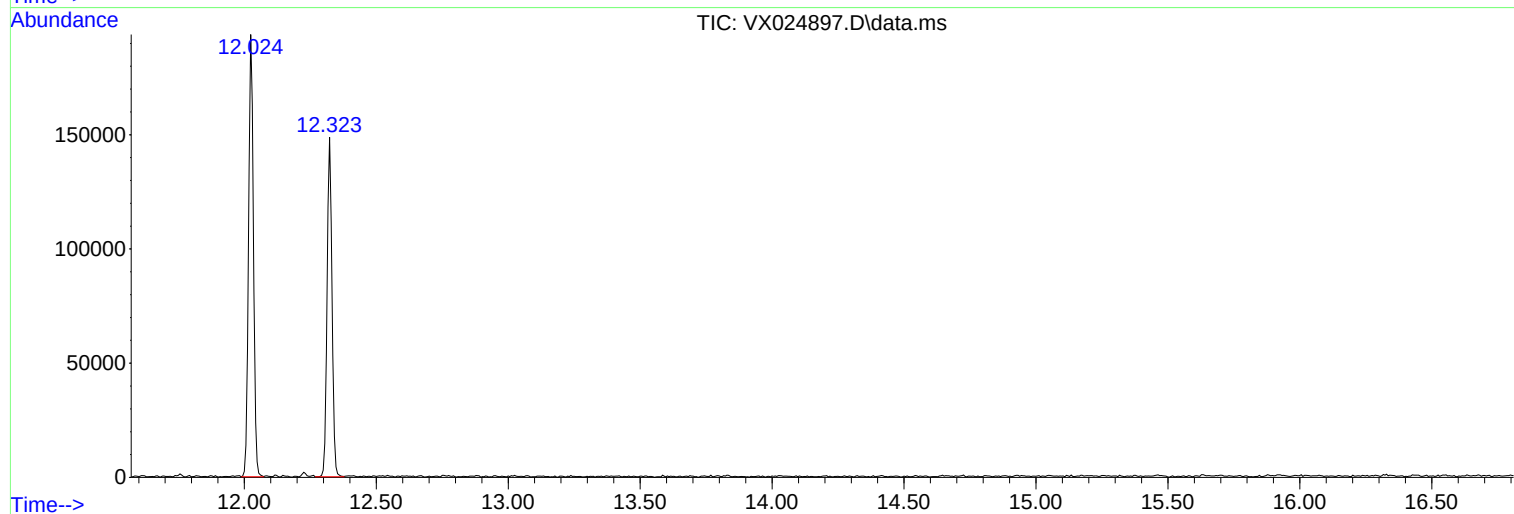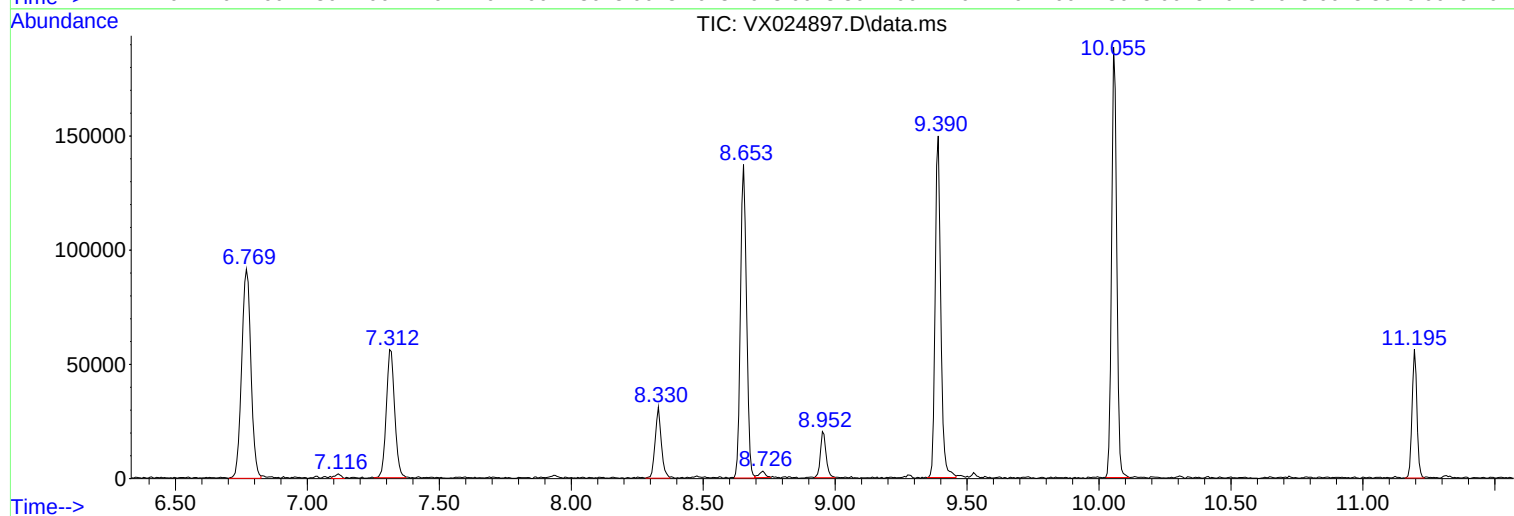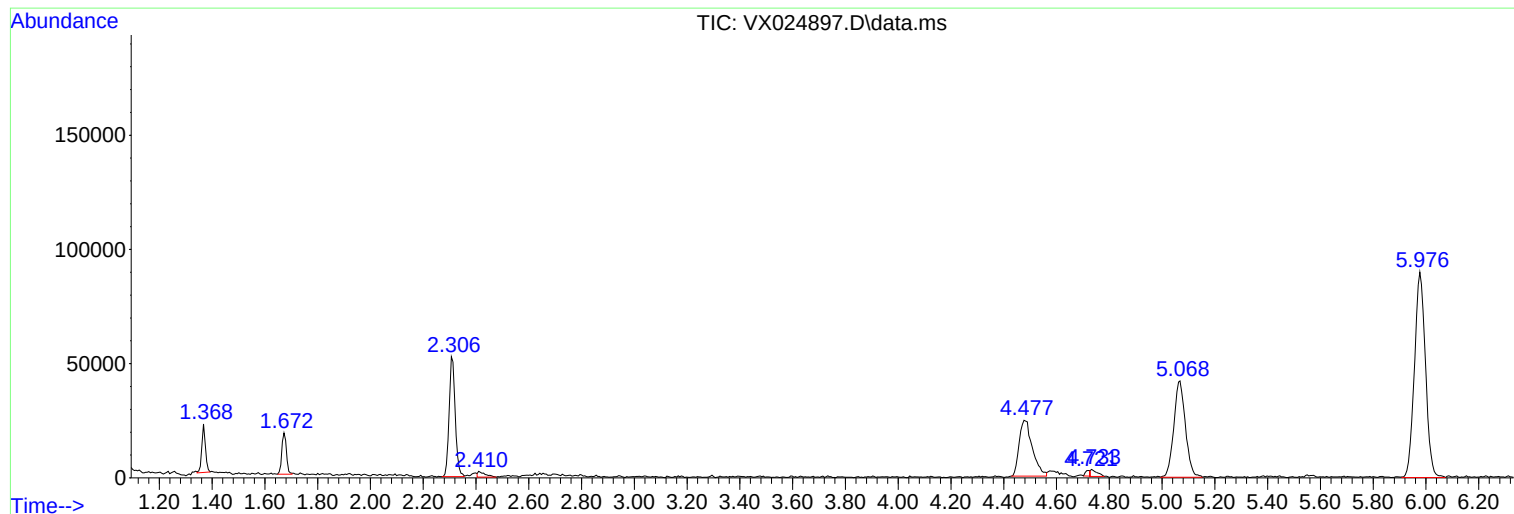

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX102321\
Data File : VX024897.D
Acq On : 23 Oct 2021 15:49
Operator : JC/MD
Sample : M4303-03
Misc : 25.0mL/MSVOA_X/WATER
ALS Vial : 12 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
P005-TW001-02

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXTR102221WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX102321\
Data File : VX024897.D
Acq On : 23 Oct 2021 15:49
Operator : JC/MD
Sample : M4303-03
Misc : 25.0mL/MSVOA_X/WATER
ALS Vial : 12 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
P005-TW001-02

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXTR102221WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc
