

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX102321\
 Data File : VX024901.D
 Acq On : 23 Oct 2021 17:24
 Operator : JC/MD
 Sample : M4303-07
 Misc : 25.0mL/MSVOA_X/WATER
 ALS Vial : 16 Sample Multiplier: 1

Instrument :
 MSVOA_X
 ClientSampleId :
 P013-TW001-02

Integration Parameters: rteint.p

Integrator: RTE

Smoothing : ON

Filtering: 5

Sampling : 1

Min Area: 3 % of largest Peak

Start Thrs: 0.1

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXTR102221WMA.M
 Title : TRACE VOA SFAM1.0

Signal : TIC: VX024901.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.288	31	33	38	rVB2	2650	3441	1.32%	0.156%
2	1.367	42	46	54	rBV	21555	21947	8.42%	0.992%
3	1.672	92	96	106	rBV	18978	23296	8.94%	1.053%
4	2.306	195	200	208	rBV	49368	81078	31.11%	3.665%
5	4.476	548	556	566	rBV	26836	82688	31.73%	3.738%
6	4.739	592	599	601	rBV2	1313	2988	1.15%	0.135%
7	5.062	641	652	666	rBV2	43307	130748	50.17%	5.911%
8	5.982	791	803	815	rBV4	87566	260635	100.00%	11.783%
9	6.769	921	932	943	rBV	87178	210749	80.86%	9.527%
10	7.317	1011	1022	1031	rBV	55151	119643	45.90%	5.409%
11	8.329	1181	1188	1195	rBV	28490	47167	18.10%	2.132%
12	8.653	1234	1241	1248	rBV	135845	217865	83.59%	9.849%
13	8.720	1249	1252	1260	rVB3	2585	4453	1.71%	0.201%
14	8.957	1286	1291	1298	rBV	19941	28483	10.93%	1.288%
15	9.390	1355	1362	1372	rBV	153203	224781	86.24%	10.162%
16	10.055	1464	1471	1480	rBV	172628	243449	93.41%	11.006%
17	11.195	1652	1658	1664	rBV	56189	72829	27.94%	3.292%
18	11.323	1672	1679	1682	rBV5	2118	3422	1.31%	0.155%
19	12.024	1787	1794	1805	rBV	184744	237831	91.25%	10.752%
20	12.323	1836	1843	1853	rBV	149080	194530	74.64%	8.794%


Sum of corrected areas: 2212023

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX102321\
Data File : VX024901.D
Acq On : 23 Oct 2021 17:24
Operator : JC/MD
Sample : M4303-07
Misc : 25.0mL/MSVOA_X/WATER
ALS Vial : 16 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
P013-TW001-02

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXTR102221WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

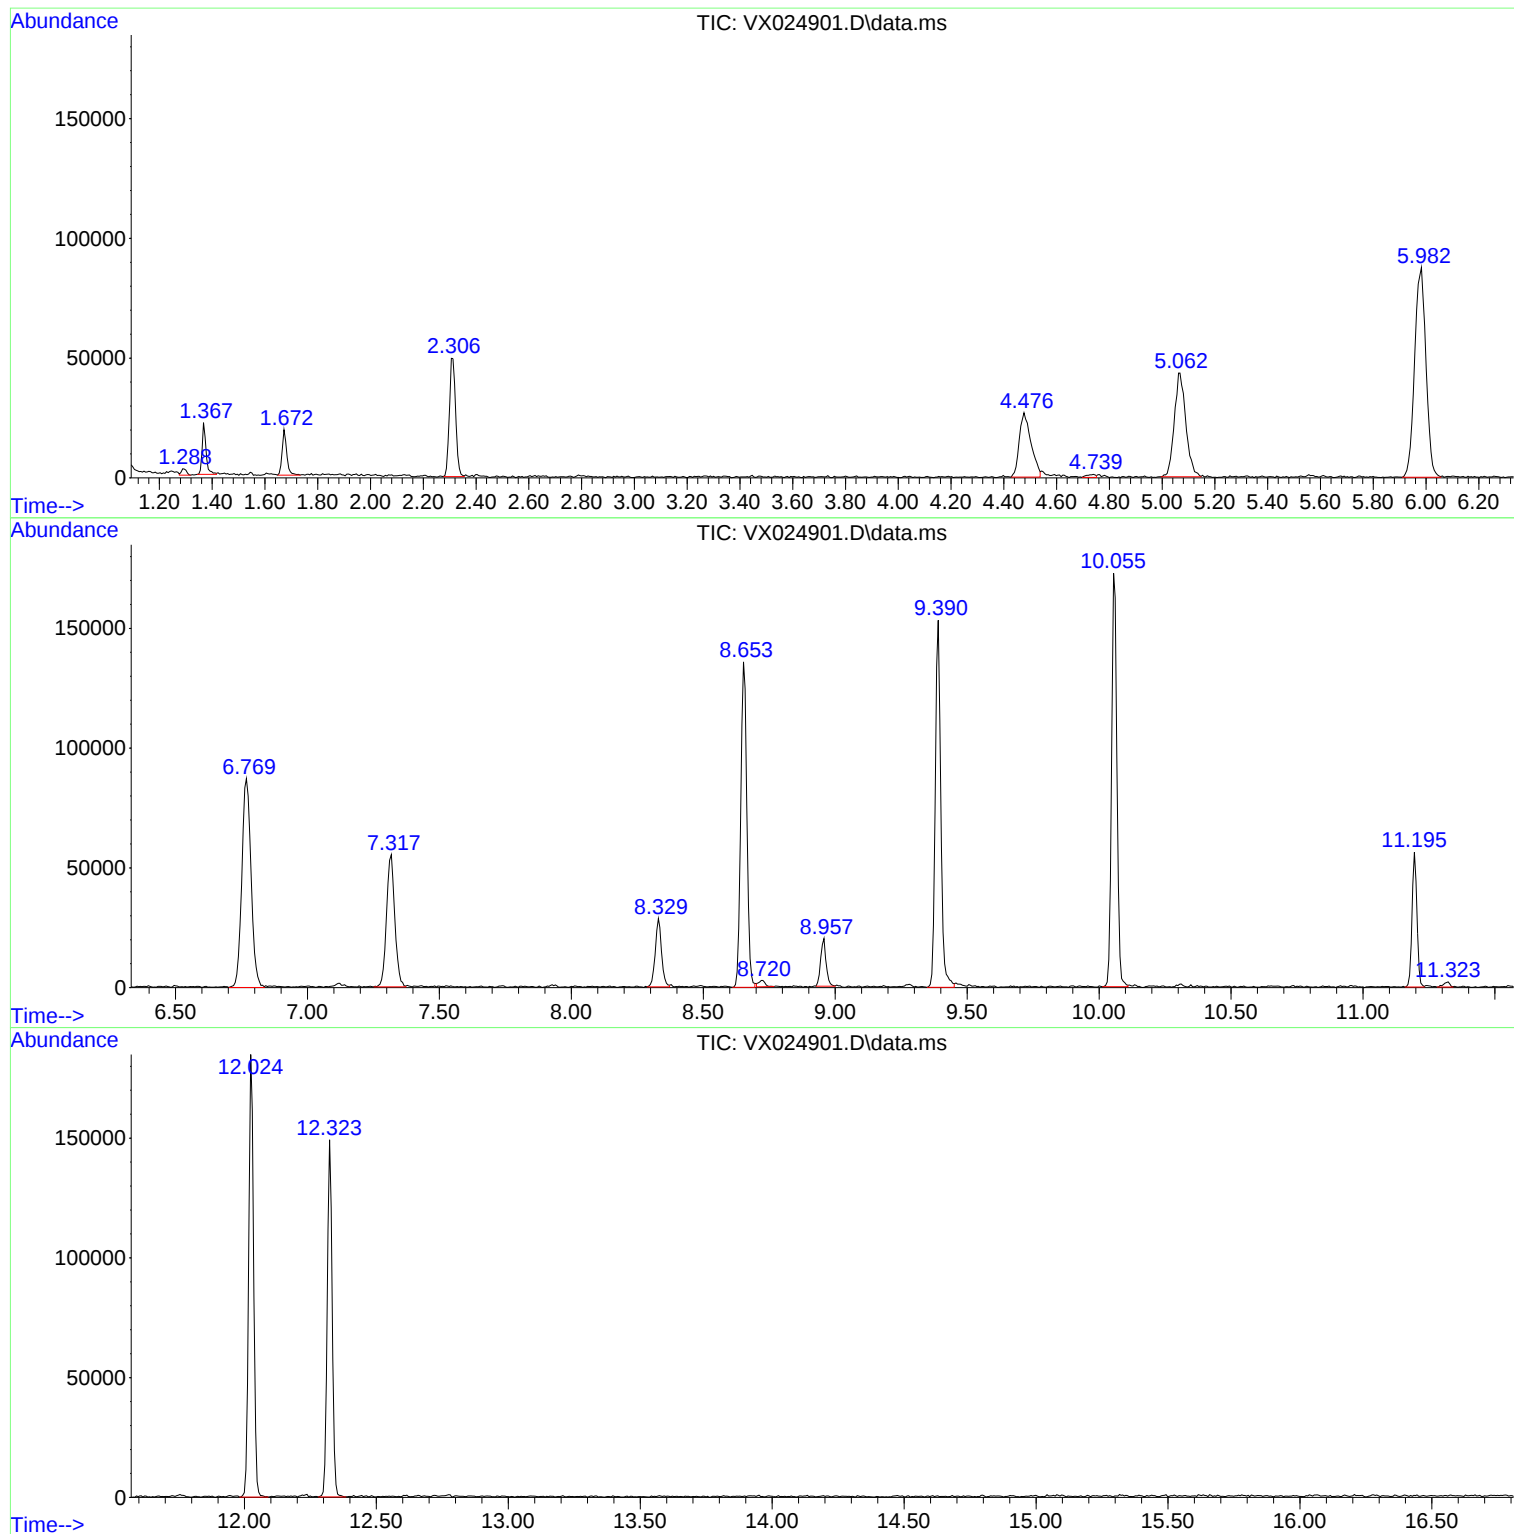

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX102321\
Data File : VX024901.D
Acq On : 23 Oct 2021 17:24
Operator : JC/MD
Sample : M4303-07
Misc : 25.0mL/MSVOA_X/WATER
ALS Vial : 16 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
P013-TW001-02

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXTR102221WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX102321\
Data File : VX024901.D
Acq On : 23 Oct 2021 17:24
Operator : JC/MD
Sample : M4303-07
Misc : 25.0mL/MSVOA_X/WATER
ALS Vial : 16 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
P013-TW001-02

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXTR102221WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc
