

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX102321\
 Data File : VX024902.D
 Acq On : 23 Oct 2021 17:48
 Operator : JC/MD
 Sample : M4303-10
 Misc : 25.0mL/MSVOA_X/WATER
 ALS Vial : 17 Sample Multiplier: 1

Instrument :
 MSVOA_X
 ClientSampleId :
 P013-TW001-03

Integration Parameters: rteint.p

Integrator: RTE

Smoothing : ON

Filtering: 5

Sampling : 1

Min Area: 3 % of largest Peak

Start Thrs: 0.1

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXTR102221WMA.M

Title : TRACE VOA SFAM1.0

Signal : TIC: VX024902.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.227	22	23	32	rVB4	1628	3057	1.25%	0.148%
2	1.368	43	46	52	rBV	20546	18566	7.57%	0.900%
3	1.672	91	96	102	rBV	17812	22015	8.98%	1.067%
4	2.313	194	201	213	rBV	47371	77380	31.57%	3.750%
5	4.483	546	557	571	rBV2	24039	83804	34.19%	4.061%
6	4.721	589	596	600	rBV4	2053	4541	1.85%	0.220%
7	5.068	642	653	666	rBV3	40378	124153	50.65%	6.017%
8	5.977	789	802	817	rBV4	83664	245124	100.00%	11.880%
9	6.769	923	932	942	rBV	79200	190121	77.56%	9.214%
10	7.110	982	988	995	rBV6	1397	2921	1.19%	0.142%
11	7.318	1013	1022	1035	rBV	51448	115226	47.01%	5.584%
12	8.330	1182	1188	1200	rVB2	27028	46374	18.92%	2.247%
13	8.488	1210	1214	1222	rVB6	1308	2775	1.13%	0.134%
14	8.653	1234	1241	1248	rBV	126429	200808	81.92%	9.732%
15	8.726	1248	1253	1259	rVB4	2443	4944	2.02%	0.240%
16	8.958	1285	1291	1299	rVB	18271	28107	11.47%	1.362%
17	9.391	1352	1362	1375	rBV	148348	215287	87.83%	10.434%
18	10.055	1466	1471	1480	rBV	153260	216735	88.42%	10.504%
19	11.195	1651	1658	1664	rVB	53709	69916	28.52%	3.388%
20	11.317	1673	1678	1681	rBV4	1859	2566	1.05%	0.124%
21	12.024	1788	1794	1804	rVB	166430	210286	85.79%	10.191%
22	12.323	1838	1843	1854	rVB	138478	178679	72.89%	8.660%


Sum of corrected areas: 2063385

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX102321\
Data File : VX024902.D
Acq On : 23 Oct 2021 17:48
Operator : JC/MD
Sample : M4303-10
Misc : 25.0mL/MSVOA_X/WATER
ALS Vial : 17 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
P013-TW001-03

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXTR102221WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

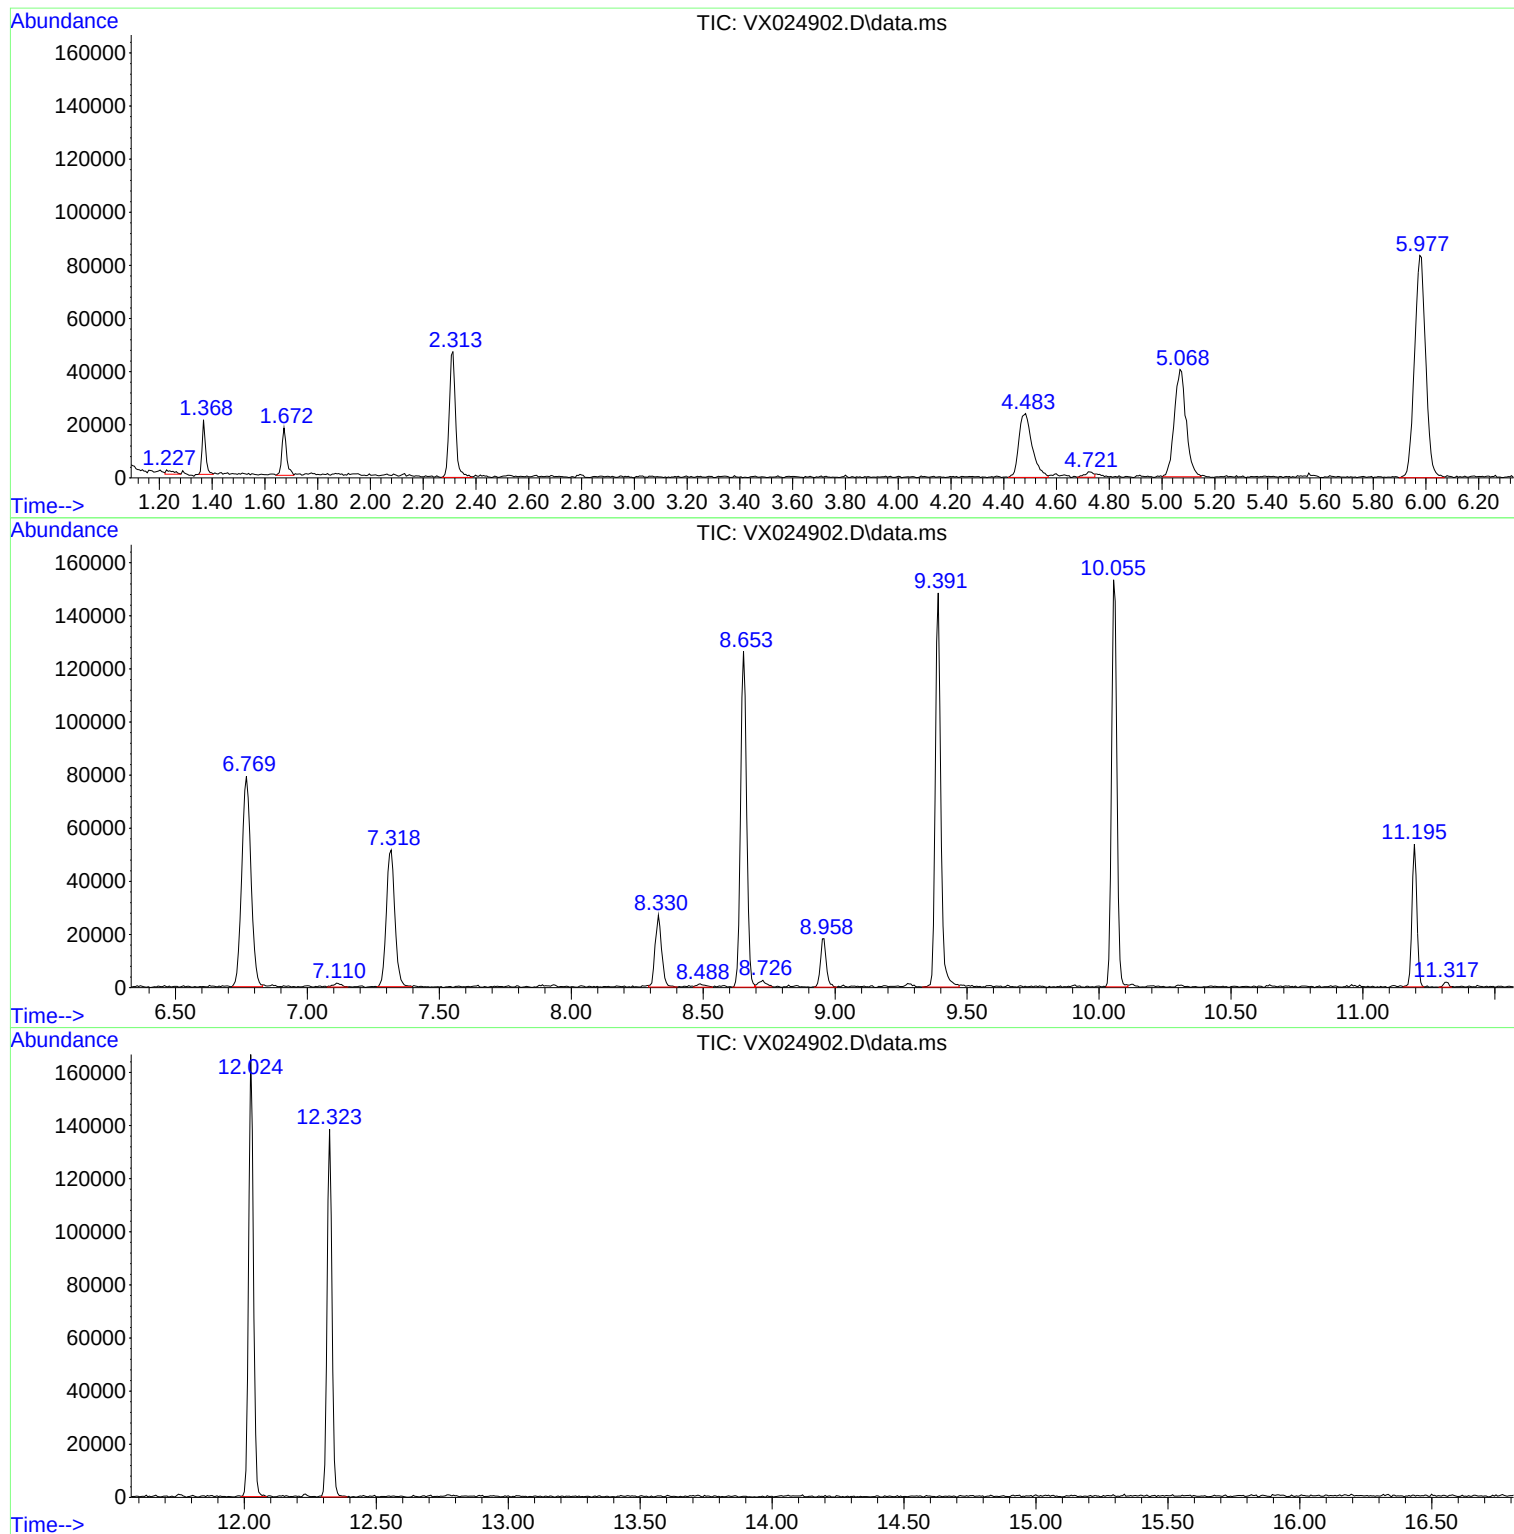

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX102321\
Data File : VX024902.D
Acq On : 23 Oct 2021 17:48
Operator : JC/MD
Sample : M4303-10
Misc : 25.0mL/MSVOA_X/WATER
ALS Vial : 17 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
P013-TW001-03

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXTR102221WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX102321\
Data File : VX024902.D
Acq On : 23 Oct 2021 17:48
Operator : JC/MD
Sample : M4303-10
Misc : 25.0mL/MSVOA_X/WATER
ALS Vial : 17 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
P013-TW001-03

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXTR102221WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST0.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc
